
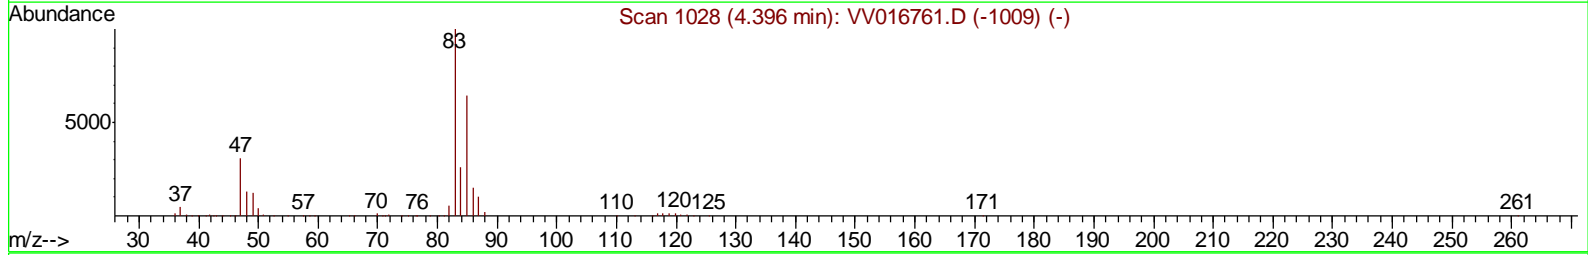
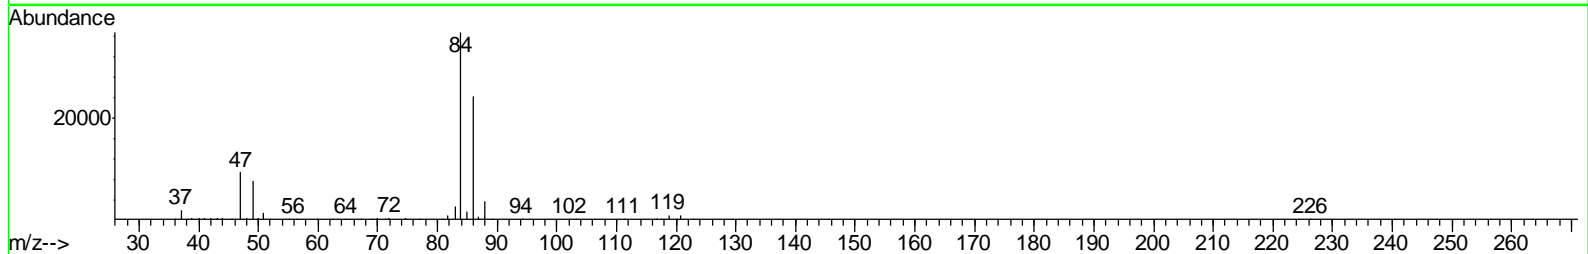


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061020\  
 Data File : VV016775.D  
 Acq On : 10 Jun 2020 17:38  
 Operator : SY/MD  
 Sample : L2914-06 20X  
 Misc : 5.0mL/MSVOA V/WATER  
 ALS Vial : 16 Sample Multiplier: 1

Quant Time: Jun 11 01:08:49 2020  
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA\_V\METHOD\SOMVLM060820WMA.M  
 Quant Title : VOC Analysis  
 QLast Update : Thu Jun 11 01:04:46 2020  
 Response via : Initial Calibration

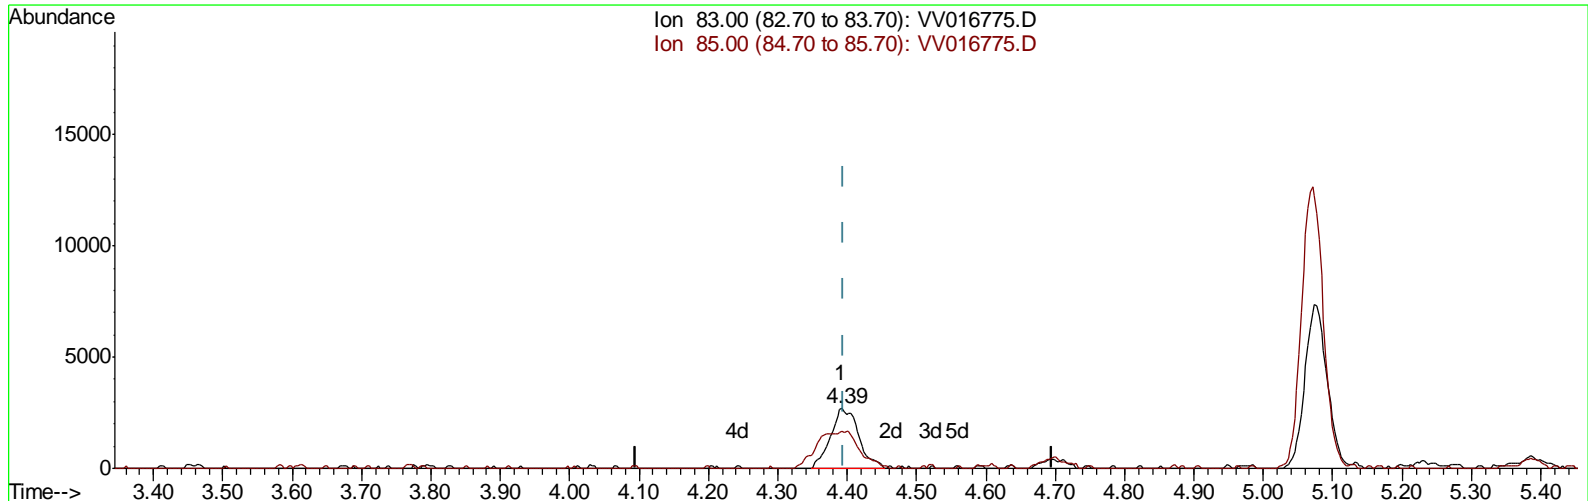

TIC: VV016775.D

(25) Chloroform (T)  
 4.392min (-0.003) 1.63ug/L m  
 response 7592

Ion	Exp%	Act%
83.00	100	100
85.00	63.00	61.95
0.00	0.00	0.00
0.00	0.00	0.00