
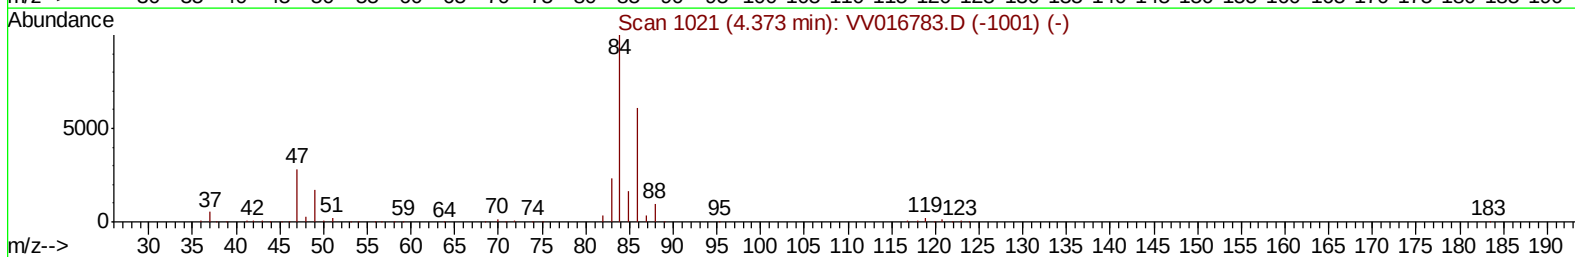
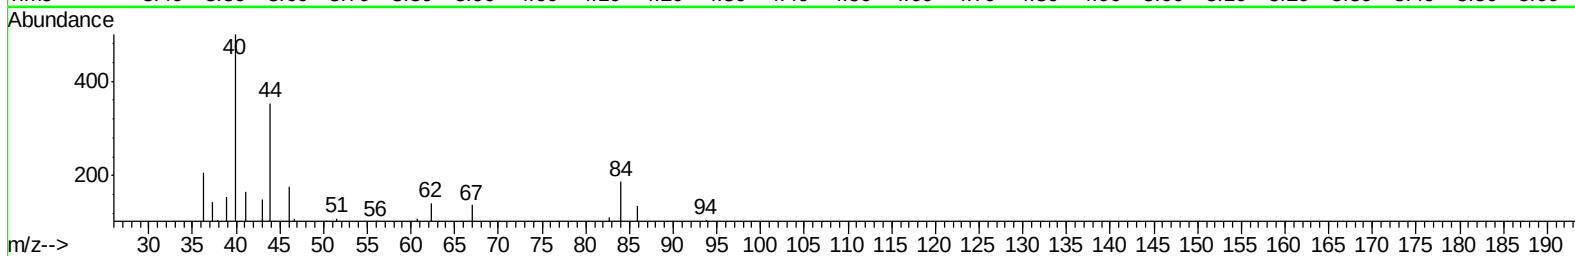


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061020\
 Data File : VV016805.D
 Acq On : 11 Jun 2020 05:56
 Operator : SY/MD
 Sample : L2901-10
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 47 Sample Multiplier: 1

Quant Time: Jun 11 06:43:12 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Jun 11 04:06:22 2020
 Response via : Initial Calibration

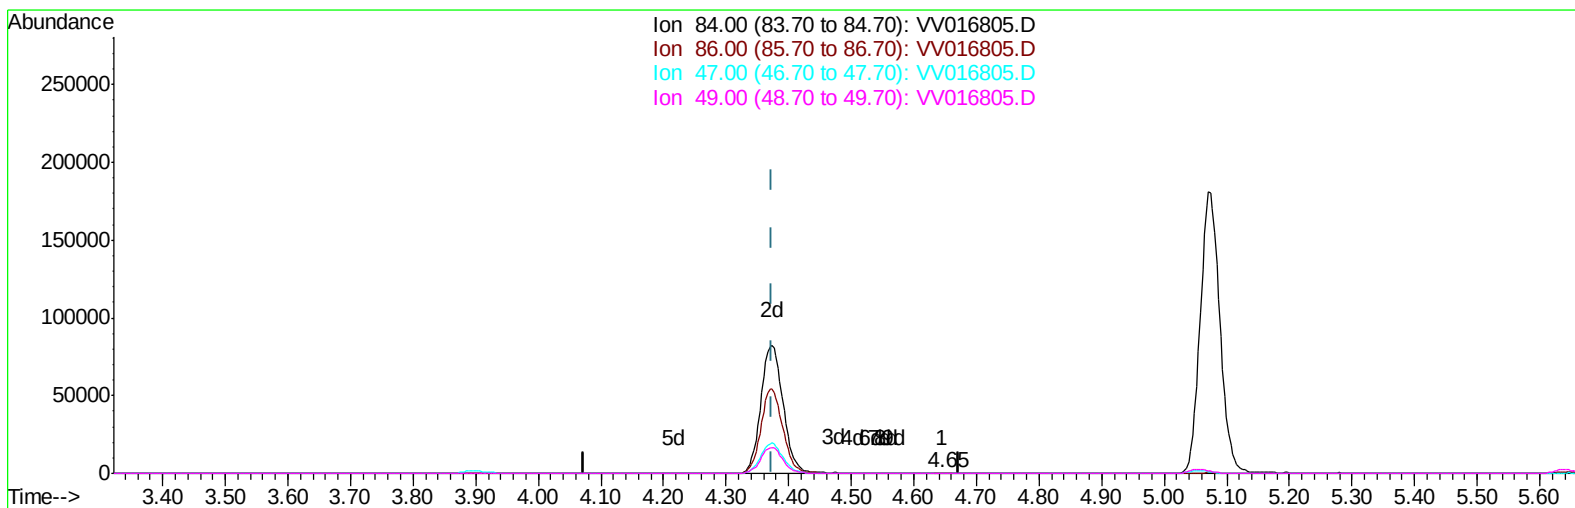

TIC: VV016805.D

(24) Chloroform-d (S)

4.647min (+0.273) 0.04ug/L

response 203

Ion	Exp%	Act%
84.00	100	100
86.00	62.80	72.91
47.00	44.50	34.48
49.00	27.40	35.47