
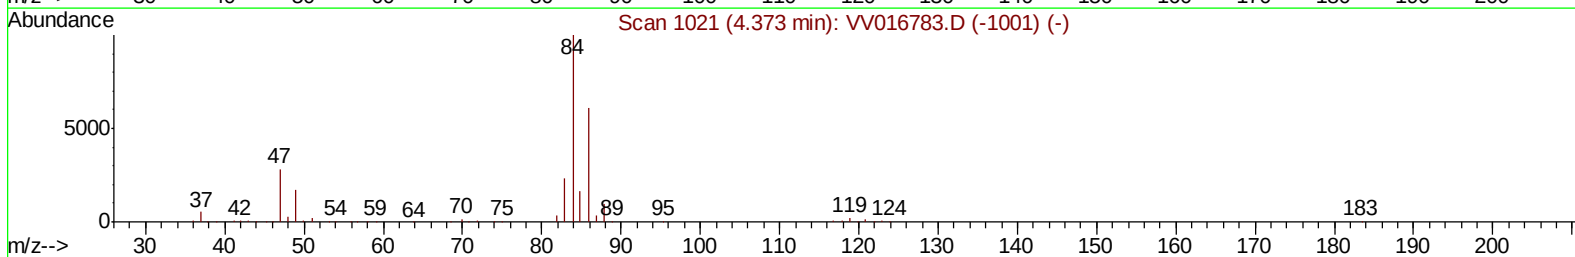
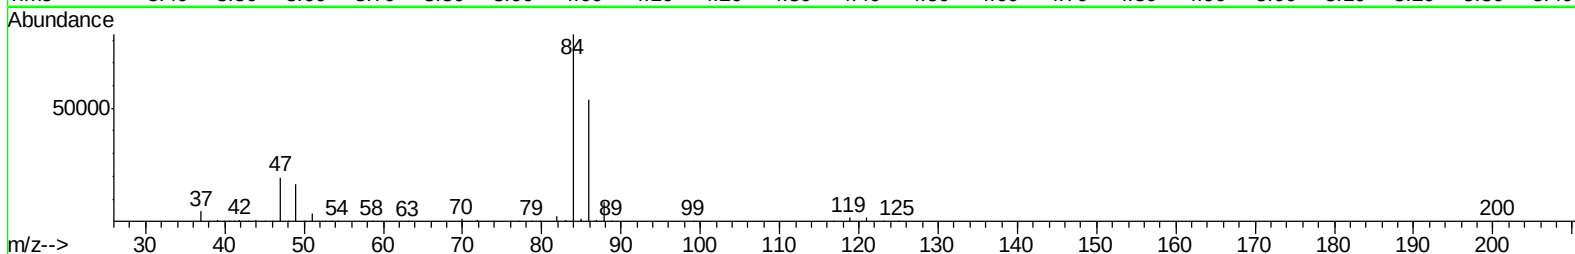


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061020\  
 Data File : VV016805.D  
 Acq On : 11 Jun 2020 05:56  
 Operator : SY/MD  
 Sample : L2901-10  
 Misc : 5.0mL/MSVOA V/WATER  
 ALS Vial : 47 Sample Multiplier: 1

Quant Time: Jun 11 06:43:12 2020  
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA\_V\METHOD\SOMVLM060820WMA.M  
 Quant Title : VOC Analysis  
 QLast Update : Thu Jun 11 04:06:22 2020  
 Response via : Initial Calibration

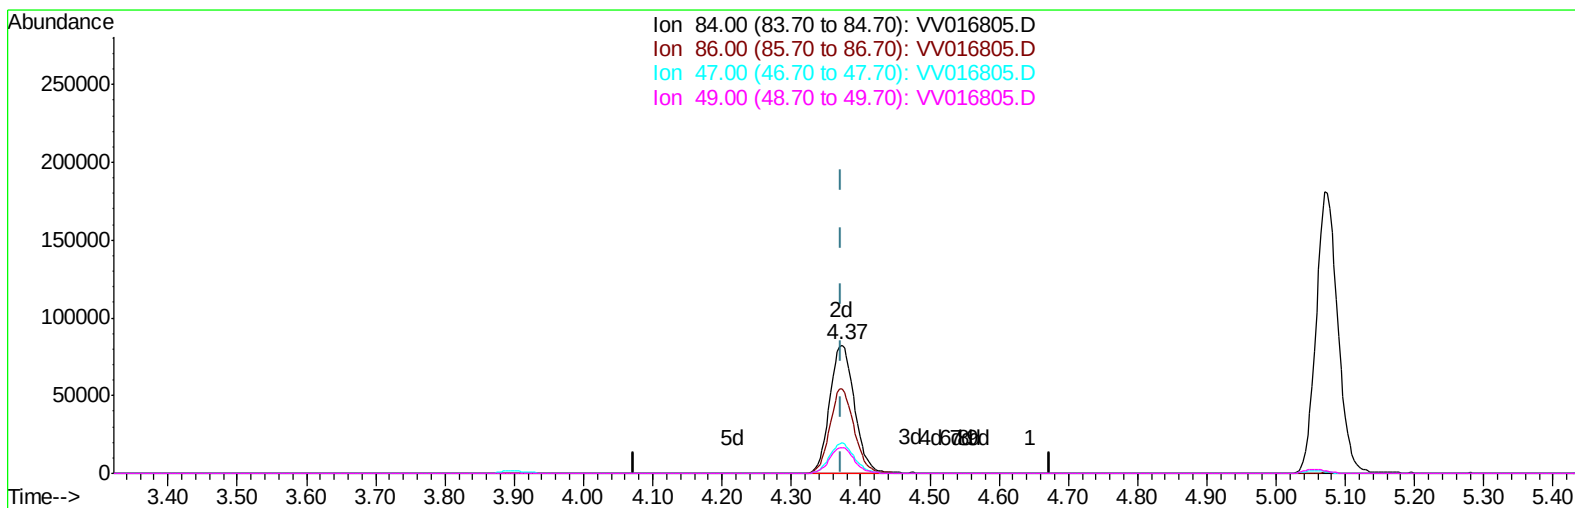

TIC: VV016805.D

(24) Chloroform-d (S)

4.373min (+0.000) 43.96ug/L m

response 203027

| Ion   | Exp%  | Act%  |
|-------|-------|-------|
| 84.00 | 100   | 100   |
| 86.00 | 62.80 | 0.07# |
| 47.00 | 44.50 | 0.03# |
| 49.00 | 27.40 | 0.04# |