


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061020\
Data File : VV016775.D
Acq On : 10 Jun 2020 17:38
Operator : SY/MD
Sample : L2914-06 20X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9E01

Manual Integrations
APPROVED

MMDadoda
6/11/2020 4:23:26 PM

Quant Time: Jun 11 02:49:20 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Jun 11 01:04:46 2020
Response via : Initial Calibration

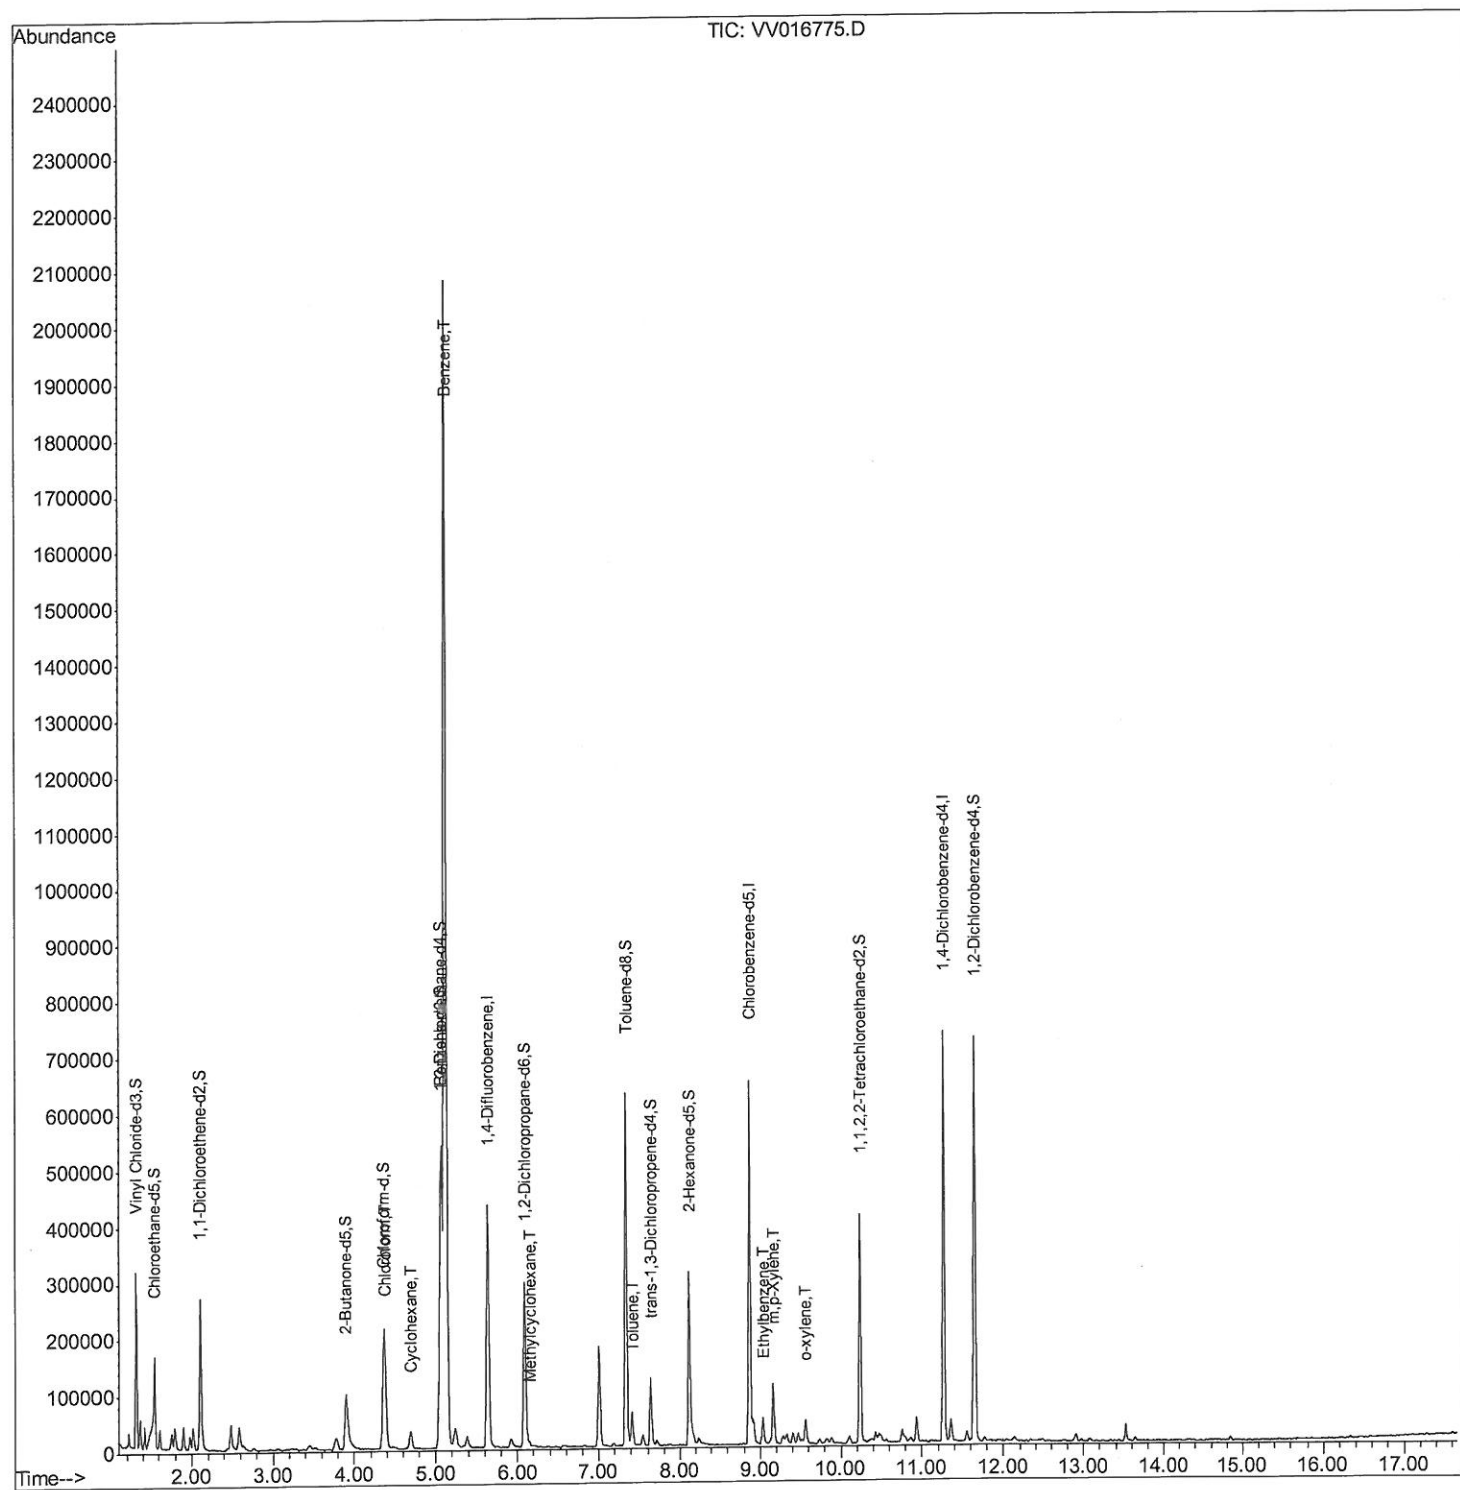

Quantitation Report (Qedit)




```
Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061020\  
Data File : VV016775.D  
Acq On : 10 Jun 2020 17:38  
Operator : SY/MD  
Sample : L2914-06 20X  
Misc : 5.0mL/MSVOA V/WATER  
ALS Vial : 16 Sample Multiplier: 1
```

Instrument :
MSVOA_V
ClientSampleId :
F9E01

Manual Integrations
APPROVED

MMDadoda
6/11/2020 4:23:26 PM

Quant Time: Jun 11 01:08:49 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Jun 11 01:04:46 2020
Response via : Initial Calibration

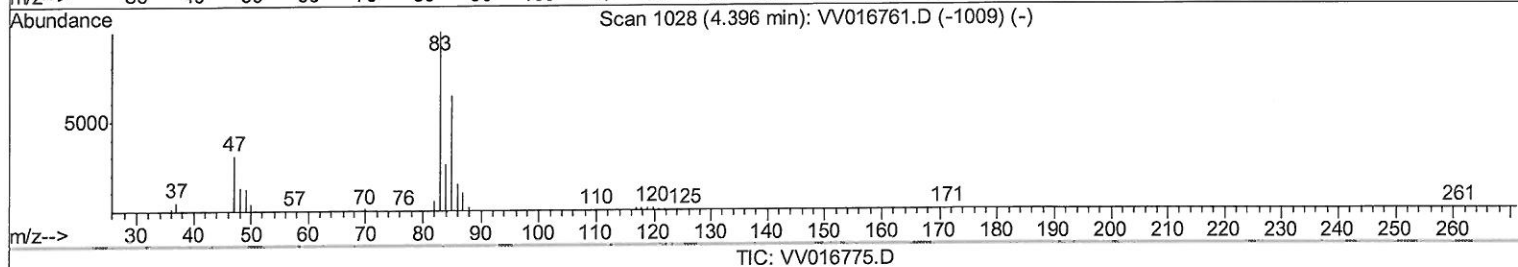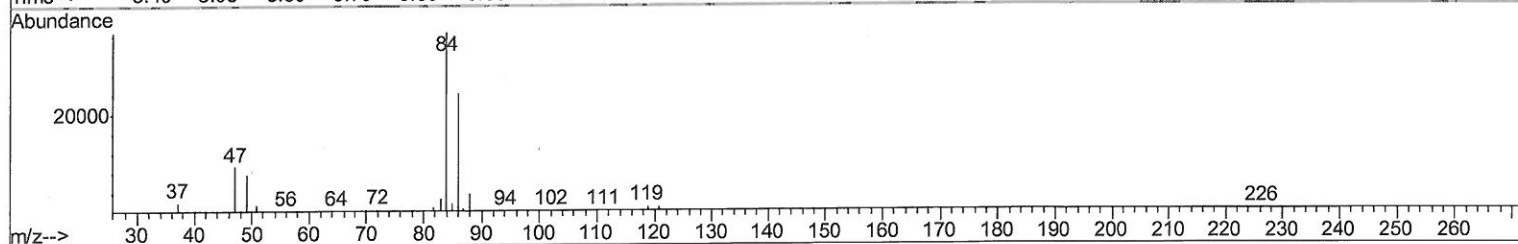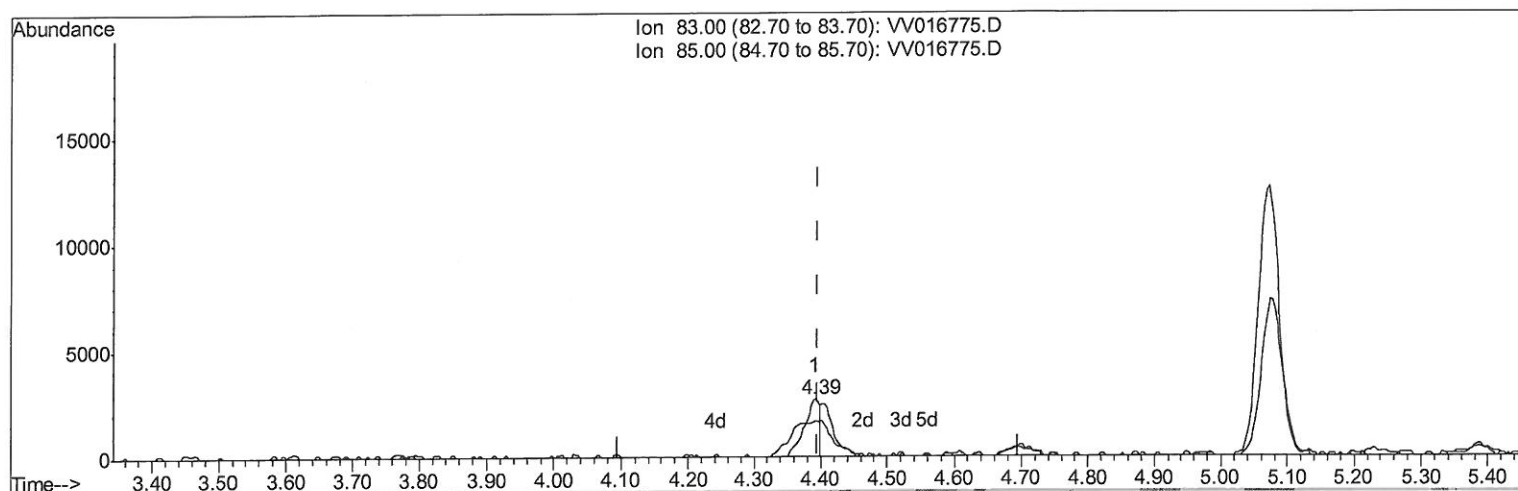

(25) Chloroform (T)

4.392min (-0.003) 0.93ug/L

response 4339

Ion	Exp%	Act%
83.00	100	100
85.00	63.00	61.95
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061020\
 Data File : VV016775.D
 Acq On : 10 Jun 2020 17:38
 Operator : SY/MD
 Sample : L2914-06 20X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9E01

Manual Integrations
 APPROVED

MMDadoda
 6/11/2020 4:23:26 PM

Quant Time: Jun 11 01:08:49 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Jun 11 01:04:46 2020
 Response via : Initial Calibration

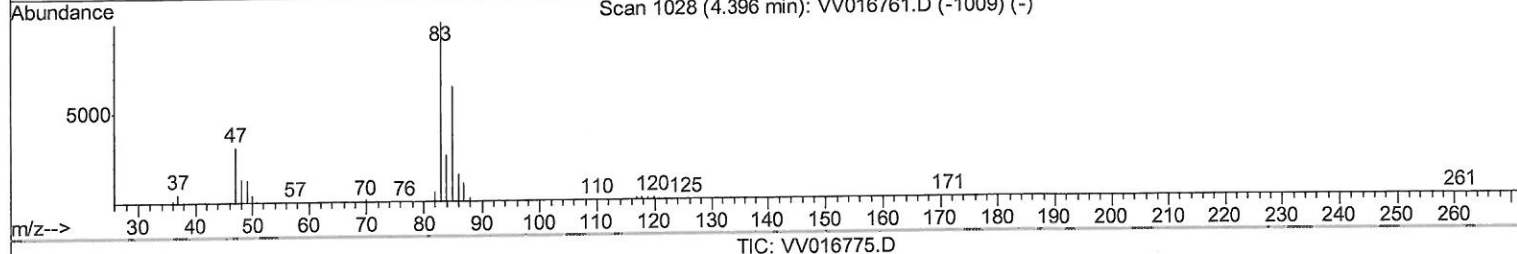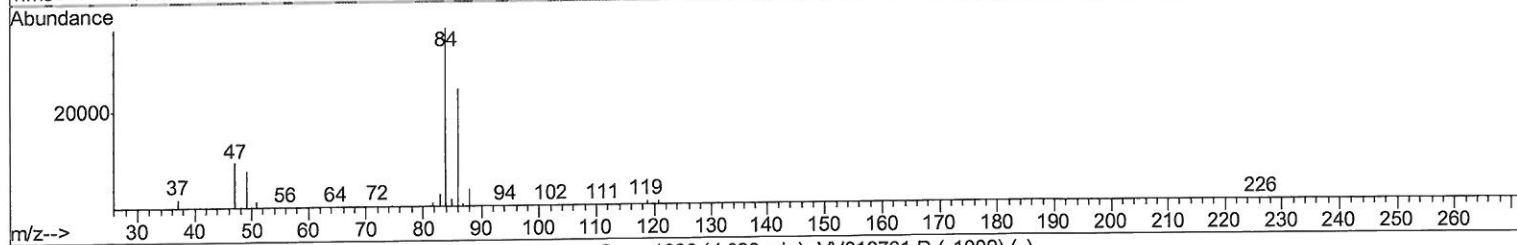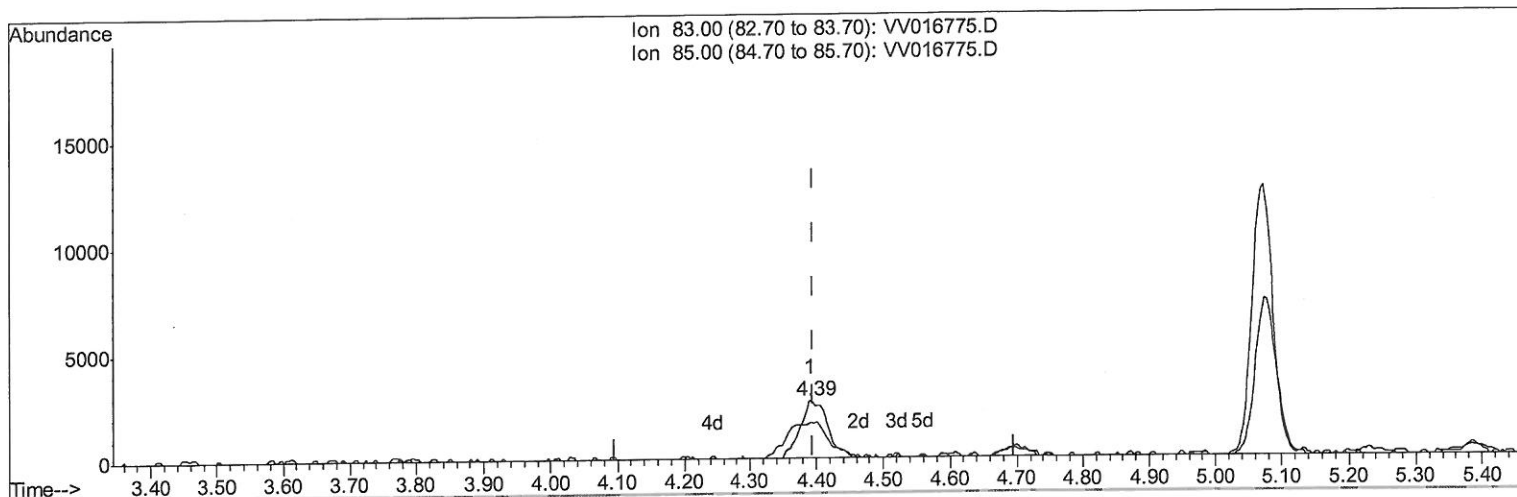

(25) Chloroform (T)

4.392min (-0.003) 1.63ug/L m

response 7592

Ion	Exp%	Act%
83.00	100	100
85.00	63.00	61.95
0.00	0.00	0.00
0.00	0.00	0.00

MD
06/12/20

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061020\
 Data File : VV016775.D
 Acq On : 10 Jun 2020 17:38
 Operator : SY/MD
 Sample : L2914-06 20X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9E01

Manual Integrations
 APPROVED

MMDadoda
 6/11/2020 4:23:26 PM

Quant Time: Jun 11 02:49:20 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Jun 11 01:04:46 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.64	114	355187	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.87	117	334840	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.27	152	176291	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.31	65	118588	47.32	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	94.64%
7) Chloroethane-d5	1.54	69	59848	39.80	ug/L	-0.02
Spiked Amount	50.000	Range	70 - 130	Recovery	=	79.60%
11) 1,1-Dichloroethene-d2	2.11	63	140521	33.39	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	66.78%
21) 2-Butanone-d5	3.90	46	164803	88.84	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	88.84%
24) Chloroform-d	4.37	84	212273	41.65	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	83.30%
26) 1,2-Dichloroethane-d4	5.05	65	157486	45.43	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	90.86%
32) Benzene-d6	5.07	84	436784	45.25	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	90.50%
36) 1,2-Dichloropropane-d6	6.09	67	133307	44.31	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	88.62%
41) Toluene-d8	7.34	98	392984	44.37	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	88.74%
43) trans-1,3-Dichloropropene-	7.64	79	65395	41.73	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	83.46%
47) 2-Hexanone-d5	8.11	63	101911	77.69	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	77.69%
57) 1,1,2,2-Tetrachloroethane-	10.24	84	181126	45.47	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	90.94%
64) 1,2-Dichlorobenzene-d4	11.65	152	174940	46.50	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	93.00%

Target Compounds

					Ovalue	
25) Chloroform	4.39	83	7592m	1.633	ug/L	
29) Cyclohexane	4.69	56	15302	3.678	ug/L	97
33) Benzene	5.12	78	1982557	200.118	ug/L	100
35) Methylcyclohexane	6.15	83	2586	0.620	ug/L	# 63
42) Toluene	7.41	91	41623	3.985	ug/L	96
52) Ethylbenzene	9.04	91	30586	2.644	ug/L	97
53) m,p-Xylene	9.16	106	28297	6.570	ug/L	98
54) o-xylene	9.57	106	10767	2.535	ug/L	91

(#) = qualifier out of range (m) = manual integration (+) = signals summed