

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061020\
 Data File : VV016774.D
 Acq On : 10 Jun 2020 17:14
 Operator : SY/MD
 Sample : L2914-05 20X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9E00

Quant Time: Jun 11 02:45:23 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Jun 11 01:04:46 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.64	114	351922	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.87	117	328615	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.27	152	172984	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.31	65	121932	49.10	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	98.20%
7) Chloroethane-d5	1.54	69	61153	41.04	ug/L	-0.02
Spiked Amount	50.000	Range	70 - 130	Recovery	=	82.08%
11) 1,1-Dichloroethene-d2	2.11	63	143769	34.48	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	68.96%
21) 2-Butanone-d5	3.90	46	165316	89.95	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	89.95%
24) Chloroform-d	4.37	84	218883	43.35	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	86.70%
26) 1,2-Dichloroethane-d4	5.05	65	161229	46.94	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	93.88%
32) Benzene-d6	5.07	84	439790	46.43	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	92.86%
36) 1,2-Dichloropropane-d6	6.09	67	133933	45.36	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	90.72%
41) Toluene-d8	7.33	98	402138	46.26	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	92.52%
43) trans-1,3-Dichloropropene-	7.64	79	67054	43.60	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	87.20%
47) 2-Hexanone-d5	8.11	63	105215	81.73	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	81.73%
57) 1,1,2,2-Tetrachloroethane-	10.24	84	179488	45.92	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	91.84%
64) 1,2-Dichlorobenzene-d4	11.65	152	178924	48.47	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	96.94%

Target Compounds


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
29) Cyclohexane	4.69	56	15621	3.825	ug/L	99
33) Benzene	5.12	78	1942141	199.752	ug/L	100
42) Toluene	7.41	91	40644	3.965	ug/L	99
52) Ethylbenzene	9.04	91	28657	2.524	ug/L	95
53) m,p-Xylene	9.16	106	28254	6.684	ug/L	99
54) o-xylene	9.57	106	10843	2.601	ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV061020\
Data File : VV016774.D
Acq On : 10 Jun 2020 17:14
Operator : SY/MD
Sample : L2914-05 20X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9E00

Quant Time: Jun 11 02:45:23 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Jun 11 01:04:46 2020
Response via : Initial Calibration




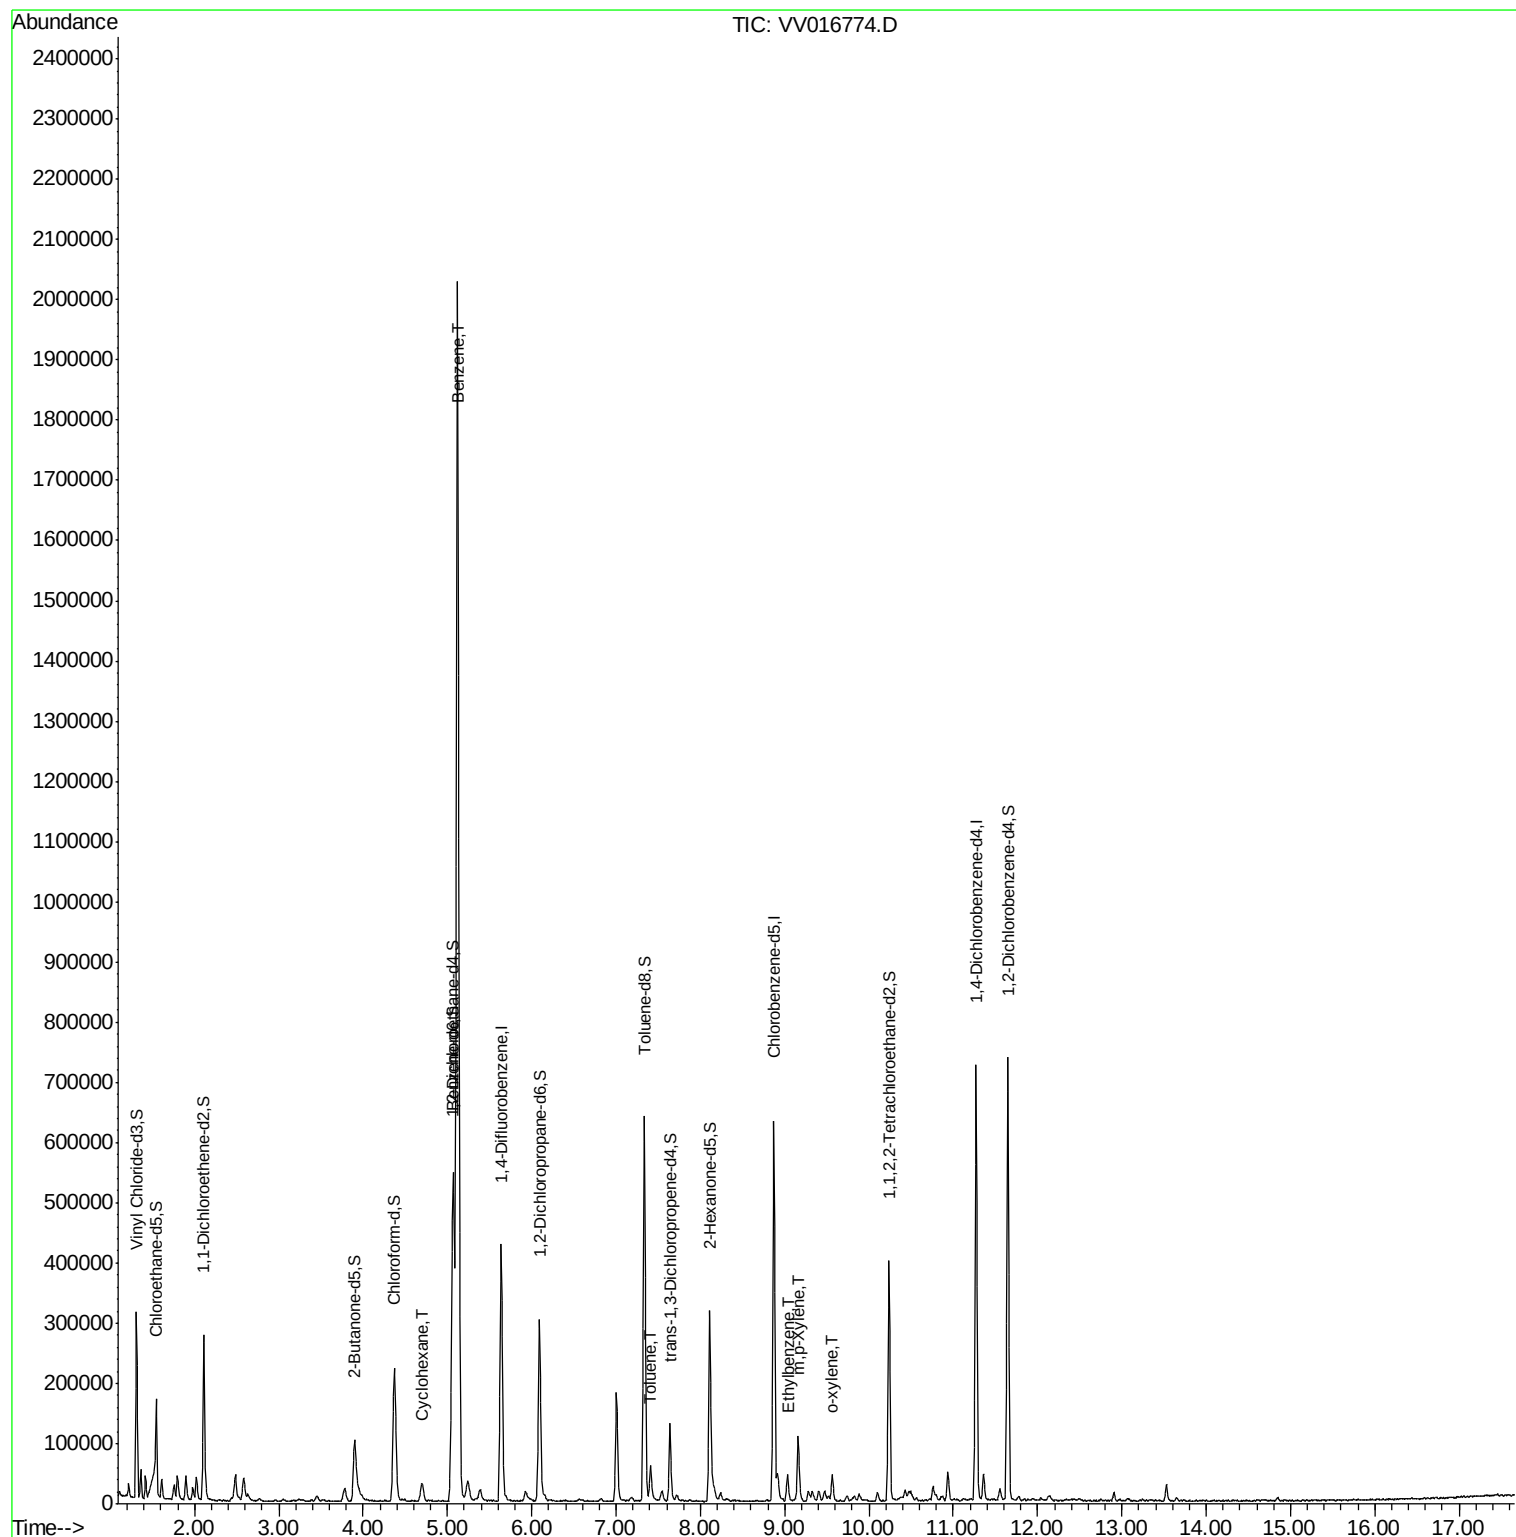


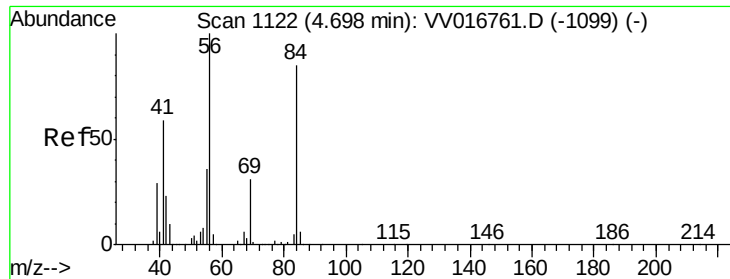

#29
Cyclohexane
Concen: 3.825 ug/L
RT: 4.69 min Scan# 1121
Delta R.T. -0.00 min
Lab File: VV016774.D
Acq: 10 Jun 2020 17:14




Instrument :
MSVOA_V
ClientSampleId :
F9E00


Tot Ion: 56 Resp: 15621
Ion Ratio Lower Upper
56 100
69 33.3 25.0 37.4
84 87.1 69.5 104.3

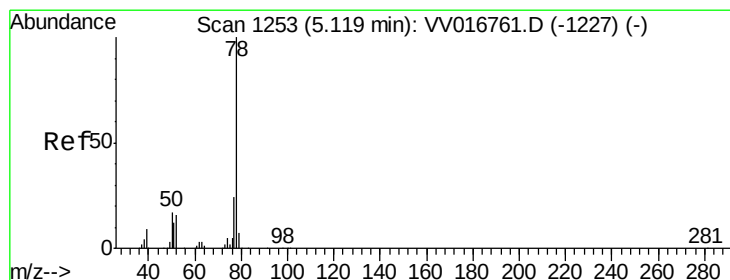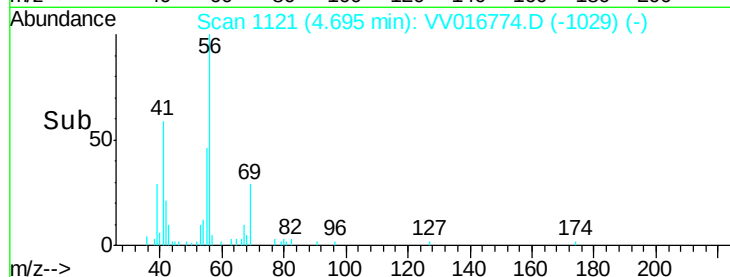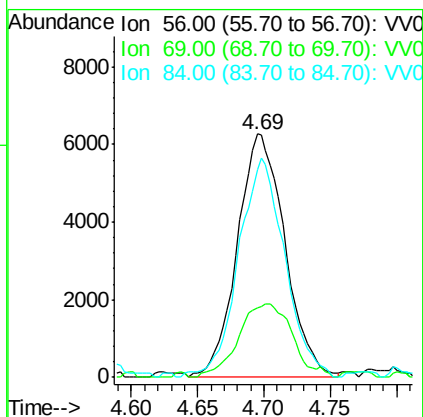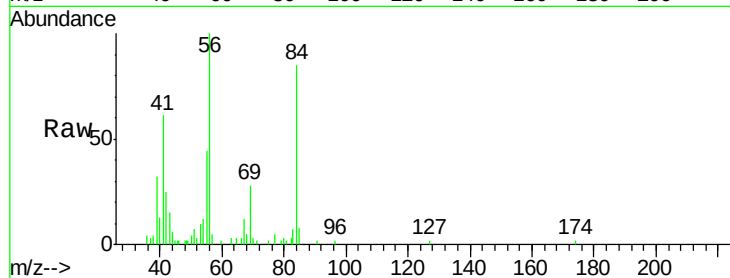

#33
Benzene
Concen: 199.752 ug/L
RT: 5.12 min Scan# 1253
Delta R.T. 0.00 min
Lab File: VV016774.D
Acq: 10 Jun 2020 17:14

Tgt Ion: 78 Resp: 1942141

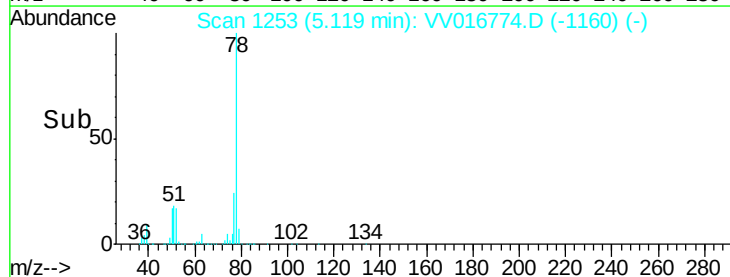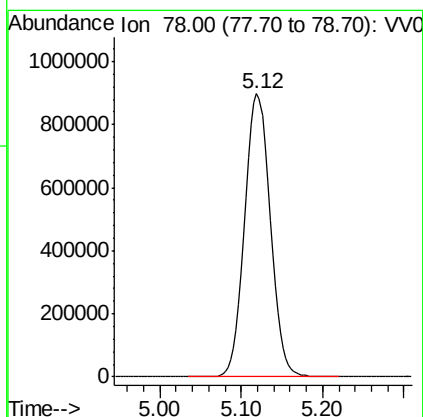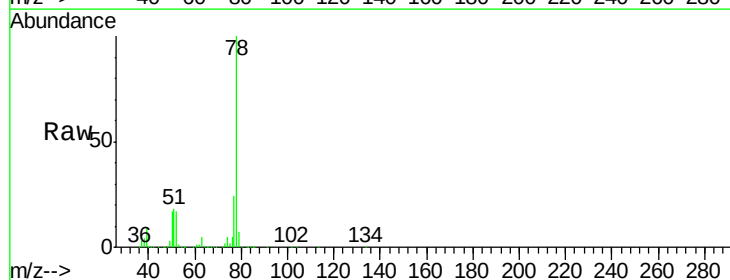

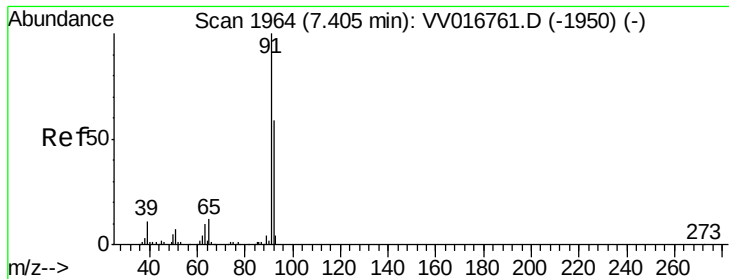

#42

Toluene

Concen: 3.965 ug/L

RT: 7.41 min Scan# 1965

Delta R.T. 0.00 min

Lab File: VV016774.D

Acq: 10 Jun 2020 17:14

Instrument :

MSVOA_V

ClientSampleId :





F9E00

Tot Ion: 91 Resp: 40644

Ion Ratio Lower Upper

91 100

92 58.8 40.4 75.0

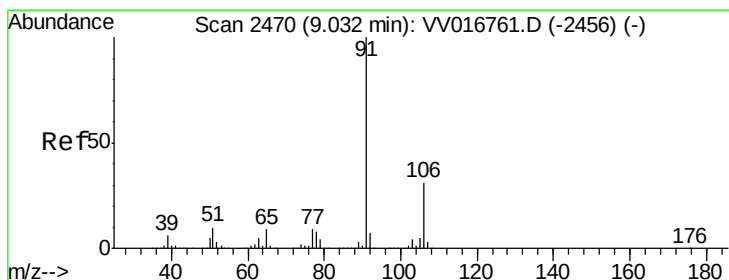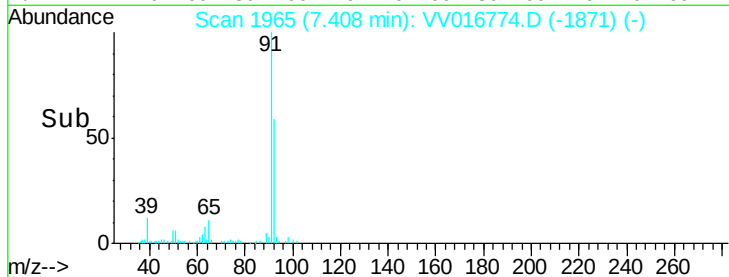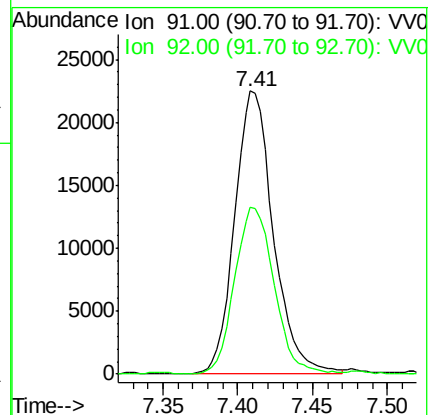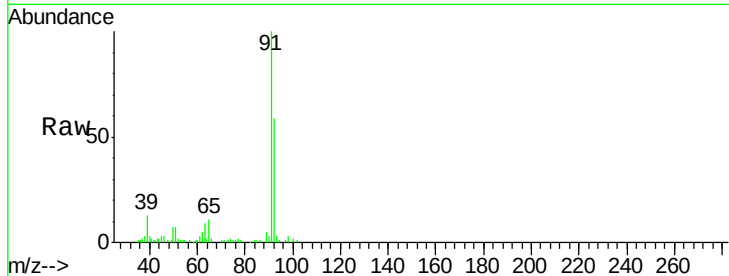

#52

Ethylbenzene

Concen: 2.524 ug/L

RT: 9.04 min Scan# 2471

Delta R.T. 0.00 min

Lab File: VV016774.D




Acq: 10 Jun 2020 17:14


Tgt Ion: 91 Resp: 28657

Ion Ratio Lower Upper

91 100

106 32.7 21.1 39.1

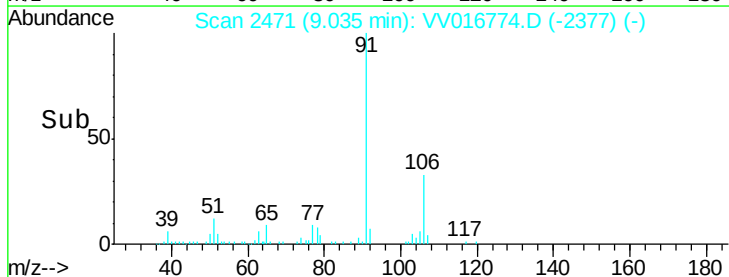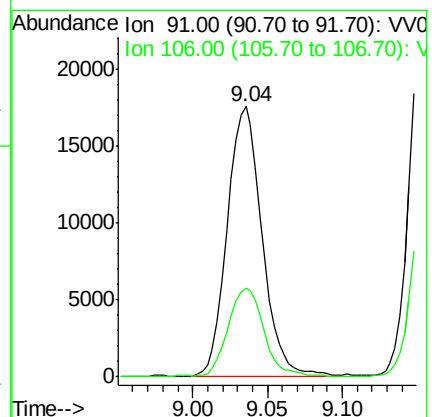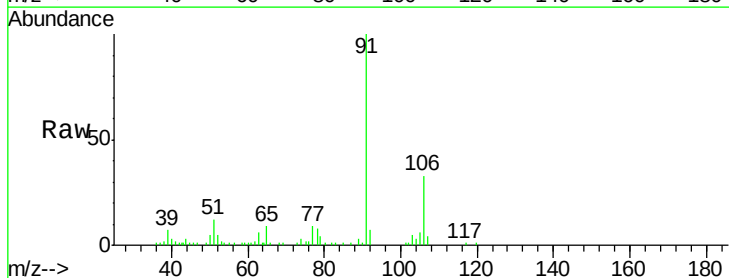

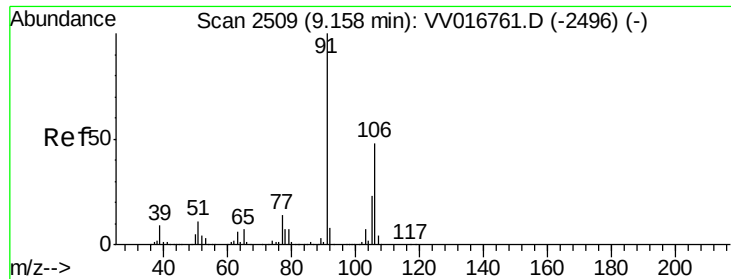

#53

m,p-Xylene

Concen: 6.684 ug/L

RT: 9.16 min Scan# 2510

Delta R.T. 0.00 min

Lab File: VV016774.D

Acq: 10 Jun 2020 17:14

Instrument :

MSVOA_V

ClientSampleId :


F9E00

Tot Ion:106 Resp: 28254

Ion Ratio Lower Upper




106 100

91 204.4 144.6 268.6

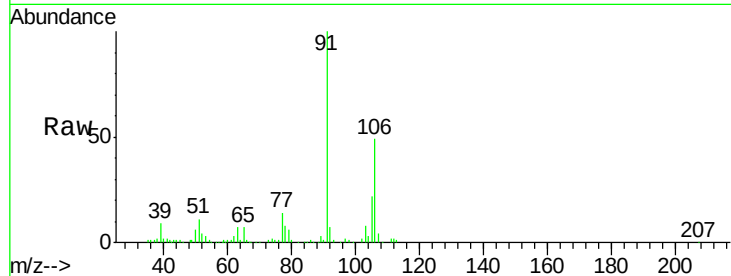

Abundance Ion 106.00 (105.70 to 106.70): V

Ion 91.00 (90.70 to 91.70): VV0

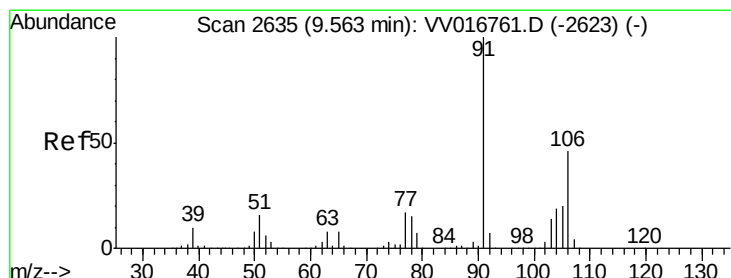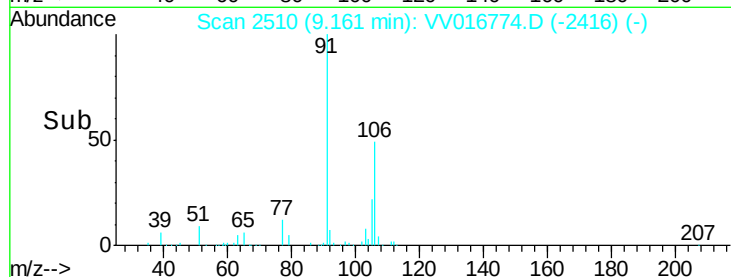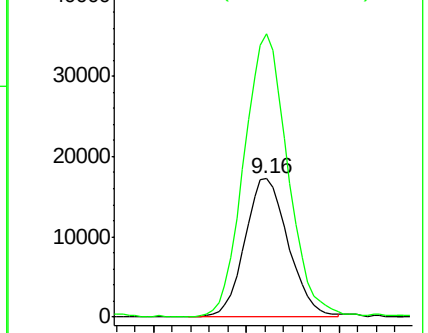

#54

o-xylene

Concen: 2.601 ug/L

RT: 9.57 min Scan# 2636

Delta R.T. 0.00 min

Lab File: VV016774.D


Acq: 10 Jun 2020 17:14

Tgt Ion:106 Resp: 10843

Ion Ratio Lower Upper

106 100

91 215.3 155.9 289.5

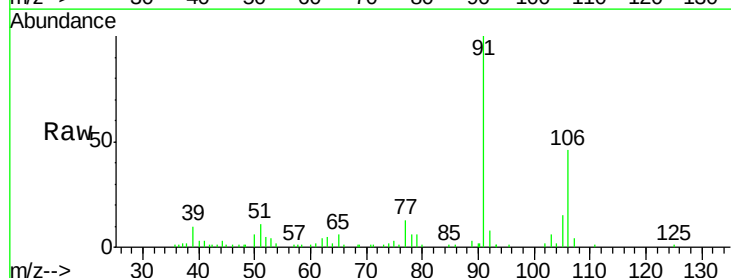

Abundance Ion 106.00 (105.70 to 106.70): V

Ion 91.00 (90.70 to 91.70): VV0

