

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061020\
 Data File : VV016801.D
 Acq On : 11 Jun 2020 04:21
 Operator : SY/MD
 Sample : L2848-10
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AG2

Quant Time: Jun 11 06:53:01 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Jun 11 04:06:22 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.64	114	307336	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.87	117	294513	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.27	152	143222	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.31	65	92869	42.82	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	85.64%
7) Chloroethane-d5	1.56	69	66967	51.46	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	102.92%
11) 1,1-Dichloroethene-d2	2.12	63	129804	35.64	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	71.28%
21) 2-Butanone-d5	3.89	46	155192	96.69	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	96.69%
24) Chloroform-d	4.37	84	204522	46.38	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	92.76%
26) 1,2-Dichloroethane-d4	5.05	65	147907	49.31	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	98.62%
32) Benzene-d6	5.07	84	402819	47.45	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	94.90%
36) 1,2-Dichloropropane-d6	6.09	67	121773	46.02	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	92.04%
41) Toluene-d8	7.34	98	359775	46.18	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	92.36%
43) trans-1,3-Dichloropropene-	7.64	79	59015	42.82	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	85.64%
47) 2-Hexanone-d5	8.11	63	87384	75.74	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	75.74%
57) 1,1,2,2-Tetrachloroethane-	10.24	84	159630	45.57	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	91.14%
64) 1,2-Dichlorobenzene-d4	11.65	152	156794	51.30	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	102.60%


Target Compounds					Ovalue
13) Acetone	2.17	43	5658	5.350 ug/L	90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061020\
Data File : VV016801.D
Acq On : 11 Jun 2020 04:21
Operator : SY/MD
Sample : L2848-10
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AG2

Quant Time: Jun 11 06:53:01 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Jun 11 04:06:22 2020
Response via : Initial Calibration

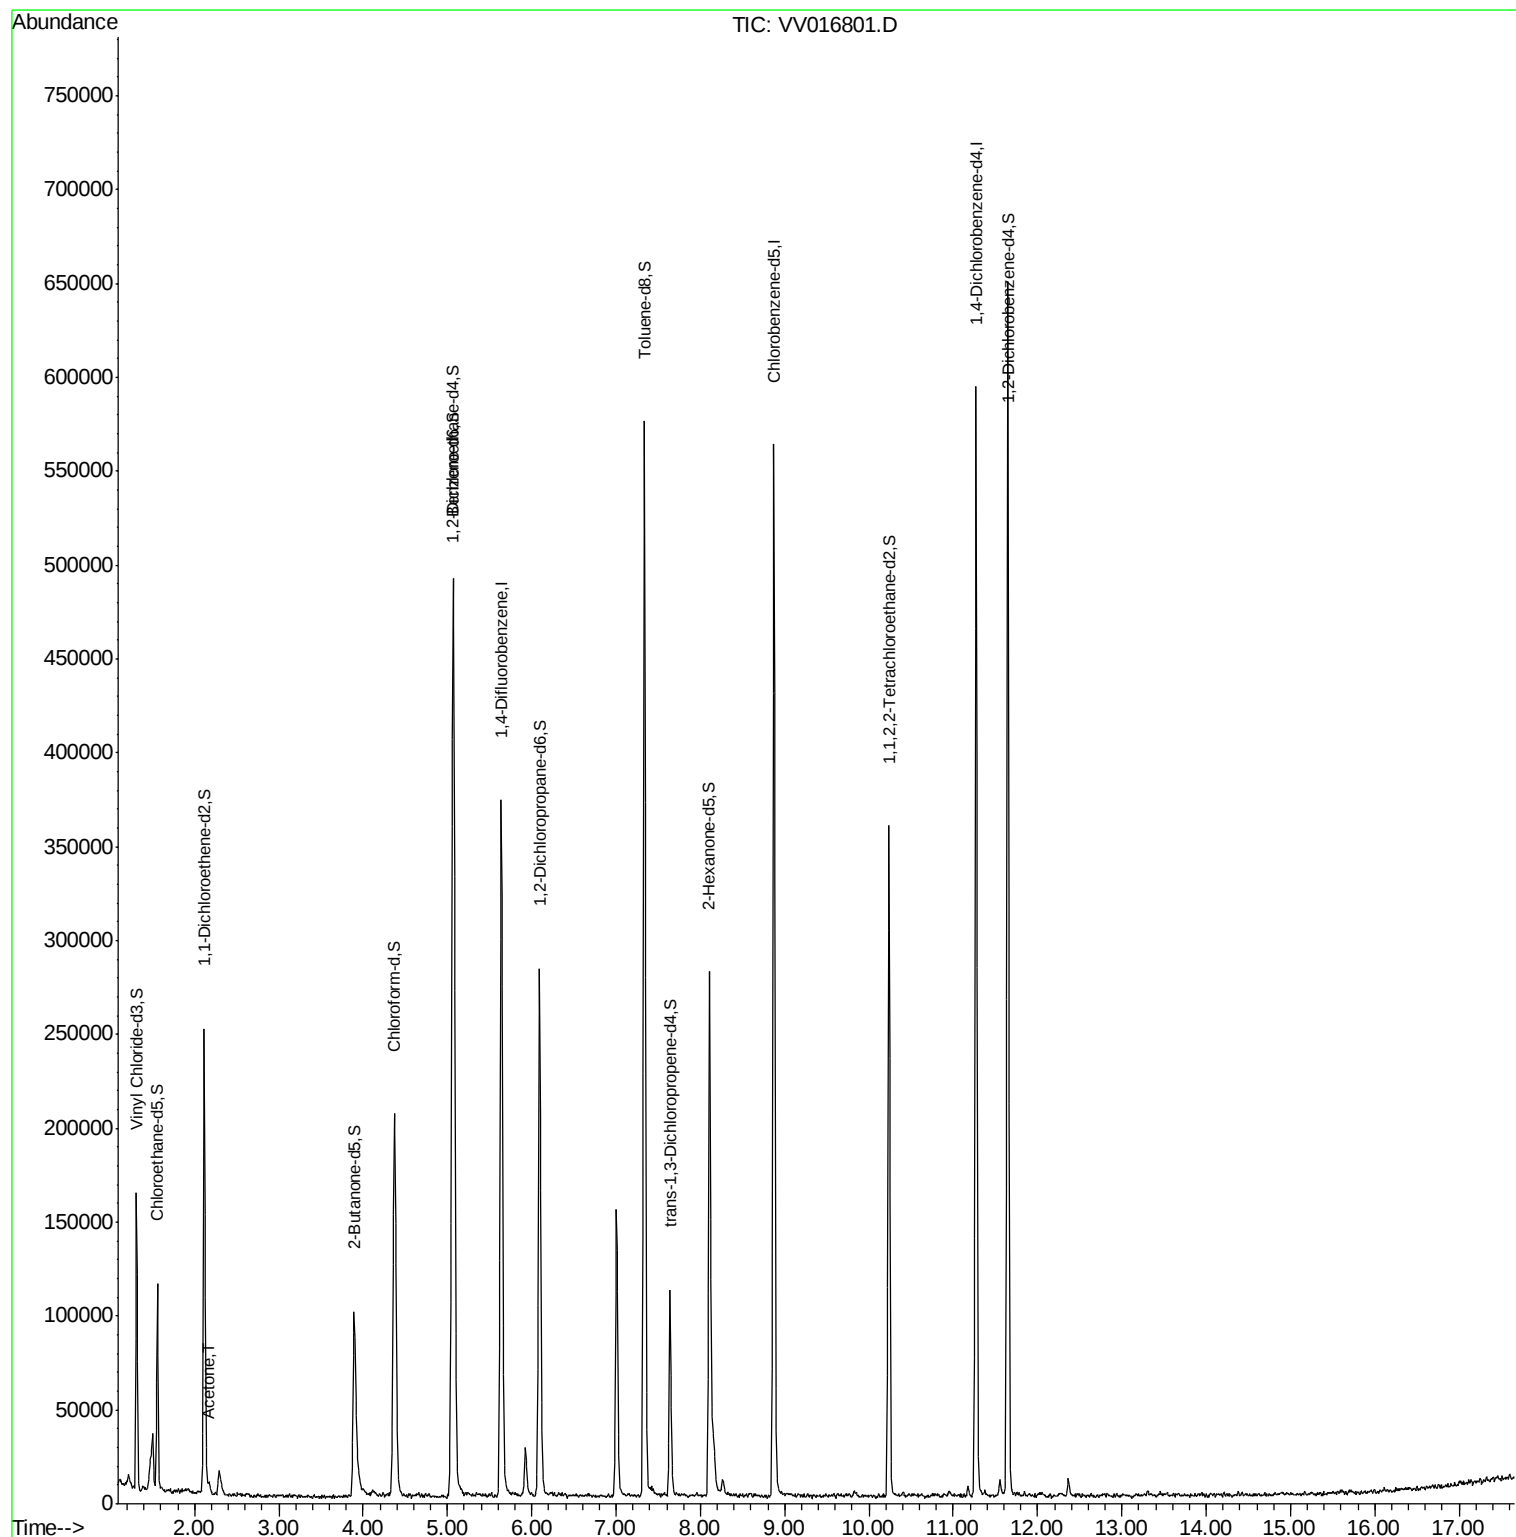

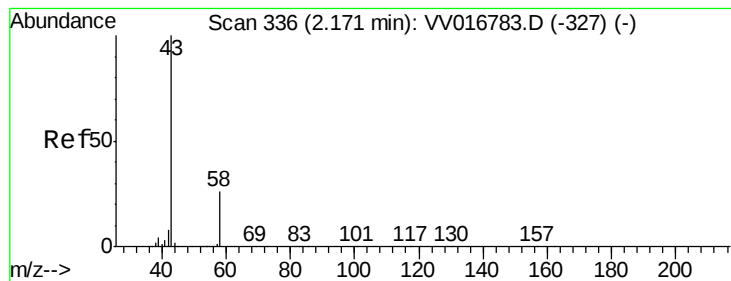

#13
 Acetone
 Concen: 5.350 ug/L
 RT: 2.17 min Scan# 335
 Delta R.T. -0.00 min
 Lab File: VV016801.D
 Acq: 11 Jun 2020 04:21

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AG2

Tot Ion: 43 Resp: 5658
 Ion Ratio Lower Upper
 43 100
 58 32.6 0.0 55.2

