

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061020\
 Data File : VV016807.D
 Acq On : 11 Jun 2020 06:43
 Operator : SY/MD
 Sample : L2945-02
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW0N1

Quant Time: Jun 11 07:52:36 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Jun 11 04:06:22 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.64	114	311554	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.87	117	297865	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.27	152	142208	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.31	65	90961	41.38	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	82.76%
7) Chloroethane-d5	1.55	69	64692	49.04	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	98.08%
11) 1,1-Dichloroethene-d2	2.11	63	127286	34.48	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	68.96%
21) 2-Butanone-d5	3.89	46	152605	93.79	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	93.79%
24) Chloroform-d	4.37	84	205256	45.92	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	91.84%
26) 1,2-Dichloroethane-d4	5.05	65	148511	48.84	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	97.68%
32) Benzene-d6	5.07	84	395519	46.06	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	92.12%
36) 1,2-Dichloropropane-d6	6.09	67	122602	45.81	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	91.62%
41) Toluene-d8	7.34	98	356931	45.30	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	90.60%
43) trans-1,3-Dichloropropene-	7.64	79	55443	39.77	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	79.54%
47) 2-Hexanone-d5	8.11	63	85747	73.48	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	73.48%
57) 1,1,2,2-Tetrachloroethane-	10.24	84	155356	43.85	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	87.70%
64) 1,2-Dichlorobenzene-d4	11.65	152	152701	50.32	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	100.64%


Target Compounds					Ovalue
13) Acetone	2.17	43	4109	3.833 ug/L	86


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061020\
Data File : VV016807.D
Acq On : 11 Jun 2020 06:43
Operator : SY/MD
Sample : L2945-02
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 49 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW0N1

Quant Time: Jun 11 07:52:36 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Jun 11 04:06:22 2020
Response via : Initial Calibration

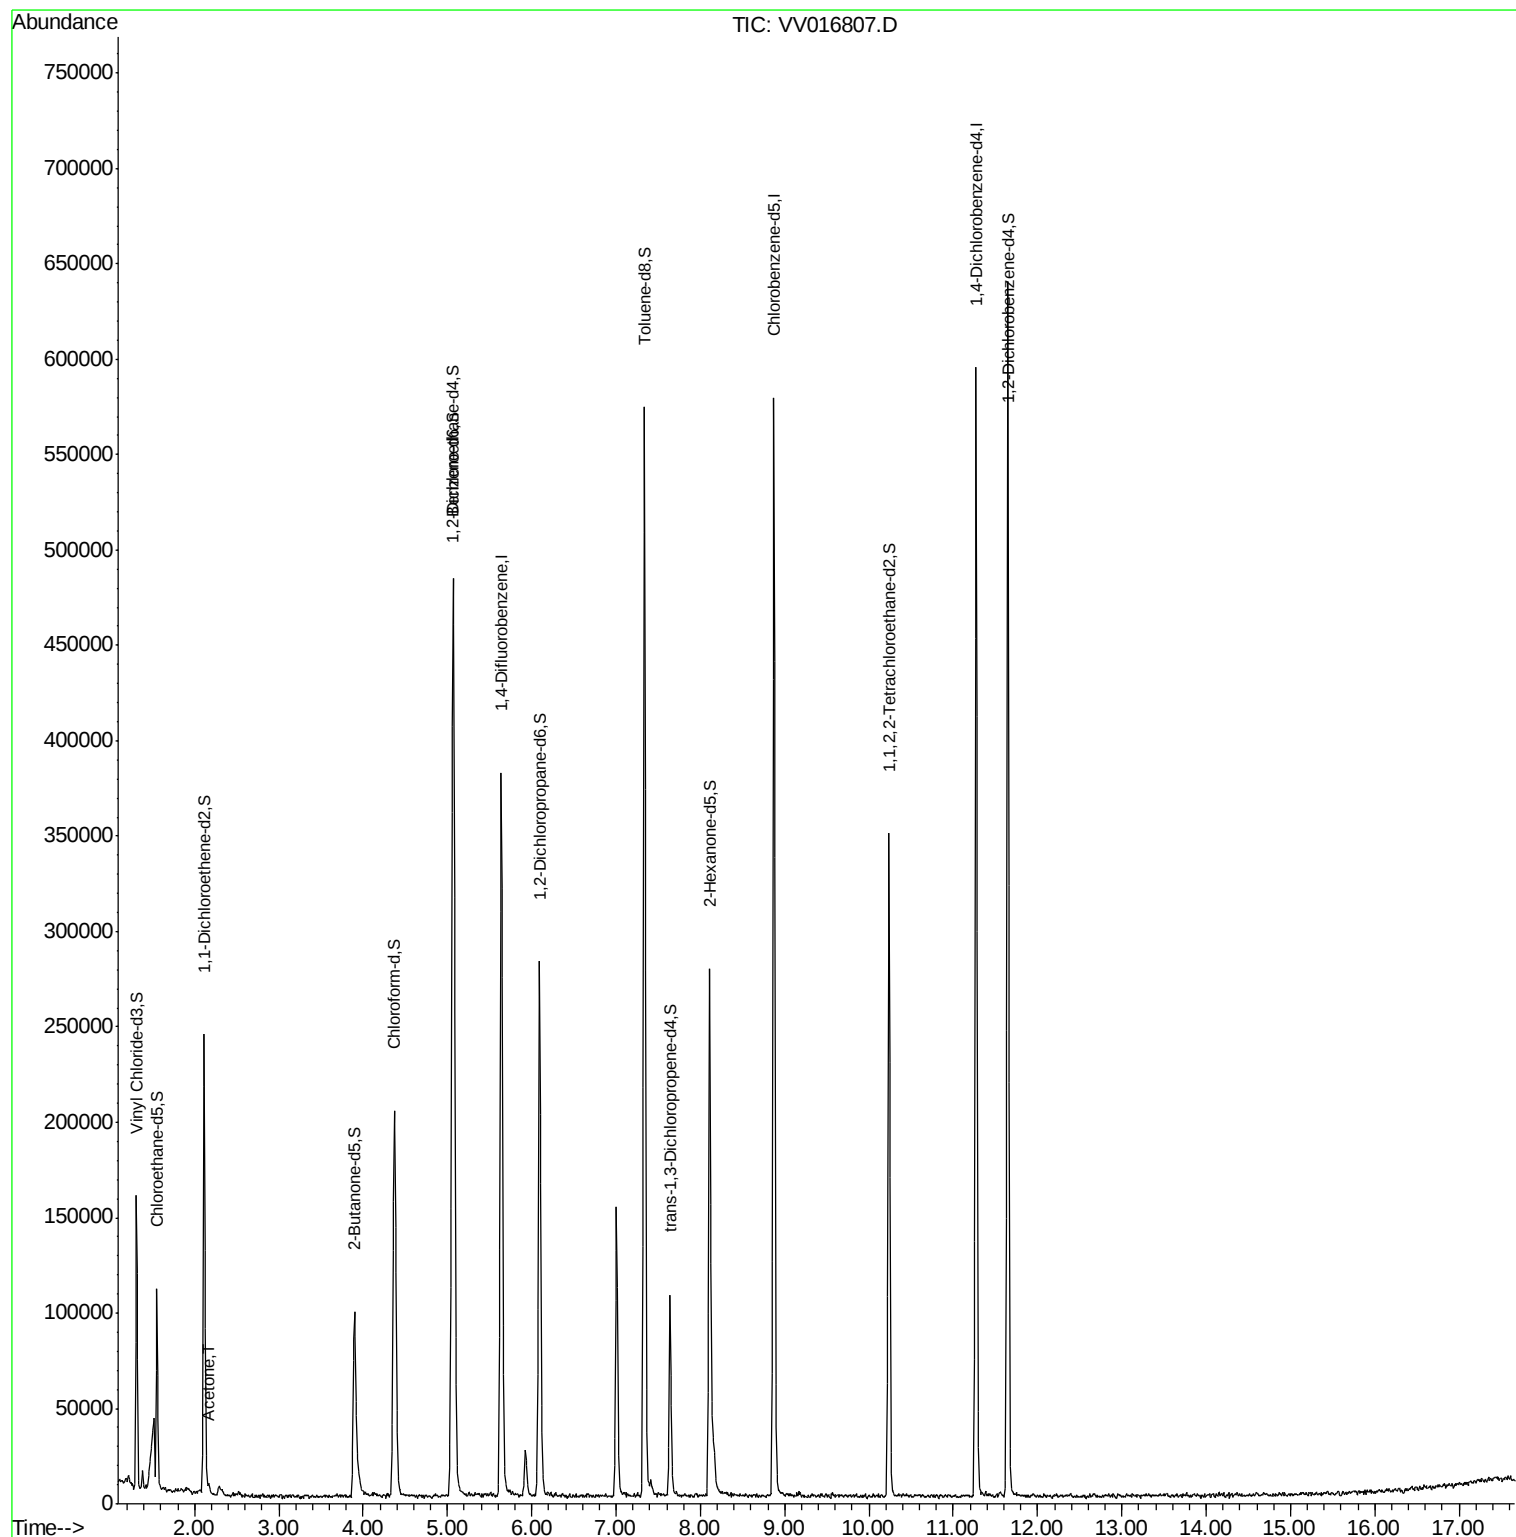

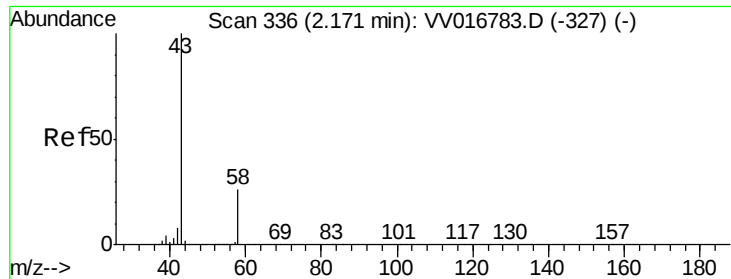

#13

Acetone

Concen: 3.833 ug/L

RT: 2.17 min Scan# 337

Delta R.T. 0.00 min

Lab File: VV016807.D

Acq: 11 Jun 2020 06:43

Instrument :

MSVOA_V

ClientSampleId :

EW0N1

Tot Ion: 43 Resp: 4109

Ion Ratio Lower Upper

43 100

58 34.9 0.0 55.2

