

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061020\
 Data File : VV016762.D
 Acq On : 10 Jun 2020 12:22
 Operator : SY/MD
 Sample : VV0610WBL01
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK78

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	64	70	82	rVB	209736	205601	13.33%	1.771%
2	1.573	143	150	164	rVB	142489	169296	10.97%	1.458%
3	2.119	311	320	343	rVB	320701	483622	31.35%	4.165%
4	2.389	402	404	406	rBV3	1793	1018	0.07%	0.009%
5	2.621	473	476	478	rBV4	1877	993	0.06%	0.009%
6	2.901	557	563	566	rBV7	2927	2205	0.14%	0.019%
7	2.952	574	579	581	rBV6	1147	956	0.06%	0.008%
8	3.010	592	597	601	rVB7	2129	2048	0.13%	0.018%
9	3.032	601	604	605	rBV3	1046	664	0.04%	0.006%
10	3.064	609	614	617	rBV6	1961	1521	0.10%	0.013%
11	3.097	622	624	626	rBV4	1260	485	0.03%	0.004%
12	3.171	643	647	649	rBV5	1140	1028	0.07%	0.009%
13	3.203	654	657	660	rBV3	1876	1488	0.10%	0.013%
14	3.270	674	678	679	rBV4	1645	976	0.06%	0.008%
15	3.380	708	712	714	rVB4	1171	886	0.06%	0.008%
16	3.441	729	731	735	rBV4	1244	945	0.06%	0.008%
17	3.518	753	755	758	rVB3	1097	747	0.05%	0.006%
18	3.556	764	767	768	rBV3	1872	909	0.06%	0.008%
19	3.650	791	796	798	rBV6	981	694	0.04%	0.006%
20	3.704	812	813	817	rVB4	1735	920	0.06%	0.008%
21	3.801	842	843	845	rBV2	1233	525	0.03%	0.005%
22	3.817	845	848	852	rVB7	1536	998	0.06%	0.009%
23	3.846	852	857	859	rBV6	1356	1125	0.07%	0.010%
24	3.891	859	871	898	rBV	119286	325655	21.11%	2.804%
25	4.135	943	947	948	rBV4	1383	929	0.06%	0.008%
26	4.225	972	975	978	rBV4	1347	957	0.06%	0.008%
27	4.370	1004	1020	1042	rBV2	246468	607004	39.34%	5.227%
28	4.544	1071	1074	1075	rBV3	1652	1080	0.07%	0.009%
29	4.592	1086	1089	1090	rBV3	838	513	0.03%	0.004%
30	4.762	1140	1142	1145	rBV4	1370	766	0.05%	0.007%
31	4.775	1145	1146	1150	rVB3	940	543	0.04%	0.005%
32	4.794	1150	1152	1154	rBV3	1218	551	0.04%	0.005%
33	4.807	1154	1156	1159	rBV3	999	715	0.05%	0.006%
34	4.910	1186	1188	1193	rVB5	1094	732	0.05%	0.006%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061020\
 Data File : VV016762.D
 Acq On : 10 Jun 2020 12:22
 Operator : SY/MD
 Sample : VV0610WBL01
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK78

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

35	4.939	1195	1197	1202	rBV5	1238	1004	0.07%	0.009%
36	5.068	1218	1237	1262	rBV2	594838	1542774	100.00%	13.286%
37	5.363	1325	1329	1330	rBV4	1640	1072	0.07%	0.009%
38	5.466	1356	1361	1363	rBV6	1904	1425	0.09%	0.012%
39	5.637	1400	1414	1435	rBV	452725	904652	58.64%	7.791%
40	6.090	1539	1555	1581	rBV	348422	698017	45.24%	6.011%
41	6.453	1666	1668	1669	rBV2	1335	490	0.03%	0.004%
42	6.666	1730	1734	1737	rBV5	3072	2841	0.18%	0.024%
43	6.730	1750	1754	1755	rBV4	767	556	0.04%	0.005%
44	6.743	1755	1758	1761	rBV5	1279	871	0.06%	0.008%
45	6.833	1784	1786	1788	rVB3	2032	741	0.05%	0.006%
46	6.881	1799	1801	1804	rBV3	870	519	0.03%	0.004%
47	7.003	1827	1839	1861	rBV	206870	368206	23.87%	3.171%
48	7.241	1911	1913	1915	rBV3	1502	820	0.05%	0.007%
49	7.334	1930	1942	1958	rBV	718968	1233985	79.98%	10.627%
50	7.572	2014	2016	2017	rBV2	1163	515	0.03%	0.004%
51	7.640	2026	2037	2054	rBV	148187	249482	16.17%	2.148%
52	7.842	2098	2100	2101	rBV2	1801	858	0.06%	0.007%
53	8.068	2166	2170	2171	rBV4	1750	1137	0.07%	0.010%
54	8.103	2171	2181	2216	rVV	352859	666213	43.18%	5.737%
55	8.588	2330	2332	2335	rBV4	1084	854	0.06%	0.007%
56	8.669	2355	2357	2359	rBV3	1071	586	0.04%	0.005%
57	8.778	2389	2391	2392	rBV2	1279	488	0.03%	0.004%
58	8.871	2409	2420	2438	rBV	683871	1095334	71.00%	9.433%
59	9.405	2584	2586	2588	rBV3	1111	571	0.04%	0.005%
60	9.530	2622	2625	2627	rBV2	1631	1065	0.07%	0.009%
61	9.563	2629	2635	2638	rBV8	3764	4585	0.30%	0.039%
62	9.656	2663	2664	2668	rVB4	1104	552	0.04%	0.005%
63	9.701	2675	2678	2682	rVB4	1732	1485	0.10%	0.013%
64	9.730	2682	2687	2689	rBV6	1638	1261	0.08%	0.011%
65	9.826	2711	2717	2721	rBV8	1498	1669	0.11%	0.014%
66	9.894	2733	2738	2740	rBV4	1764	1590	0.10%	0.014%
67	9.932	2747	2750	2751	rBV3	1313	770	0.05%	0.007%
68	10.019	2773	2777	2780	rBV4	1328	1422	0.09%	0.012%
69	10.100	2800	2802	2807	rBV4	1362	1169	0.08%	0.010%
70	10.238	2831	2845	2861	rBV	438457	689608	44.70%	5.939%
71	10.466	2913	2916	2917	rBV2	972	576	0.04%	0.005%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061020\
 Data File : VV016762.D
 Acq On : 10 Jun 2020 12:22
 Operator : SY/MD
 Sample : VV0610WBL01
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK78

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

72	10.524	2930	2934	2938	rBV6	1643	1578	0.10%	0.014%
73	10.556	2939	2944	2951	rVV9	2826	4234	0.27%	0.036%
74	10.672	2978	2980	2983	rBV4	1528	885	0.06%	0.008%
75	10.704	2988	2990	2992	rVB3	1244	456	0.03%	0.004%
76	10.723	2992	2996	2998	rBV3	1351	1153	0.07%	0.010%
77	10.736	2998	3000	3002	rBV3	1333	786	0.05%	0.007%
78	10.804	3020	3021	3028	rBV6	1497	1399	0.09%	0.012%
79	10.874	3040	3043	3044	rBV3	1058	589	0.04%	0.005%
80	11.199	3136	3144	3148	rBV10	4511	6846	0.44%	0.059%
81	11.270	3155	3166	3187	rVB	719996	1094313	70.93%	9.424%
82	11.527	3243	3246	3248	rBV4	1615	853	0.06%	0.007%
83	11.646	3272	3283	3298	rBV	748878	1165228	75.53%	10.035%
84	11.855	3342	3348	3352	rBV8	3039	3247	0.21%	0.028%
85	12.074	3412	3416	3420	rBV6	2284	2034	0.13%	0.018%
86	12.270	3473	3477	3479	rBV6	1468	1119	0.07%	0.010%
87	12.302	3484	3487	3489	rBV3	2599	1692	0.11%	0.015%
88	12.354	3501	3503	3507	rVB5	1616	831	0.05%	0.007%
89	12.427	3522	3526	3528	rBV6	1543	1357	0.09%	0.012%
90	12.624	3585	3587	3591	rBV5	1416	941	0.06%	0.008%
91	12.646	3591	3594	3595	rBV3	2029	1224	0.08%	0.011%
92	12.746	3622	3625	3627	rBV4	1331	1112	0.07%	0.010%
93	12.971	3690	3695	3696	rBV4	1261	848	0.05%	0.007%
94	13.135	3742	3746	3747	rBV3	1076	589	0.04%	0.005%
95	13.775	3934	3945	3950	rBV3	8612	15693	1.02%	0.135%
96	13.836	3962	3964	3965	rBV2	1403	485	0.03%	0.004%
97	13.951	3998	4000	4001	rBV2	1165	496	0.03%	0.004%
98	14.714	4235	4237	4239	rBV3	2069	1158	0.08%	0.010%
99	14.797	4261	4263	4265	rBV3	1365	704	0.05%	0.006%
100	14.942	4304	4308	4311	rBV4	1815	1362	0.09%	0.012%


Sum of corrected areas: 11612070

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV061020\
Data File : VV016762.D
Acq On : 10 Jun 2020 12:22
Operator : SY/MD
Sample : VV0610WBL01
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK78

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

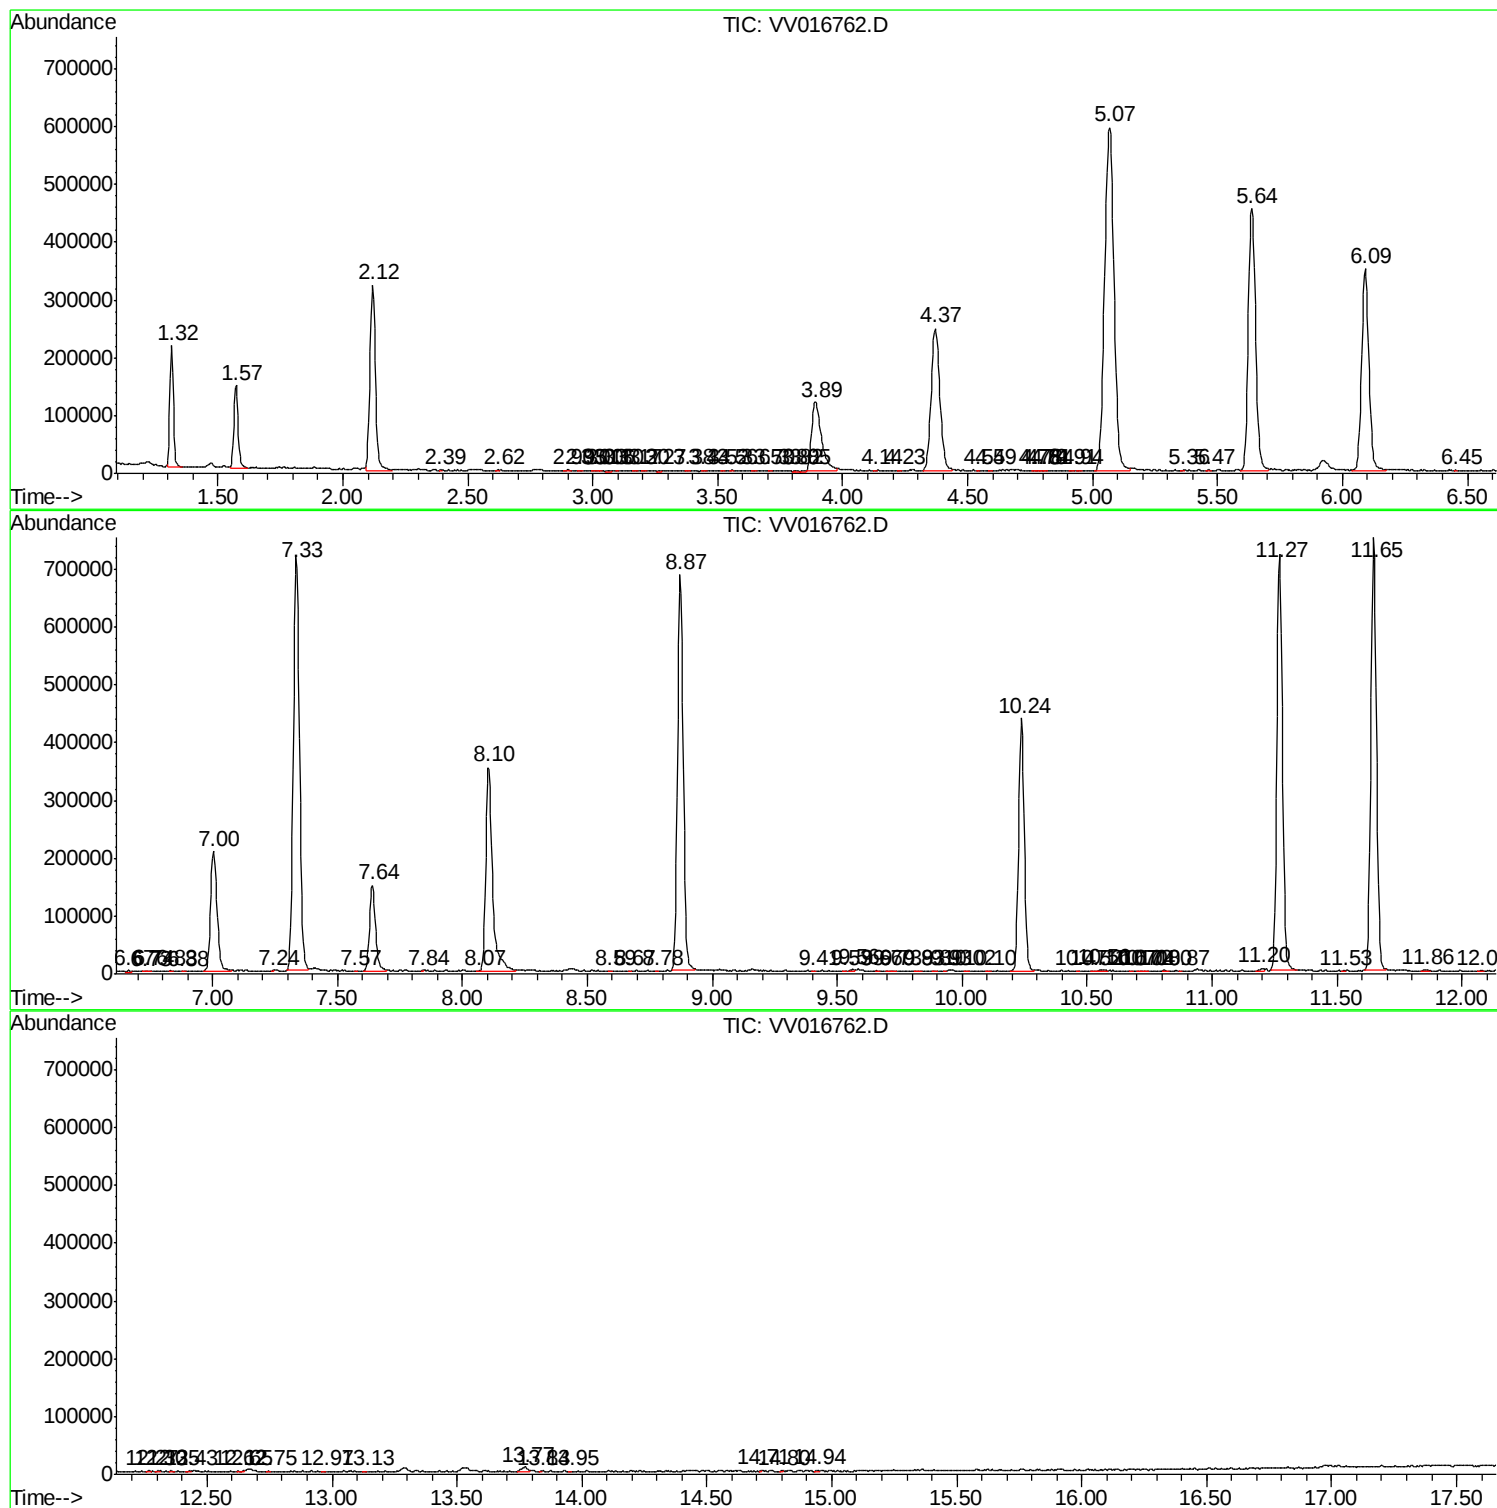

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV061020\
Data File : VV016762.D
Acq On : 10 Jun 2020 12:22
Operator : SY/MD
Sample : VV0610WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK78

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV061020\
Data File : VV016762.D
Acq On : 10 Jun 2020 12:22
Operator : SY/MD
Sample : VV0610WBL01
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
VBLK78

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc