

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061020\
 Data File : VV016764.D
 Acq On : 10 Jun 2020 13:15
 Operator : SY/MD
 Sample : L2901-22DL 5X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTS3DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	63	70	83	rVB2	581153	629870	43.97%	4.983%
2	2.110	308	317	332	rBV	292379	431153	30.10%	3.411%
3	2.627	464	478	492	rBV	10784	26458	1.85%	0.209%
4	2.862	549	551	552	rBV2	930	468	0.03%	0.004%
5	2.904	562	564	568	rBV3	2441	1629	0.11%	0.013%
6	2.920	568	569	572	rVB3	938	453	0.03%	0.004%
7	2.942	572	576	579	rBV5	1778	1599	0.11%	0.013%
8	2.981	587	588	591	rBV3	950	529	0.04%	0.004%
9	3.029	601	603	608	rVB6	1709	1206	0.08%	0.010%
10	3.087	619	621	624	rVB3	1176	453	0.03%	0.004%
11	3.116	629	630	632	rBV2	1404	790	0.06%	0.006%
12	3.148	637	640	643	rBV5	1569	1180	0.08%	0.009%
13	3.196	653	655	656	rBV	1092	504	0.04%	0.004%
14	3.219	659	662	664	rBV3	1253	826	0.06%	0.007%
15	3.264	672	676	677	rBV3	1063	593	0.04%	0.005%
16	3.299	685	687	690	rBV3	1142	874	0.06%	0.007%
17	3.335	696	698	700	rBV3	982	545	0.04%	0.004%
18	3.383	708	713	715	rBV6	2395	1900	0.13%	0.015%
19	3.409	719	721	724	rBV4	1892	1089	0.08%	0.009%
20	3.473	738	741	742	rBV3	1150	591	0.04%	0.005%
21	3.515	753	754	757	rBV3	2071	1278	0.09%	0.010%
22	3.582	773	775	779	rVB4	1275	715	0.05%	0.006%
23	3.605	779	782	784	rBV4	1740	1165	0.08%	0.009%
24	3.679	799	805	807	rBV7	1417	1374	0.10%	0.011%
25	3.698	807	811	812	rBV3	1174	719	0.05%	0.006%
26	3.781	833	837	838	rBV4	1230	880	0.06%	0.007%
27	3.823	843	850	862	rVV6	12661	30331	2.12%	0.240%
28	3.929	863	883	925	rVV2	396873	1259112	87.90%	9.962%
29	4.283	990	993	996	rBV4	1654	1537	0.11%	0.012%
30	4.373	1006	1021	1046	rVB	243037	574896	40.13%	4.548%
31	4.598	1089	1091	1092	rBV2	1676	794	0.06%	0.006%
32	4.669	1110	1113	1114	rBV3	1052	468	0.03%	0.004%
33	4.679	1114	1116	1118	rVV3	1572	787	0.05%	0.006%
34	4.691	1118	1120	1124	rVV4	1858	1345	0.09%	0.011%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061020\
 Data File : VV016764.D
 Acq On : 10 Jun 2020 13:15
 Operator : SY/MD
 Sample : L2901-22DL 5X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTS3DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

35	4.785	1144	1149	1151	rBV6	1320	1302	0.09%	0.010%
36	4.888	1178	1181	1182	rBV3	1026	509	0.04%	0.004%
37	4.949	1198	1200	1203	rVB4	1177	686	0.05%	0.005%
38	5.068	1220	1237	1259	rBV2	567855	1432509	100.00%	11.333%
39	5.408	1341	1343	1345	rBV3	1202	507	0.04%	0.004%
40	5.441	1349	1353	1356	rBV5	1158	1136	0.08%	0.009%
41	5.579	1394	1396	1398	rBV3	1372	686	0.05%	0.005%
42	5.637	1401	1414	1440	rVV	446232	891210	62.21%	7.051%
43	5.923	1493	1503	1504	rBV8	14458	17923	1.25%	0.142%
44	6.090	1543	1555	1579	rBV	322115	645715	45.08%	5.109%
45	6.469	1671	1673	1674	rBV2	1046	417	0.03%	0.003%
46	6.875	1797	1799	1803	rBV4	989	467	0.03%	0.004%
47	7.006	1829	1840	1855	rBV	189917	339897	23.73%	2.689%
48	7.334	1930	1942	1963	rBV	672219	1159565	80.95%	9.174%
49	7.640	2025	2037	2053	rBV	141214	240021	16.76%	1.899%
50	7.723	2061	2063	2069	rVB7	2039	1305	0.09%	0.010%
51	7.846	2099	2101	2104	rBV4	1423	817	0.06%	0.006%
52	7.891	2113	2115	2117	rBV2	1133	578	0.04%	0.005%
53	7.952	2130	2134	2136	rBV4	1085	821	0.06%	0.006%
54	7.994	2144	2147	2148	rBV4	1560	1013	0.07%	0.008%
55	8.109	2172	2183	2216	rBV	369727	755394	52.73%	5.976%
56	8.617	2339	2341	2343	rBV3	1207	594	0.04%	0.005%
57	8.794	2393	2396	2398	rBV4	1598	902	0.06%	0.007%
58	8.871	2409	2420	2440	rBV	662320	1074341	75.00%	8.500%
59	9.116	2494	2496	2499	rBV3	1556	642	0.04%	0.005%
60	9.328	2560	2562	2565	rVB4	1508	712	0.05%	0.006%
61	9.344	2565	2567	2570	rBV4	1437	942	0.07%	0.007%
62	9.405	2583	2586	2590	rBV5	1244	888	0.06%	0.007%
63	9.502	2613	2616	2619	rBV5	1842	1431	0.10%	0.011%
64	9.543	2628	2629	2632	rVB3	1423	573	0.04%	0.005%
65	9.569	2634	2637	2639	rVV4	1223	700	0.05%	0.006%
66	9.727	2674	2686	2687	rBV10	2852	4582	0.32%	0.036%
67	9.781	2701	2703	2706	rBV3	1622	1163	0.08%	0.009%
68	9.958	2756	2758	2761	rVB3	1873	968	0.07%	0.008%
69	9.977	2761	2764	2766	rBV3	1515	810	0.06%	0.006%
70	10.038	2781	2783	2786	rVB2	1962	1100	0.08%	0.009%
71	10.067	2790	2792	2795	rVB4	917	478	0.03%	0.004%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061020\
 Data File : VV016764.D
 Acq On : 10 Jun 2020 13:15
 Operator : SY/MD
 Sample : L2901-22DL 5X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTS3DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

72	10.084	2795	2797	2798	rBV2	1076	411	0.03%	0.003%
73	10.106	2802	2804	2806	rBV3	925	467	0.03%	0.004%
74	10.238	2832	2845	2860	rBV	445887	708474	49.46%	5.605%
75	10.389	2888	2892	2893	rBV3	1882	1045	0.07%	0.008%
76	10.463	2912	2915	2918	rVB5	3084	1989	0.14%	0.016%
77	10.482	2918	2921	2924	rBV5	2191	1647	0.11%	0.013%
78	10.527	2929	2935	2938	rBV8	1358	1511	0.11%	0.012%
79	10.592	2952	2955	2956	rBV3	1764	1186	0.08%	0.009%
80	10.669	2977	2979	2981	rBV3	910	410	0.03%	0.003%
81	10.752	3003	3005	3008	rBV3	1884	1258	0.09%	0.010%
82	10.823	3025	3027	3029	rBV3	1582	768	0.05%	0.006%
83	10.865	3037	3040	3042	rBV4	1587	880	0.06%	0.007%
84	11.064	3095	3102	3110	rBV4	4232	6313	0.44%	0.050%
85	11.270	3155	3166	3183	rBV	740576	1137727	79.42%	9.001%
86	11.402	3202	3207	3208	rBV4	1518	1535	0.11%	0.012%
87	11.427	3213	3215	3219	rBV4	1638	1259	0.09%	0.010%
88	11.646	3272	3283	3296	rBV	761260	1199557	83.74%	9.490%
89	11.833	3340	3341	3344	rVB3	2867	1179	0.08%	0.009%
90	11.852	3344	3347	3348	rBV2	1833	1004	0.07%	0.008%
91	12.009	3394	3396	3400	rBV4	1457	1189	0.08%	0.009%
92	12.058	3409	3411	3413	rBV3	1571	575	0.04%	0.005%
93	12.347	3498	3501	3503	rBV3	1894	1351	0.09%	0.011%
94	12.624	3584	3587	3588	rBV2	1272	549	0.04%	0.004%
95	12.997	3701	3703	3707	rVB5	1516	1032	0.07%	0.008%
96	13.225	3771	3774	3778	rBV6	1182	1101	0.08%	0.009%
97	13.337	3806	3809	3811	rBV4	2024	1200	0.08%	0.009%
98	13.765	3939	3942	3943	rBV3	2241	1315	0.09%	0.010%
99	13.807	3954	3955	3957	rBV2	1435	663	0.05%	0.005%
100	13.871	3973	3975	3976	rBV2	1672	647	0.05%	0.005%


Sum of corrected areas: 12639657

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV061020\
Data File : VV016764.D
Acq On : 10 Jun 2020 13:15
Operator : SY/MD
Sample : L2901-22DL 5X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTS3DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

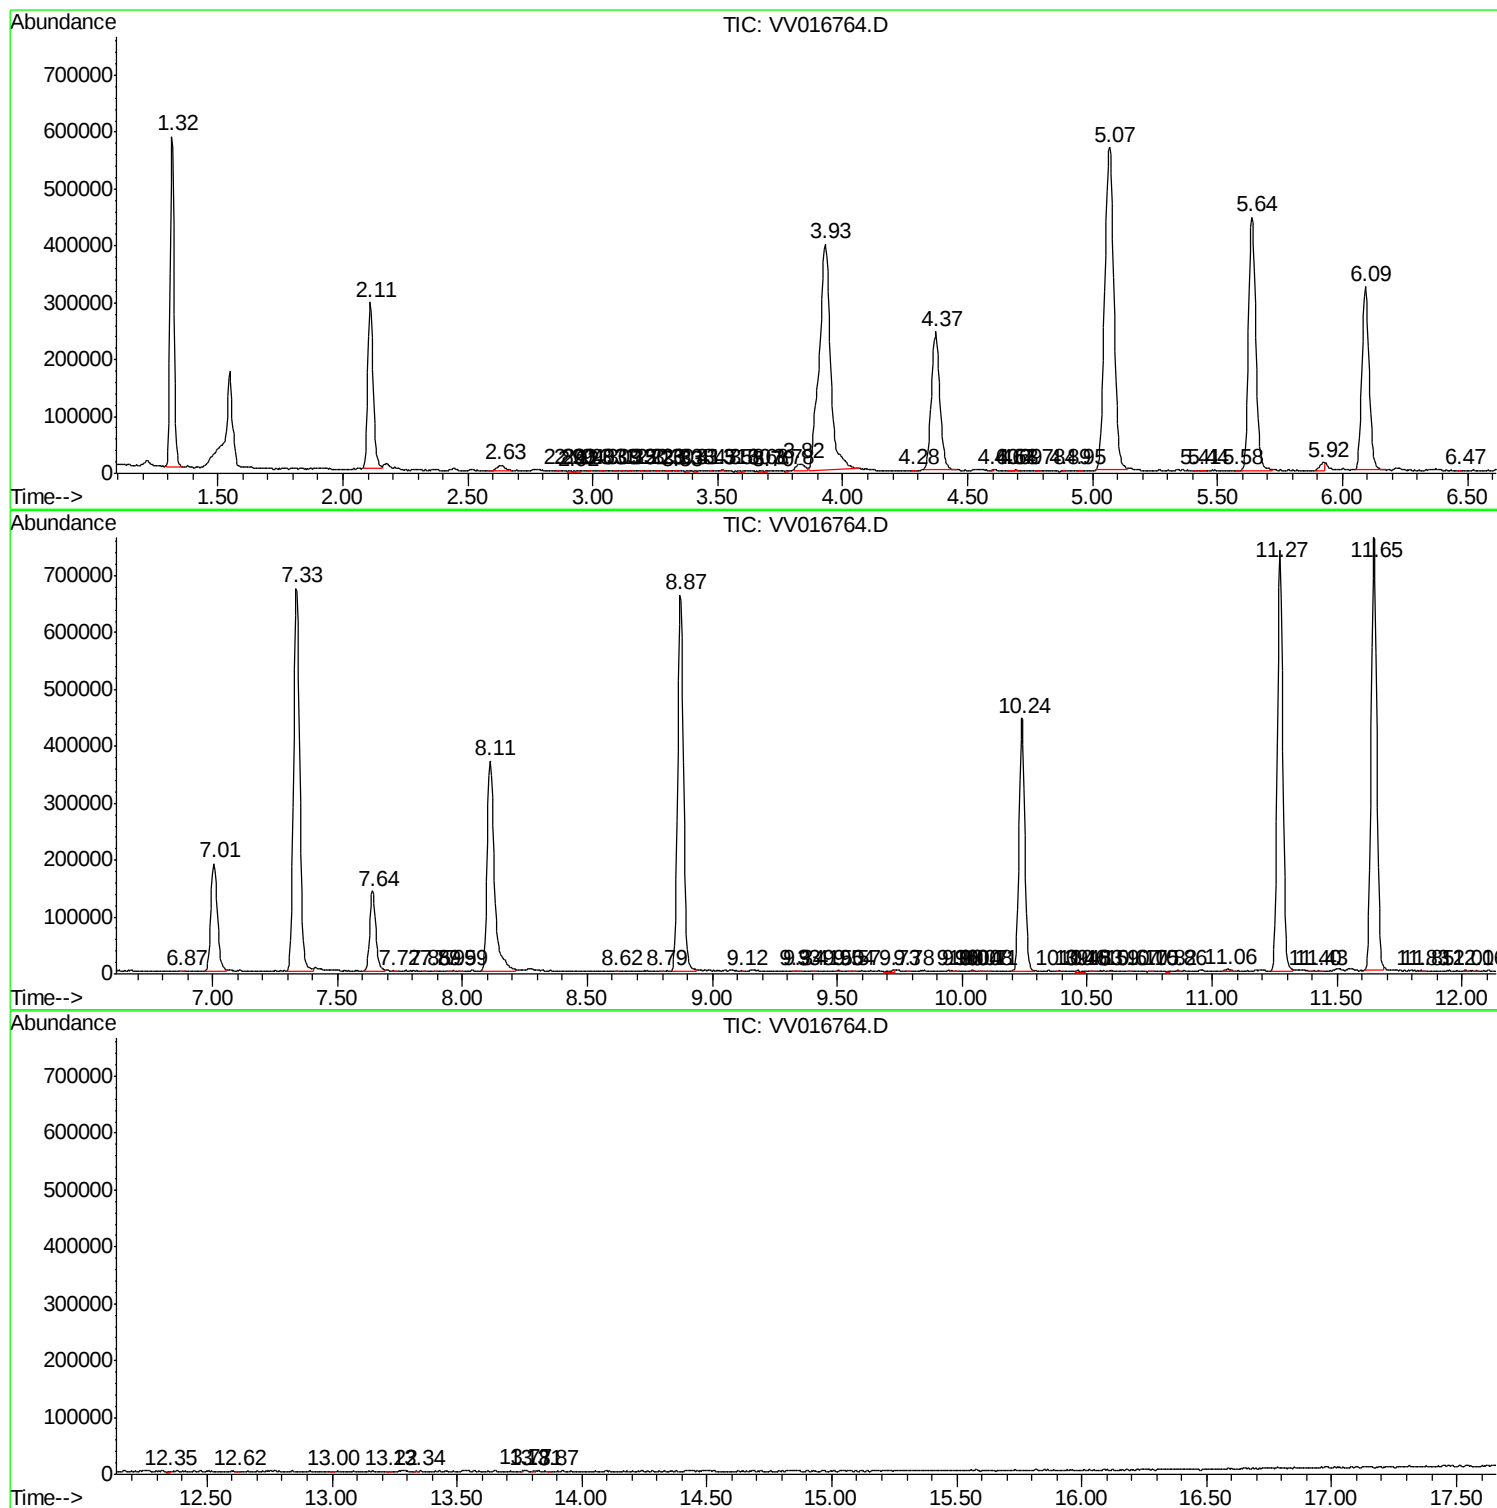

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV061020\
Data File : VV016764.D
Acq On : 10 Jun 2020 13:15
Operator : SY/MD
Sample : L2901-22DL 5X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTS3DL

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV061020\
Data File : VV016764.D
Acq On : 10 Jun 2020 13:15
Operator : SY/MD
Sample : L2901-22DL 5X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTS3DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc