

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061020\
 Data File : VV016769.D
 Acq On : 10 Jun 2020 15:15
 Operator : SY/MD
 Sample : L2914-12DL 500X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9E15DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.316	63	70	81	rVB	195847	198344	14.85%	1.802%
2	1.557	139	145	159	rVB	116557	145715	10.91%	1.324%
3	2.116	309	319	331	rBV	277872	415201	31.09%	3.772%
4	2.377	396	400	403	rBV5	1966	1864	0.14%	0.017%
5	2.714	504	505	508	rVB2	1293	572	0.04%	0.005%
6	2.730	508	510	513	rBV4	1020	622	0.05%	0.006%
7	2.820	536	538	541	rVB4	1832	864	0.06%	0.008%
8	2.843	542	545	546	rBV3	1003	550	0.04%	0.005%
9	3.000	592	594	596	rBV2	1562	859	0.06%	0.008%
10	3.036	602	605	607	rBV4	1388	1052	0.08%	0.010%
11	3.103	620	626	627	rBV4	1543	1476	0.11%	0.013%
12	3.151	639	641	644	rVV3	1711	840	0.06%	0.008%
13	3.229	661	665	669	rBV8	2045	1883	0.14%	0.017%
14	3.528	751	758	763	rBV9	1648	2187	0.16%	0.020%
15	3.579	771	774	777	rBV4	1342	757	0.06%	0.007%
16	3.598	777	780	782	rBV5	1575	980	0.07%	0.009%
17	3.637	789	792	796	rBV5	2158	1455	0.11%	0.013%
18	3.894	861	872	902	rBV	110678	308253	23.08%	2.800%
19	4.225	972	975	978	rBV4	1886	1227	0.09%	0.011%
20	4.373	1006	1021	1042	rBV	224548	543233	40.68%	4.935%
21	4.524	1066	1068	1070	rVV3	1426	543	0.04%	0.005%
22	4.540	1071	1073	1079	rVB6	2317	1945	0.15%	0.018%
23	4.576	1082	1084	1089	rBV5	858	613	0.05%	0.006%
24	4.608	1092	1094	1096	rBV3	2145	1306	0.10%	0.012%
25	4.692	1110	1120	1122	rBV9	4135	5796	0.43%	0.053%
26	4.859	1169	1172	1175	rVB5	1110	747	0.06%	0.007%
27	4.926	1189	1193	1197	rBV5	1754	1644	0.12%	0.015%
28	4.975	1207	1208	1212	rVB4	981	614	0.05%	0.006%
29	5.068	1219	1237	1245	rBV2	542105	1335319	100.00%	12.131%
30	5.592	1397	1400	1401	rBV3	2279	1187	0.09%	0.011%
31	5.640	1402	1415	1435	rVV	440347	883929	66.20%	8.030%
32	5.926	1491	1504	1516	rBV4	18128	40865	3.06%	0.371%
33	6.090	1543	1555	1574	rVB	301983	608156	45.54%	5.525%
34	6.196	1585	1588	1591	rBV5	1979	1287	0.10%	0.012%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061020\
 Data File : VV016769.D
 Acq On : 10 Jun 2020 15:15
 Operator : SY/MD
 Sample : L2914-12DL 500X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9E15DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

35	6.386	1644	1647	1649	rBV4	1688	1150	0.09%	0.010%
36	6.425	1657	1659	1662	rBV4	1451	1028	0.08%	0.009%
37	6.528	1689	1691	1695	rBV4	1528	1195	0.09%	0.011%
38	6.576	1704	1706	1709	rBV4	1376	868	0.07%	0.008%
39	6.701	1741	1745	1750	rBV8	1348	1177	0.09%	0.011%
40	6.756	1759	1762	1765	rBV5	1212	874	0.07%	0.008%
41	6.843	1787	1789	1792	rBV4	1283	710	0.05%	0.006%
42	6.875	1795	1799	1803	rBV7	1862	1428	0.11%	0.013%
43	6.949	1817	1822	1825	rBV7	2579	2473	0.19%	0.022%
44	7.007	1828	1840	1855	rBV	178961	322393	24.14%	2.929%
45	7.084	1862	1864	1867	rBV4	1965	1101	0.08%	0.010%
46	7.338	1927	1943	1956	rBV	640009	1099551	82.34%	9.989%
47	7.412	1958	1966	1984	rVB	95995	175837	13.17%	1.597%
48	7.640	2028	2037	2049	rBV	126875	211992	15.88%	1.926%
49	7.981	2141	2143	2147	rBV5	795	613	0.05%	0.006%
50	8.007	2147	2151	2153	rBV4	1894	1482	0.11%	0.013%
51	8.106	2172	2182	2213	rBV2	320287	628391	47.06%	5.709%
52	8.499	2301	2304	2306	rBV3	1406	862	0.06%	0.008%
53	8.608	2335	2338	2341	rVB4	1343	717	0.05%	0.007%
54	8.650	2349	2351	2355	rBV4	1555	1235	0.09%	0.011%
55	8.717	2370	2372	2378	rVB6	1447	1072	0.08%	0.010%
56	8.762	2383	2386	2387	rBV3	1073	697	0.05%	0.006%
57	8.823	2402	2405	2407	rBV3	772	641	0.05%	0.006%
58	8.871	2409	2420	2444	rVV	663342	1083813	81.17%	9.846%
59	9.035	2462	2471	2486	rVB	61375	97049	7.27%	0.882%
60	9.225	2527	2530	2532	rBV4	1231	758	0.06%	0.007%
61	9.389	2577	2581	2582	rBV4	1359	801	0.06%	0.007%
62	9.569	2629	2637	2645	rBV3	9036	14435	1.08%	0.131%
63	9.781	2701	2703	2706	rBV4	1389	648	0.05%	0.006%
64	9.952	2749	2756	2757	rBV7	2940	3086	0.23%	0.028%
65	10.090	2793	2799	2800	rBV5	1769	1767	0.13%	0.016%
66	10.142	2809	2815	2817	rBV7	1606	1631	0.12%	0.015%
67	10.238	2834	2845	2860	rBV	398831	624900	46.80%	5.677%
68	10.540	2936	2939	2940	rBV4	1587	844	0.06%	0.008%
69	10.646	2970	2972	2977	rVB4	2733	2152	0.16%	0.020%
70	10.711	2987	2992	2994	rBV6	1197	1445	0.11%	0.013%
71	10.733	2997	2999	3001	rBV3	1230	594	0.04%	0.005%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061020\
 Data File : VV016769.D
 Acq On : 10 Jun 2020 15:15
 Operator : SY/MD
 Sample : L2914-12DL 500X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9E15DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

72	10.759	3001	3007	3009	rBV6	3360	3311	0.25%	0.030%
73	10.842	3027	3033	3034	rBV6	2019	1851	0.14%	0.017%
74	10.984	3073	3077	3080	rBV5	2073	1724	0.13%	0.016%
75	11.055	3093	3099	3103	rBV6	2260	2074	0.16%	0.019%
76	11.270	3155	3166	3179	rBV	709328	1080414	80.91%	9.815%
77	11.540	3244	3250	3252	rBV7	2281	2345	0.18%	0.021%
78	11.585	3262	3264	3265	rBV2	1343	600	0.04%	0.005%
79	11.646	3271	3283	3300	rBV	695869	1086558	81.37%	9.871%
80	11.842	3342	3344	3347	rBV4	1288	786	0.06%	0.007%
81	11.926	3367	3370	3376	rBV6	2064	1728	0.13%	0.016%
82	12.084	3417	3419	3426	rVB7	1950	1672	0.13%	0.015%
83	12.122	3426	3431	3433	rBV5	2028	1928	0.14%	0.018%
84	12.238	3463	3467	3470	rBV5	1791	1438	0.11%	0.013%
85	12.257	3470	3473	3475	rBV3	1204	639	0.05%	0.006%
86	12.431	3525	3527	3528	rBV2	1594	662	0.05%	0.006%
87	12.489	3541	3545	3547	rBV4	2187	1522	0.11%	0.014%
88	12.842	3653	3655	3658	rVB3	1677	733	0.05%	0.007%
89	12.942	3684	3686	3688	rBV3	1481	601	0.05%	0.005%
90	12.997	3700	3703	3709	rBV7	2033	1777	0.13%	0.016%
91	13.026	3709	3712	3715	rBV4	1069	762	0.06%	0.007%
92	13.219	3770	3772	3776	rVB4	1379	703	0.05%	0.006%
93	13.614	3893	3895	3898	rBV3	1742	790	0.06%	0.007%
94	13.646	3901	3905	3908	rBV7	1551	1450	0.11%	0.013%
95	13.698	3917	3921	3924	rBV4	1605	1535	0.11%	0.014%
96	14.016	4013	4020	4021	rBV6	2144	1971	0.15%	0.018%
97	14.209	4076	4080	4081	rBV4	1713	1012	0.08%	0.009%
98	14.537	4180	4182	4186	rBV4	1183	1012	0.08%	0.009%
99	14.579	4193	4195	4199	rBV4	1953	1327	0.10%	0.012%
100	14.781	4255	4258	4259	rBV3	2122	1066	0.08%	0.010%


Sum of corrected areas: 11007286

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV061020\
Data File : VV016769.D
Acq On : 10 Jun 2020 15:15
Operator : SY/MD
Sample : L2914-12DL 500X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9E15DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

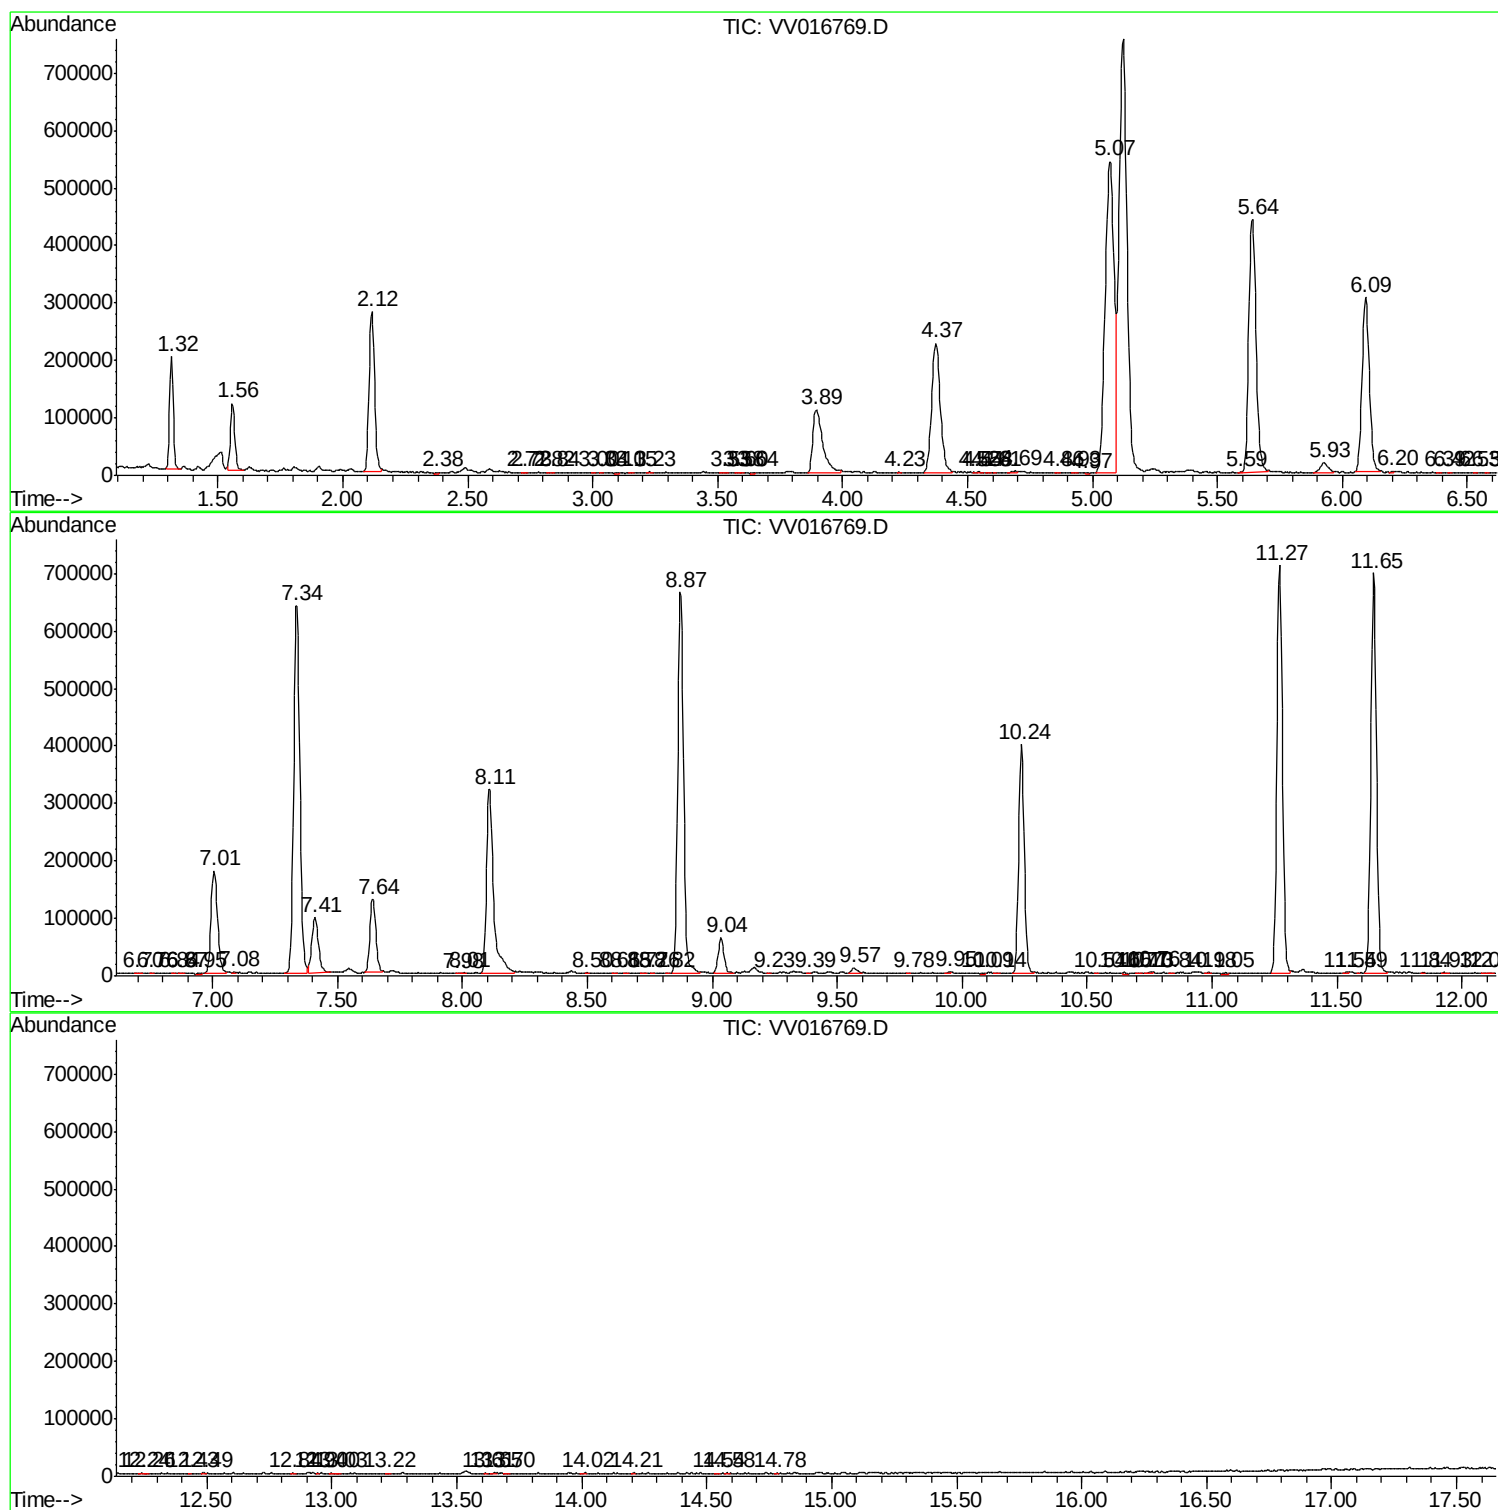

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV061020\
Data File : VV016769.D
Acq On : 10 Jun 2020 15:15
Operator : SY/MD
Sample : L2914-12DL 500X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9E15DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV061020\
Data File : VV016769.D
Acq On : 10 Jun 2020 15:15
Operator : SY/MD
Sample : L2914-12DL 500X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9E15DL

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc