

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061020\
 Data File : VV016772.D
 Acq On : 10 Jun 2020 16:26
 Operator : SY/MD
 Sample : L2914-03DL 50X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9D96DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.312	62	69	80	rVB	211669	217235	17.20%	1.963%
2	1.553	138	144	157	rVB	110790	140078	11.09%	1.265%
3	2.113	310	318	333	rVB	260531	380470	30.13%	3.437%
4	2.431	415	417	418	rBV	1617	655	0.05%	0.006%
5	2.701	498	501	505	rBV4	1382	1181	0.09%	0.011%
6	2.766	516	521	522	rBV5	1804	1532	0.12%	0.014%
7	2.820	536	538	540	rBV3	1244	477	0.04%	0.004%
8	2.923	565	570	573	rBV5	1526	1292	0.10%	0.012%
9	3.036	602	605	608	rBV4	1727	1170	0.09%	0.011%
10	3.129	631	634	635	rBV3	1006	472	0.04%	0.004%
11	3.193	651	654	655	rBV2	1102	712	0.06%	0.006%
12	3.238	662	668	672	rVB8	2317	2341	0.19%	0.021%
13	3.254	672	673	676	rBV3	1206	529	0.04%	0.005%
14	3.303	686	688	691	rVB4	1180	684	0.05%	0.006%
15	3.315	691	692	694	rBV2	1395	725	0.06%	0.007%
16	3.335	697	698	701	rBV2	1226	595	0.05%	0.005%
17	3.380	708	712	715	rBV6	1032	942	0.07%	0.009%
18	3.418	719	724	726	rBV5	1404	1263	0.10%	0.011%
19	3.447	726	733	736	rBV6	3833	4020	0.32%	0.036%
20	3.499	746	749	751	rBV4	1195	901	0.07%	0.008%
21	3.566	768	770	771	rBV2	1049	423	0.03%	0.004%
22	3.595	776	779	782	rBV5	1632	1299	0.10%	0.012%
23	3.611	782	784	786	rBV3	1088	545	0.04%	0.005%
24	3.643	791	794	795	rBV3	931	549	0.04%	0.005%
25	3.701	808	812	814	rBV4	1949	1648	0.13%	0.015%
26	3.733	820	822	824	rVB2	781	426	0.03%	0.004%
27	3.749	824	827	829	rBV3	1808	1316	0.10%	0.012%
28	3.897	862	873	899	rBV	104032	291225	23.06%	2.631%
29	4.232	975	977	982	rVB5	1721	977	0.08%	0.009%
30	4.302	997	999	1002	rVB3	1569	763	0.06%	0.007%
31	4.373	1002	1021	1042	rBV2	215490	538726	42.66%	4.867%
32	4.544	1071	1074	1075	rBV3	890	414	0.03%	0.004%
33	4.624	1097	1099	1104	rVB5	1632	1349	0.11%	0.012%
34	4.647	1104	1106	1109	rBV3	1659	1100	0.09%	0.010%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061020\
 Data File : VV016772.D
 Acq On : 10 Jun 2020 16:26
 Operator : SY/MD
 Sample : L2914-03DL 50X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9D96DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

35	4.701	1114	1123	1132	rVV3	7505	15959	1.26%	0.144%
36	4.791	1148	1151	1153	rVV4	1156	651	0.05%	0.006%
37	4.804	1153	1155	1158	rVB4	1304	584	0.05%	0.005%
38	4.884	1178	1180	1182	rBV3	1161	531	0.04%	0.005%
39	4.920	1189	1191	1192	rBV2	1747	697	0.06%	0.006%
40	4.962	1198	1204	1205	rBV5	1364	1018	0.08%	0.009%
41	5.071	1221	1238	1244	rBV2	523972	1262867	100.00%	11.409%
42	5.640	1400	1415	1434	rBV	421408	847045	67.07%	7.652%
43	5.852	1480	1481	1485	rVB4	1769	698	0.06%	0.006%
44	5.926	1496	1504	1515	rBV3	12493	25429	2.01%	0.230%
45	6.032	1536	1537	1540	rBV3	922	606	0.05%	0.005%
46	6.093	1541	1556	1574	rVV	293968	599988	47.51%	5.420%
47	6.376	1640	1644	1648	rBV6	1604	1336	0.11%	0.012%
48	6.511	1683	1686	1689	rVB5	2163	1390	0.11%	0.013%
49	6.544	1689	1696	1698	rBV7	1980	2224	0.18%	0.020%
50	6.598	1709	1713	1715	rBV4	1992	1503	0.12%	0.014%
51	6.643	1725	1727	1730	rVB4	1302	700	0.06%	0.006%
52	6.659	1730	1732	1735	rBV3	1508	1233	0.10%	0.011%
53	6.717	1748	1750	1753	rVB4	1380	629	0.05%	0.006%
54	6.765	1763	1765	1766	rBV2	1373	623	0.05%	0.006%
55	6.817	1776	1781	1784	rBV7	1689	1581	0.13%	0.014%
56	6.862	1792	1795	1798	rBV4	2020	1303	0.10%	0.012%
57	6.900	1805	1807	1809	rBV3	1397	768	0.06%	0.007%
58	6.936	1817	1818	1821	rVB3	1255	529	0.04%	0.005%
59	6.952	1821	1823	1825	rBV2	1174	608	0.05%	0.005%
60	7.007	1829	1840	1857	rBV	174323	307068	24.32%	2.774%
61	7.090	1863	1866	1869	rBV4	1670	1317	0.10%	0.012%
62	7.338	1931	1943	1955	rBV	625454	1070632	84.78%	9.672%
63	7.408	1958	1965	1985	rVB	174237	302853	23.98%	2.736%
64	7.640	2029	2037	2054	rVB	124031	200424	15.87%	1.811%
65	7.868	2106	2108	2111	rVB3	1961	1142	0.09%	0.010%
66	7.916	2121	2123	2127	rVB4	1642	1053	0.08%	0.010%
67	7.971	2136	2140	2144	rVB5	2189	1820	0.14%	0.016%
68	8.106	2172	2182	2209	rBV	314759	594460	47.07%	5.370%
69	8.392	2269	2271	2274	rBV4	1547	827	0.07%	0.007%
70	8.447	2286	2288	2292	rBV6	1875	1285	0.10%	0.012%
71	8.482	2297	2299	2301	rBV2	1142	573	0.05%	0.005%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061020\
 Data File : VV016772.D
 Acq On : 10 Jun 2020 16:26
 Operator : SY/MD
 Sample : L2914-03DL 50X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9D96DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

72	8.540	2313	2317	2319	rBV4	1763	1290	0.10%	0.012%
73	8.572	2324	2327	2329	rBV3	988	421	0.03%	0.004%
74	8.695	2363	2365	2367	rBV2	773	407	0.03%	0.004%
75	8.871	2410	2420	2431	rBV	632498	1015162	80.39%	9.171%
76	9.032	2461	2470	2486	rBV	182417	295076	23.37%	2.666%
77	9.283	2540	2548	2556	rBV	11456	20309	1.61%	0.183%
78	9.566	2628	2636	2648	rVB	49542	76772	6.08%	0.694%
79	9.785	2702	2704	2705	rBV2	2173	958	0.08%	0.009%
80	10.238	2834	2845	2858	rBV	398153	624478	49.45%	5.642%
81	11.270	3155	3166	3181	rBV	693986	1052399	83.33%	9.507%
82	11.646	3272	3283	3306	rVB	687536	1088220	86.17%	9.831%
83	12.122	3421	3431	3435	rBV	4476	8161	0.65%	0.074%
84	12.241	3466	3468	3473	rBV4	1481	1568	0.12%	0.014%
85	12.312	3486	3490	3492	rBV5	1967	1699	0.13%	0.015%
86	12.428	3521	3526	3527	rBV5	1900	1424	0.11%	0.013%
87	12.656	3595	3597	3598	rBV2	1101	453	0.04%	0.004%
88	12.672	3598	3602	3606	rBV6	2647	2553	0.20%	0.023%
89	12.733	3619	3621	3624	rBV3	1087	602	0.05%	0.005%
90	13.177	3754	3759	3763	rBV7	2423	2319	0.18%	0.021%
91	13.251	3780	3782	3784	rBV3	1192	552	0.04%	0.005%
92	13.527	3862	3868	3878	rVB4	8226	15054	1.19%	0.136%
93	13.852	3968	3969	3972	rBV2	972	488	0.04%	0.004%
94	13.871	3973	3975	3979	rVV4	1581	1071	0.08%	0.010%
95	13.948	3997	3999	4001	rBV3	1288	760	0.06%	0.007%
96	14.100	4043	4046	4048	rBV3	968	620	0.05%	0.006%
97	14.157	4062	4064	4067	rBV4	1496	946	0.07%	0.009%
98	14.280	4099	4102	4105	rBV5	1819	1608	0.13%	0.015%
99	14.437	4149	4151	4153	rBV3	1656	951	0.08%	0.009%
100	14.672	4221	4224	4225	rBV3	1373	928	0.07%	0.008%


Sum of corrected areas: 11069237

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV061020\
Data File : VV016772.D
Acq On : 10 Jun 2020 16:26
Operator : SY/MD
Sample : L2914-03DL 50X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9D96DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

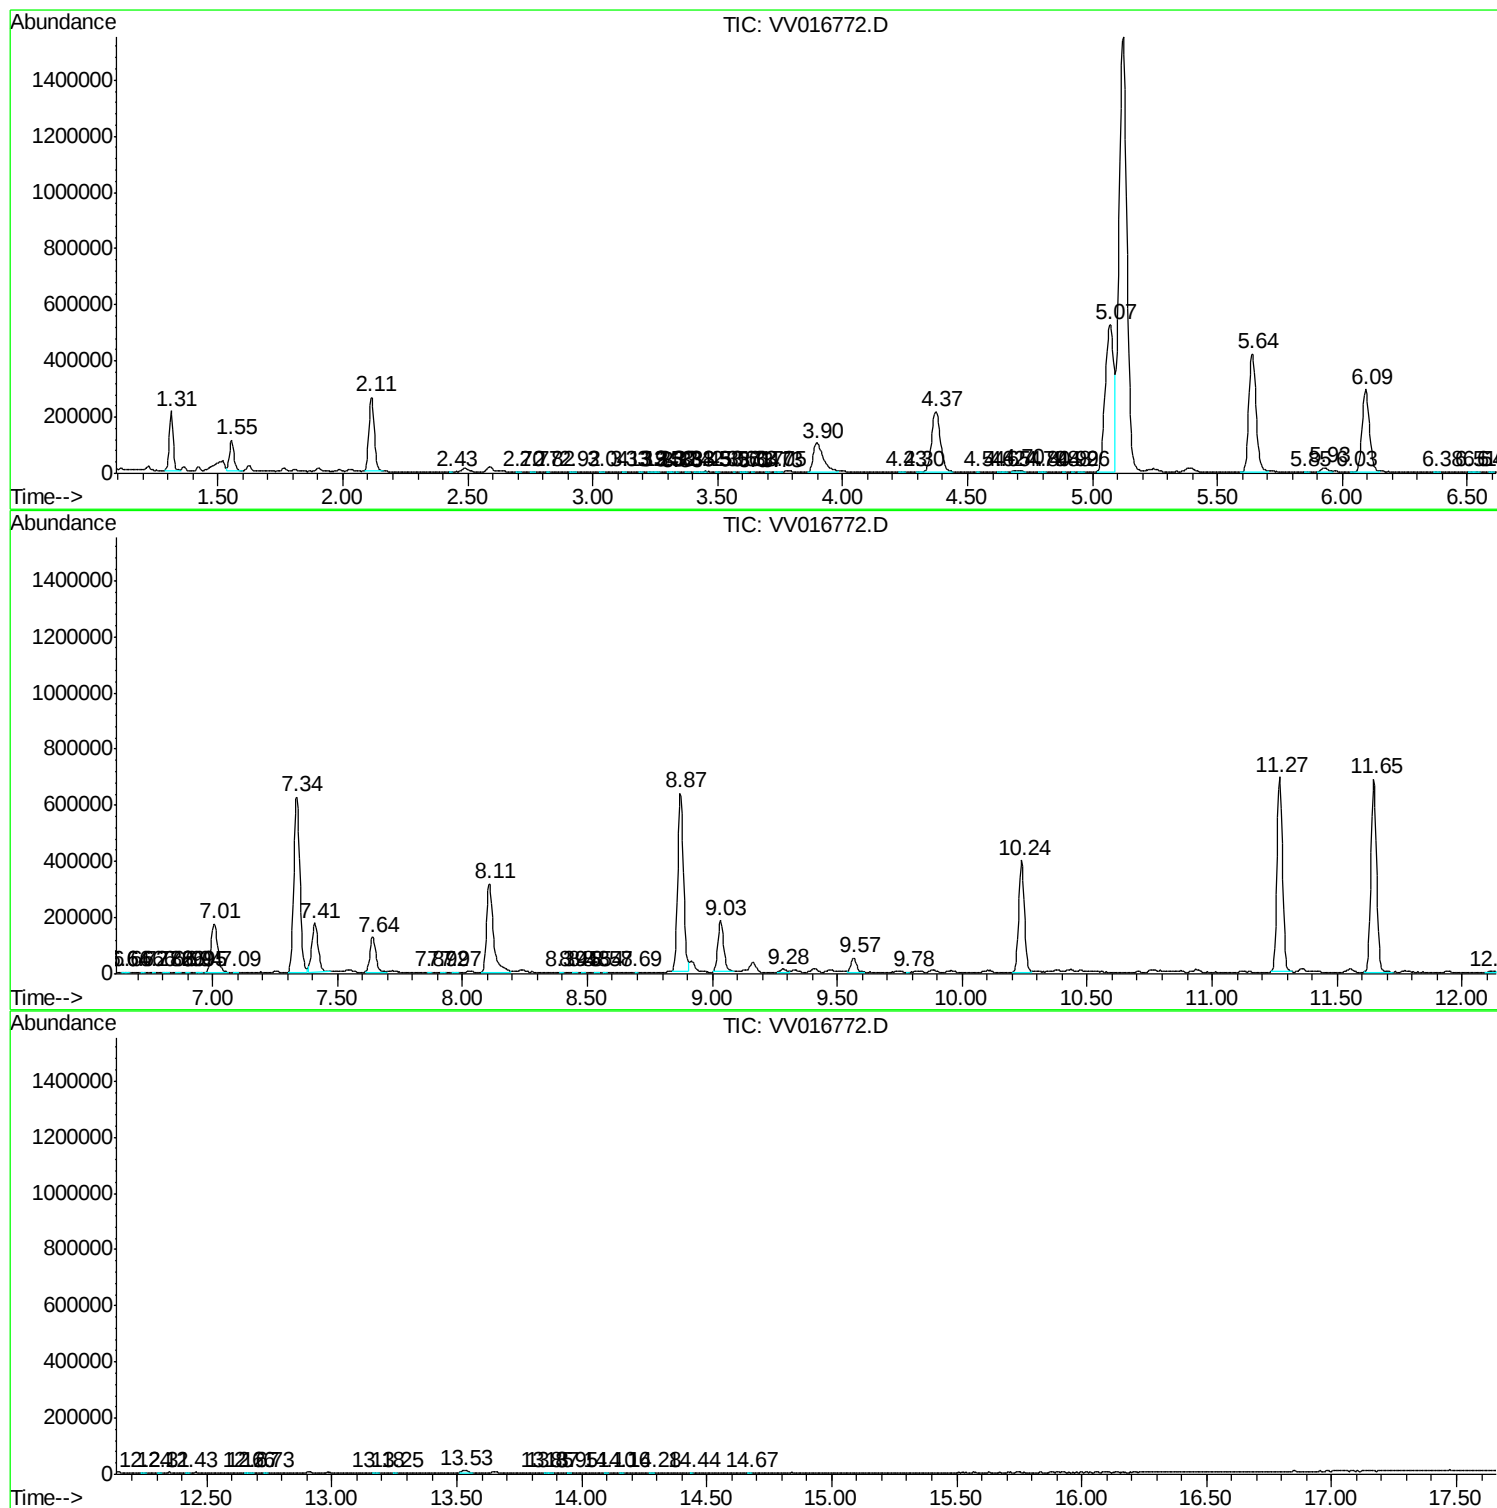

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV061020\
Data File : VV016772.D
Acq On : 10 Jun 2020 16:26
Operator : SY/MD
Sample : L2914-03DL 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9D96DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV061020\
Data File : VV016772.D
Acq On : 10 Jun 2020 16:26
Operator : SY/MD
Sample : L2914-03DL 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9D96DL

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc