

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061020\
 Data File : VV016780.D
 Acq On : 10 Jun 2020 19:37
 Operator : SY/MD
 Sample : L2901-03DL 200X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTR3DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.316	63	70	81	rVB2	253183	258920	19.48%	2.371%
2	1.557	139	145	157	rVB	111589	136108	10.24%	1.246%
3	2.113	310	318	337	rVB	265532	395864	29.79%	3.625%
4	2.370	394	398	401	rBV5	2086	1745	0.13%	0.016%
5	2.479	427	432	433	rBV5	1088	881	0.07%	0.008%
6	2.553	452	455	457	rBV4	1365	668	0.05%	0.006%
7	2.817	535	537	541	rVB3	2265	1598	0.12%	0.015%
8	2.849	545	547	549	rBV3	1423	736	0.06%	0.007%
9	2.926	567	571	573	rBV5	1686	1344	0.10%	0.012%
10	3.094	620	623	627	rBV6	1369	1123	0.08%	0.010%
11	3.148	638	640	644	rVB3	2075	1257	0.09%	0.012%
12	3.177	644	649	651	rBV5	1672	937	0.07%	0.009%
13	3.264	673	676	678	rBV3	1128	850	0.06%	0.008%
14	3.409	717	721	722	rBV3	1151	830	0.06%	0.008%
15	3.441	729	731	733	rBV3	1528	860	0.06%	0.008%
16	3.541	760	762	765	rVB4	1391	703	0.05%	0.006%
17	3.711	813	815	820	rVB4	1356	836	0.06%	0.008%
18	3.759	827	830	831	rBV2	1349	731	0.06%	0.007%
19	3.801	841	843	847	rVB4	1837	1214	0.09%	0.011%
20	3.827	847	851	853	rBV3	1493	1038	0.08%	0.010%
21	3.846	853	857	859	rBV4	1212	1020	0.08%	0.009%
22	3.930	862	883	907	rBV2	237697	817999	61.55%	7.490%
23	4.370	1004	1020	1042	rBV	213848	533151	40.12%	4.882%
24	4.727	1127	1131	1133	rBV3	1515	1253	0.09%	0.011%
25	5.068	1221	1237	1259	rBV2	524203	1328921	100.00%	12.168%
26	5.418	1341	1346	1348	rBV5	2749	1846	0.14%	0.017%
27	5.637	1401	1414	1434	rBV	422849	844021	63.51%	7.728%
28	5.891	1491	1493	1494	rBV2	1781	731	0.06%	0.007%
29	6.010	1528	1530	1534	rVB4	1608	783	0.06%	0.007%
30	6.090	1542	1555	1580	rVB	296379	604204	45.47%	5.532%
31	6.534	1691	1693	1696	rBV3	1475	801	0.06%	0.007%
32	6.737	1755	1756	1760	rBV4	1055	743	0.06%	0.007%
33	6.801	1768	1776	1779	rBV8	1643	2025	0.15%	0.019%
34	6.820	1779	1782	1786	rBV4	1432	987	0.07%	0.009%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061020\
 Data File : VV016780.D
 Acq On : 10 Jun 2020 19:37
 Operator : SY/MD
 Sample : L2901-03DL 200X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTR3DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

35	6.897	1803	1806	1809	rVB4	1423	1077	0.08%	0.010%
36	6.949	1819	1822	1826	rBV4	1530	1064	0.08%	0.010%
37	7.007	1829	1840	1862	rVV	175999	308197	23.19%	2.822%
38	7.161	1886	1888	1891	rVB3	1826	916	0.07%	0.008%
39	7.335	1931	1942	1958	rBV	622356	1063757	80.05%	9.740%
40	7.640	2027	2037	2050	rBV2	121742	203973	15.35%	1.868%
41	7.929	2124	2127	2128	rBV3	1583	1028	0.08%	0.009%
42	8.106	2172	2182	2210	rVV2	316775	615114	46.29%	5.632%
43	8.566	2321	2325	2328	rVB6	2056	1354	0.10%	0.012%
44	8.601	2333	2336	2338	rVB3	2184	1113	0.08%	0.010%
45	8.627	2338	2344	2349	rBV9	1803	2408	0.18%	0.022%
46	8.672	2356	2358	2361	rBV3	1570	858	0.06%	0.008%
47	8.753	2379	2383	2384	rBV4	1667	897	0.07%	0.008%
48	8.791	2393	2395	2401	rVB5	1564	1263	0.10%	0.012%
49	8.871	2409	2420	2438	rBV	632410	1020125	76.76%	9.341%
50	9.029	2467	2469	2472	rBV3	1768	1067	0.08%	0.010%
51	9.138	2501	2503	2505	rBV3	1170	675	0.05%	0.006%
52	9.309	2553	2556	2560	rVB4	2387	1424	0.11%	0.013%
53	9.370	2573	2575	2577	rBV3	1623	841	0.06%	0.008%
54	9.431	2591	2594	2596	rBV3	1037	761	0.06%	0.007%
55	9.466	2603	2605	2609	rBV6	1931	965	0.07%	0.009%
56	9.572	2633	2638	2639	rBV4	1965	1749	0.13%	0.016%
57	9.643	2658	2660	2664	rVB4	1385	954	0.07%	0.009%
58	9.675	2664	2670	2673	rBV7	1697	1633	0.12%	0.015%
59	9.740	2684	2690	2694	rBV7	1517	2092	0.16%	0.019%
60	9.797	2704	2708	2709	rBV4	1312	740	0.06%	0.007%
61	9.843	2717	2722	2724	rBV4	1975	1648	0.12%	0.015%
62	9.910	2740	2743	2746	rBV4	1983	1244	0.09%	0.011%
63	10.087	2794	2798	2801	rBV5	1570	1163	0.09%	0.011%
64	10.122	2807	2809	2811	rBV2	1304	672	0.05%	0.006%
65	10.187	2826	2829	2832	rBV3	1579	1009	0.08%	0.009%
66	10.238	2833	2845	2862	rBV	395631	622461	46.84%	5.700%
67	10.351	2877	2880	2885	rBV6	1834	2162	0.16%	0.020%
68	10.515	2927	2931	2934	rBV5	1567	997	0.08%	0.009%
69	10.669	2974	2979	2980	rBV5	1118	776	0.06%	0.007%
70	10.682	2980	2983	2988	rVV6	1679	1360	0.10%	0.012%
71	11.000	3075	3082	3084	rBV7	2057	2474	0.19%	0.023%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061020\
 Data File : VV016780.D
 Acq On : 10 Jun 2020 19:37
 Operator : SY/MD
 Sample : L2901-03DL 200X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTR3DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

72	11.019	3084	3088	3093	rBV7	1508	1970	0.15%	0.018%
73	11.106	3113	3115	3119	rBV4	1231	1103	0.08%	0.010%
74	11.170	3132	3135	3138	rBV4	2006	1442	0.11%	0.013%
75	11.270	3154	3166	3185	rBV	661328	1010442	76.03%	9.252%
76	11.415	3209	3211	3214	rBV4	1324	734	0.06%	0.007%
77	11.489	3232	3234	3236	rBV3	1860	1091	0.08%	0.010%
78	11.527	3242	3246	3248	rBV3	1708	1409	0.11%	0.013%
79	11.646	3271	3283	3297	rBV	671707	1056784	79.52%	9.677%
80	11.884	3354	3357	3359	rBV3	1226	835	0.06%	0.008%
81	12.026	3399	3401	3405	rVV4	1191	987	0.07%	0.009%
82	12.058	3409	3411	3415	rBV5	1395	1141	0.09%	0.010%
83	12.096	3421	3423	3427	rVB5	1841	1072	0.08%	0.010%
84	12.122	3427	3431	3434	rBV5	1725	1824	0.14%	0.017%
85	12.215	3455	3460	3462	rBV5	2105	1830	0.14%	0.017%
86	12.260	3470	3474	3477	rBV6	2411	1861	0.14%	0.017%
87	12.495	3544	3547	3550	rBV4	1563	1124	0.08%	0.010%
88	12.540	3558	3561	3563	rBV4	1671	1497	0.11%	0.014%
89	12.778	3631	3635	3637	rBV4	1568	1018	0.08%	0.009%
90	12.900	3669	3673	3675	rBV4	2264	1778	0.13%	0.016%
91	13.186	3756	3762	3767	rBV8	2919	3125	0.24%	0.029%
92	13.293	3791	3795	3796	rBV4	1591	1063	0.08%	0.010%
93	13.457	3844	3846	3850	rBV6	1388	909	0.07%	0.008%
94	13.765	3940	3942	3943	rBV2	1623	827	0.06%	0.008%
95	14.055	4029	4032	4034	rBV3	1833	1353	0.10%	0.012%
96	14.501	4168	4171	4174	rBV5	947	746	0.06%	0.007%
97	14.601	4200	4202	4203	rBV2	2049	896	0.07%	0.008%
98	15.051	4340	4342	4346	rBV4	1702	963	0.07%	0.009%
99	15.071	4346	4348	4353	rVV5	1789	1347	0.10%	0.012%
100	15.518	4485	4487	4489	rBV3	2345	1089	0.08%	0.010%


Sum of corrected areas: 10920999

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV061020\
Data File : VV016780.D
Acq On : 10 Jun 2020 19:37
Operator : SY/MD
Sample : L2901-03DL 200X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTR3DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

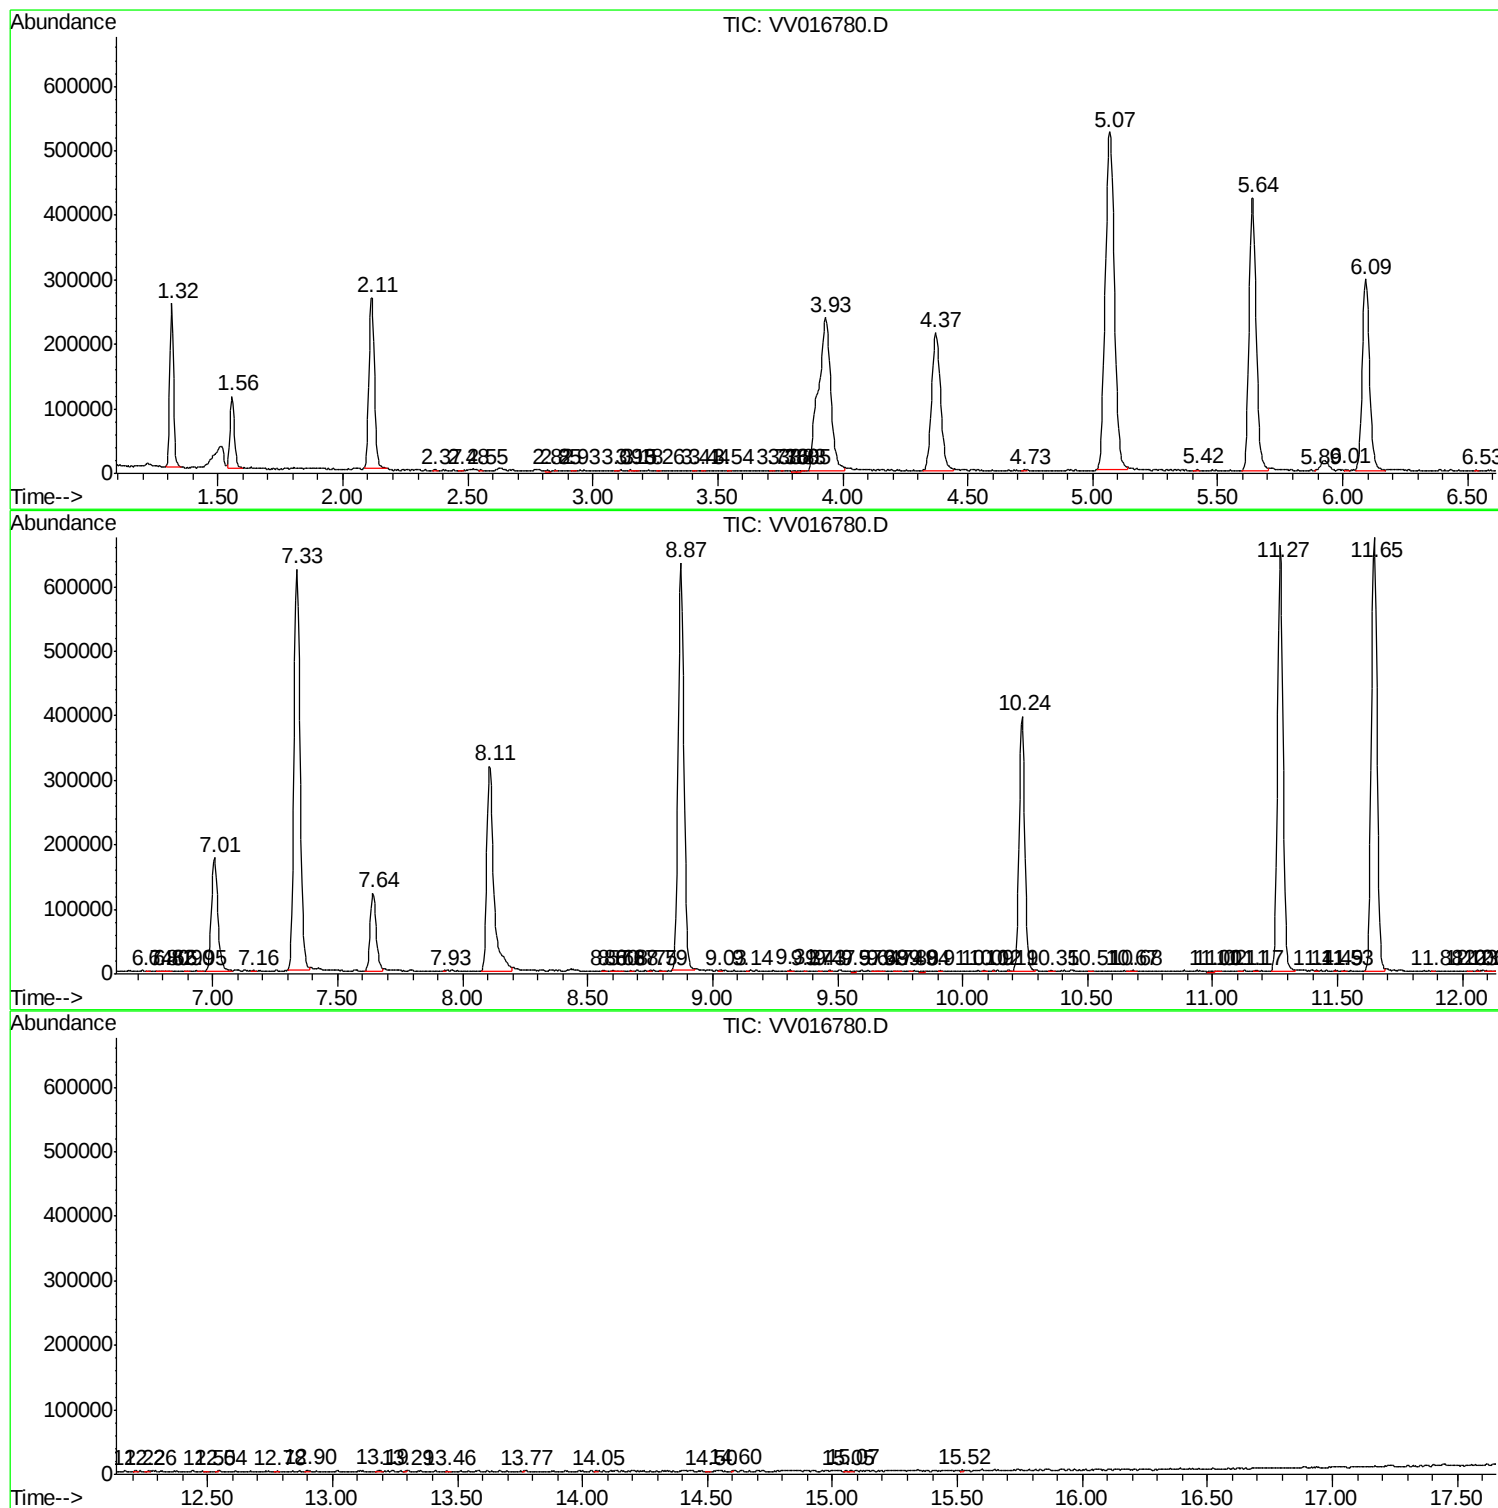

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV061020\
Data File : VV016780.D
Acq On : 10 Jun 2020 19:37
Operator : SY/MD
Sample : L2901-03DL 200X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTR3DL

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV061020\
Data File : VV016780.D
Acq On : 10 Jun 2020 19:37
Operator : SY/MD
Sample : L2901-03DL 200X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTR3DL

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc