

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061020\
 Data File : VV016781.D
 Acq On : 10 Jun 2020 20:01
 Operator : SY/MD
 Sample : L2901-04DL 200X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTR4DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	63	70	81	rVB2	248108	261655	19.51%	2.365%
2	1.560	139	146	157	rVB	113638	138736	10.34%	1.254%
3	2.116	309	319	336	rVB	264698	392681	29.28%	3.550%
4	2.283	369	371	375	rBV5	2010	1338	0.10%	0.012%
5	2.335	384	387	388	rBV3	1324	635	0.05%	0.006%
6	2.695	497	499	500	rBV2	1206	479	0.04%	0.004%
7	2.724	507	508	511	rBV4	1432	633	0.05%	0.006%
8	2.881	554	557	562	rBV6	1301	1054	0.08%	0.010%
9	2.968	580	584	586	rBV4	2785	1730	0.13%	0.016%
10	3.019	597	600	601	rBV3	993	588	0.04%	0.005%
11	3.126	630	633	637	rBV5	1180	926	0.07%	0.008%
12	3.155	637	642	644	rBV5	1519	1117	0.08%	0.010%
13	3.171	644	647	651	rVB5	1663	1324	0.10%	0.012%
14	3.212	657	660	665	rBV6	1439	1756	0.13%	0.016%
15	3.412	720	722	725	rBV3	1161	764	0.06%	0.007%
16	3.463	736	738	742	rBV5	1191	1037	0.08%	0.009%
17	3.521	753	756	758	rBV4	791	537	0.04%	0.005%
18	3.589	776	777	781	rBV3	1106	595	0.04%	0.005%
19	3.782	835	837	840	rBV4	820	530	0.04%	0.005%
20	3.933	862	884	905	rBV3	271428	887971	66.21%	8.027%
21	4.171	956	958	959	rBV2	1123	622	0.05%	0.006%
22	4.251	981	983	986	rBV4	2238	1747	0.13%	0.016%
23	4.306	998	1000	1002	rBV3	1468	605	0.05%	0.005%
24	4.373	1006	1021	1043	rVV	216987	531265	39.61%	4.802%
25	4.566	1078	1081	1084	rBV3	2208	1468	0.11%	0.013%
26	4.659	1108	1110	1113	rBV4	812	480	0.04%	0.004%
27	4.688	1117	1119	1121	rBV3	1195	558	0.04%	0.005%
28	4.833	1161	1164	1165	rVV3	1611	791	0.06%	0.007%
29	4.859	1169	1172	1175	rVB5	1917	998	0.07%	0.009%
30	4.949	1197	1200	1202	rBV3	1156	724	0.05%	0.007%
31	5.068	1220	1237	1259	rBV2	516374	1341191	100.00%	12.124%
32	5.640	1402	1415	1438	rBV	435849	857463	63.93%	7.751%
33	6.093	1538	1556	1577	rBV	301684	610846	45.55%	5.522%
34	6.363	1638	1640	1641	rBV2	1626	714	0.05%	0.006%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061020\
 Data File : VV016781.D
 Acq On : 10 Jun 2020 20:01
 Operator : SY/MD
 Sample : L2901-04DL 200X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTR4DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

35	6.396	1647	1650	1654	rBV3	1236	1166	0.09%	0.011%
36	6.527	1689	1691	1696	rVV6	1213	901	0.07%	0.008%
37	6.653	1728	1730	1733	rBV4	890	489	0.04%	0.004%
38	6.910	1807	1810	1811	rBV3	1067	666	0.05%	0.006%
39	7.006	1828	1840	1857	rBV	175387	308269	22.98%	2.787%
40	7.209	1900	1903	1908	rBV5	1798	1381	0.10%	0.012%
41	7.232	1908	1910	1913	rVB4	1343	770	0.06%	0.007%
42	7.338	1931	1943	1959	rBV	619558	1065662	79.46%	9.633%
43	7.640	2028	2037	2057	rVB	122546	205209	15.30%	1.855%
44	7.904	2115	2119	2121	rBV5	1438	912	0.07%	0.008%
45	8.106	2169	2182	2213	rBV2	307842	605194	45.12%	5.471%
46	8.559	2320	2323	2325	rBV4	1270	956	0.07%	0.009%
47	8.871	2409	2420	2439	rVV	663489	1062617	79.23%	9.606%
48	9.260	2539	2541	2543	rBV3	1577	528	0.04%	0.005%
49	9.318	2557	2559	2560	rBV2	1300	605	0.05%	0.005%
50	9.383	2578	2579	2584	rVB6	1382	996	0.07%	0.009%
51	9.415	2587	2589	2591	rBV2	1051	535	0.04%	0.005%
52	9.482	2607	2610	2612	rBV4	929	501	0.04%	0.005%
53	9.669	2665	2668	2669	rBV3	1124	611	0.05%	0.006%
54	9.752	2692	2694	2696	rBV3	1284	587	0.04%	0.005%
55	9.765	2696	2698	2702	rVV4	1377	1023	0.08%	0.009%
56	9.804	2706	2710	2712	rBV5	2096	1030	0.08%	0.009%
57	9.826	2715	2717	2719	rBV3	1610	830	0.06%	0.008%
58	9.858	2723	2727	2728	rBV3	1008	697	0.05%	0.006%
59	9.958	2756	2758	2761	rVB4	2476	1140	0.08%	0.010%
60	9.981	2761	2765	2766	rBV3	1286	918	0.07%	0.008%
61	10.074	2792	2794	2796	rBV3	1073	511	0.04%	0.005%
62	10.125	2805	2810	2815	rBV9	1838	2666	0.20%	0.024%
63	10.186	2823	2829	2831	rBV7	1758	1868	0.14%	0.017%
64	10.238	2833	2845	2859	rVV	386105	605684	45.16%	5.475%
65	10.373	2883	2887	2894	rVB8	2556	2877	0.21%	0.026%
66	10.579	2946	2951	2953	rBV3	1940	1603	0.12%	0.014%
67	10.601	2956	2958	2960	rVV3	1239	549	0.04%	0.005%
68	10.646	2969	2972	2974	rBV3	972	663	0.05%	0.006%
69	10.698	2985	2988	2991	rBV4	997	886	0.07%	0.008%
70	10.733	2998	2999	3001	rBV2	1054	574	0.04%	0.005%
71	10.961	3066	3070	3074	rBV6	1834	2086	0.16%	0.019%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061020\
 Data File : VV016781.D
 Acq On : 10 Jun 2020 20:01
 Operator : SY/MD
 Sample : L2901-04DL 200X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTR4DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

72	11.032	3087	3092	3094	rBV5	3053	3208	0.24%	0.029%
73	11.103	3111	3114	3118	rBV5	1318	1462	0.11%	0.013%
74	11.174	3134	3136	3139	rBV3	1492	923	0.07%	0.008%
75	11.270	3152	3166	3182	rBV	677748	1054417	78.62%	9.532%
76	11.646	3271	3283	3306	rVB	681088	1049263	78.23%	9.485%
77	11.916	3365	3367	3370	rBV3	1288	989	0.07%	0.009%
78	11.948	3375	3377	3379	rBV3	1618	852	0.06%	0.008%
79	12.087	3417	3420	3422	rBV3	2169	1448	0.11%	0.013%
80	12.119	3428	3430	3432	rBV3	1479	858	0.06%	0.008%
81	12.183	3448	3450	3452	rBV3	1351	665	0.05%	0.006%
82	12.241	3466	3468	3474	rVB5	1489	1063	0.08%	0.010%
83	12.299	3484	3486	3488	rBV3	1406	829	0.06%	0.007%
84	12.373	3508	3509	3513	rVB4	1345	538	0.04%	0.005%
85	12.649	3593	3595	3596	rBV2	1977	836	0.06%	0.008%
86	12.772	3631	3633	3635	rBV2	1752	966	0.07%	0.009%
87	12.810	3643	3645	3646	rBV2	1269	619	0.05%	0.006%
88	12.852	3656	3658	3660	rBV3	1016	682	0.05%	0.006%
89	13.132	3741	3745	3746	rBV3	1305	703	0.05%	0.006%
90	13.170	3755	3757	3760	rBV4	1449	912	0.07%	0.008%
91	13.231	3774	3776	3779	rBV3	1633	884	0.07%	0.008%
92	13.273	3785	3789	3792	rBV5	1744	1869	0.14%	0.017%
93	13.328	3803	3806	3809	rVB4	1822	966	0.07%	0.009%
94	13.395	3825	3827	3831	rVB3	1624	932	0.07%	0.008%
95	13.415	3831	3833	3838	rBV4	2168	1764	0.13%	0.016%
96	13.521	3864	3866	3867	rBV2	1543	650	0.05%	0.006%
97	13.836	3961	3964	3966	rBV4	1910	1310	0.10%	0.012%
98	13.968	4002	4005	4008	rBV3	1632	868	0.06%	0.008%
99	14.112	4048	4050	4052	rBV3	1177	648	0.05%	0.006%
100	14.308	4107	4111	4112	rBV3	2493	1420	0.11%	0.013%


Sum of corrected areas: 11062262

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV061020\
Data File : VV016781.D
Acq On : 10 Jun 2020 20:01
Operator : SY/MD
Sample : L2901-04DL 200X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTR4DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

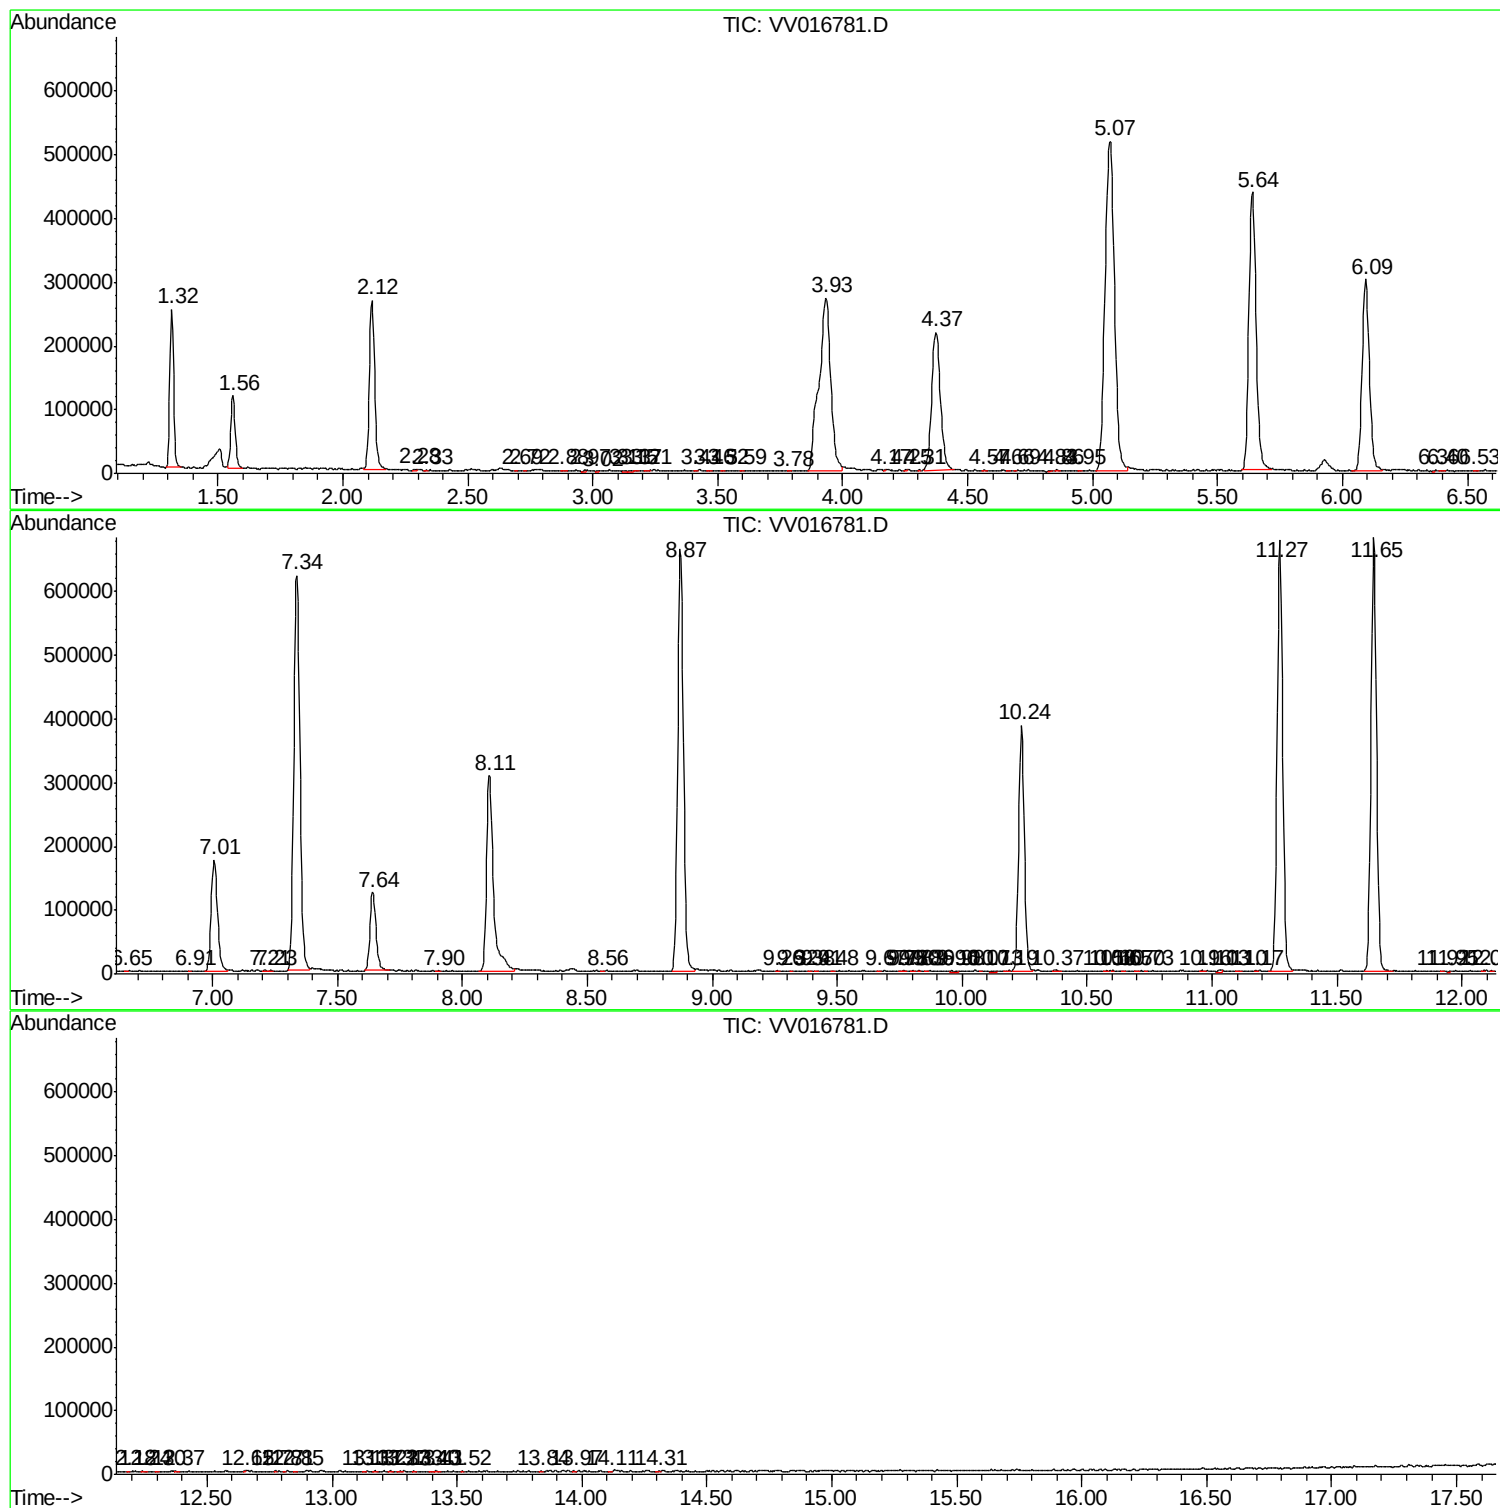

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV061020\
Data File : VV016781.D
Acq On : 10 Jun 2020 20:01
Operator : SY/MD
Sample : L2901-04DL 200X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTR4DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV061020\
Data File : VV016781.D
Acq On : 10 Jun 2020 20:01
Operator : SY/MD
Sample : L2901-04DL 200X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTR4DL

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc