

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061020\
 Data File : VV016787.D
 Acq On : 10 Jun 2020 22:47
 Operator : SY/MD
 Sample : L2929-01 100X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETT55

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	63	70	87	rVB2	615952	646400	4.06%	2.184%
2	1.553	138	144	157	rVB	103901	133186	0.84%	0.450%
3	2.116	310	319	332	rVB2	265712	407042	2.55%	1.375%
4	2.518	434	444	446	rBV10	3944	6246	0.04%	0.021%
5	2.611	471	473	476	rBV3	1498	1000	0.01%	0.003%
6	2.688	495	497	500	rBV4	1212	1002	0.01%	0.003%
7	2.730	508	510	512	rBV3	1213	625	0.00%	0.002%
8	2.775	515	524	538	rVB	26753	50394	0.32%	0.170%
9	2.994	590	592	596	rBV6	1285	1088	0.01%	0.004%
10	3.142	636	638	640	rBV3	1351	713	0.00%	0.002%
11	3.277	676	680	681	rBV3	1162	897	0.01%	0.003%
12	3.351	701	703	707	rVB4	1287	721	0.00%	0.002%
13	3.392	713	716	719	rBV3	1379	803	0.01%	0.003%
14	3.412	719	722	724	rBV4	1100	694	0.00%	0.002%
15	3.479	740	743	745	rBV3	1403	739	0.00%	0.002%
16	3.495	745	748	750	rVB4	1461	757	0.00%	0.003%
17	3.569	768	771	772	rBV3	1320	611	0.00%	0.002%
18	3.605	779	782	785	rVB4	1788	1307	0.01%	0.004%
19	3.749	823	827	829	rBV5	1774	1228	0.01%	0.004%
20	3.781	834	837	839	rBV4	1018	638	0.00%	0.002%
21	3.836	851	854	856	rBV5	1211	788	0.00%	0.003%
22	3.933	862	884	925	rBV	6524143	15934439	100.00%	53.831%
23	4.373	1008	1021	1040	rVB	204968	489745	3.07%	1.655%
24	4.579	1082	1085	1088	rBV5	2147	1569	0.01%	0.005%
25	4.769	1141	1144	1145	rBV3	1339	750	0.00%	0.003%
26	4.810	1154	1157	1159	rBV3	1258	769	0.00%	0.003%
27	4.852	1166	1170	1175	rVB8	2542	2353	0.01%	0.008%
28	5.068	1220	1237	1262	rBV2	490966	1264951	7.94%	4.273%
29	5.640	1402	1415	1436	rBV	378628	746726	4.69%	2.523%
30	5.936	1492	1507	1533	rVV	1919129	3715679	23.32%	12.553%
31	6.093	1544	1556	1578	rVB	291076	580389	3.64%	1.961%
32	6.563	1700	1702	1705	rVB3	1416	600	0.00%	0.002%
33	6.621	1718	1720	1723	rBV4	1325	916	0.01%	0.003%
34	6.794	1771	1774	1779	rBV6	1319	1100	0.01%	0.004%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061020\
 Data File : VV016787.D
 Acq On : 10 Jun 2020 22:47
 Operator : SY/MD
 Sample : L2929-01 100X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETT55

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

35	6.884	1800	1802	1805	rBV3	953	703	0.00%	0.002%
36	6.936	1815	1818	1822	rBV6	1844	1331	0.01%	0.004%
37	7.006	1829	1840	1854	rBV	167783	291826	1.83%	0.986%
38	7.103	1868	1870	1872	rBV3	1286	744	0.00%	0.003%
39	7.260	1916	1919	1925	rBV8	1549	1283	0.01%	0.004%
40	7.293	1925	1929	1931	rBV4	1673	1098	0.01%	0.004%
41	7.338	1931	1943	1958	rBV	587696	1007320	6.32%	3.403%
42	7.640	2027	2037	2056	rBV2	117456	203245	1.28%	0.687%
43	7.788	2080	2083	2084	rBV3	1308	877	0.01%	0.003%
44	7.849	2098	2102	2105	rBV5	2314	2289	0.01%	0.008%
45	7.900	2115	2118	2120	rBV4	1255	997	0.01%	0.003%
46	8.048	2161	2164	2169	rBV6	1479	1455	0.01%	0.005%
47	8.109	2172	2183	2212	rVV	298473	582210	3.65%	1.967%
48	8.412	2275	2277	2278	rBV2	2110	844	0.01%	0.003%
49	8.669	2355	2357	2360	rBV4	1366	877	0.01%	0.003%
50	8.743	2378	2380	2385	rVB6	1115	774	0.00%	0.003%
51	8.765	2385	2387	2390	rBV4	938	657	0.00%	0.002%
52	8.871	2409	2420	2438	rBV	567766	915815	5.75%	3.094%
53	9.109	2491	2494	2496	rBV4	2300	1645	0.01%	0.006%
54	9.186	2516	2518	2524	rVB6	1689	1609	0.01%	0.005%
55	9.296	2547	2552	2553	rBV4	1782	1571	0.01%	0.005%
56	9.341	2561	2566	2569	rBV6	2312	1927	0.01%	0.007%
57	9.524	2617	2623	2627	rBV8	1760	2015	0.01%	0.007%
58	9.961	2756	2759	2762	rBV4	1184	697	0.00%	0.002%
59	10.190	2824	2830	2833	rBV8	2093	2559	0.02%	0.009%
60	10.238	2833	2845	2861	rVV	372551	591995	3.72%	2.000%
61	10.309	2864	2867	2868	rBV3	1238	591	0.00%	0.002%
62	10.595	2952	2956	2959	rVB5	1246	827	0.01%	0.003%
63	10.611	2959	2961	2965	rBV5	1044	655	0.00%	0.002%
64	10.781	3011	3014	3016	rBV4	1193	714	0.00%	0.002%
65	11.000	3079	3082	3088	rVB8	1695	1324	0.01%	0.004%
66	11.128	3120	3122	3126	rBV5	1482	1042	0.01%	0.004%
67	11.183	3137	3139	3142	rBV3	1689	854	0.01%	0.003%
68	11.270	3154	3166	3182	rBV	614521	929712	5.83%	3.141%
69	11.366	3195	3196	3200	rBV4	1891	1017	0.01%	0.003%
70	11.511	3237	3241	3243	rBV4	1544	1097	0.01%	0.004%
71	11.598	3266	3268	3270	rBV3	1632	774	0.00%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061020\
 Data File : VV016787.D
 Acq On : 10 Jun 2020 22:47
 Operator : SY/MD
 Sample : L2929-01 100X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETT55

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

72	11.646	3272	3283	3296	rVV	657911	1016265	6.38%	3.433%
73	11.736	3308	3311	3313	rBV4	1531	1226	0.01%	0.004%
74	11.865	3349	3351	3354	rBV3	901	694	0.00%	0.002%
75	11.887	3356	3358	3360	rBV2	1372	593	0.00%	0.002%
76	11.993	3389	3391	3399	rVB7	1793	1490	0.01%	0.005%
77	12.025	3399	3401	3402	rBV2	1369	612	0.00%	0.002%
78	12.116	3426	3429	3430	rBV4	1394	647	0.00%	0.002%
79	12.415	3518	3522	3524	rBV4	1512	904	0.01%	0.003%
80	12.460	3534	3536	3539	rBV3	1362	780	0.00%	0.003%
81	12.514	3551	3553	3556	rVB4	1337	641	0.00%	0.002%
82	12.534	3556	3559	3563	rBV6	2175	1621	0.01%	0.005%
83	12.604	3579	3581	3585	rVB5	1386	786	0.00%	0.003%
84	12.669	3597	3601	3608	rBV10	2460	3483	0.02%	0.012%
85	12.720	3613	3617	3618	rBV3	1785	894	0.01%	0.003%
86	12.833	3649	3652	3655	rBV3	1914	1143	0.01%	0.004%
87	12.852	3655	3658	3660	rBV4	2005	1063	0.01%	0.004%
88	13.016	3706	3709	3710	rBV2	1609	1050	0.01%	0.004%
89	13.080	3727	3729	3732	rBV3	1946	1497	0.01%	0.005%
90	13.138	3745	3747	3750	rVB3	1577	912	0.01%	0.003%
91	13.154	3750	3752	3753	rBV2	1672	712	0.00%	0.002%
92	13.472	3849	3851	3855	rVB5	1730	770	0.00%	0.003%
93	13.508	3859	3862	3863	rBV3	1545	957	0.01%	0.003%
94	13.601	3889	3891	3895	rBV4	1396	791	0.00%	0.003%
95	13.659	3905	3909	3911	rBV4	1228	1037	0.01%	0.004%
96	13.752	3934	3938	3940	rBV3	2084	1442	0.01%	0.005%
97	13.897	3980	3983	3988	rBV7	956	908	0.01%	0.003%
98	14.080	4038	4040	4044	rBV4	1741	894	0.01%	0.003%
99	14.202	4075	4078	4081	rBV4	2058	1761	0.01%	0.006%
100	15.029	4333	4335	4339	rBV5	1886	1332	0.01%	0.004%


Sum of corrected areas: 29600740

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV061020\
Data File : VV016787.D
Acq On : 10 Jun 2020 22:47
Operator : SY/MD
Sample : L2929-01 100X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTS5

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

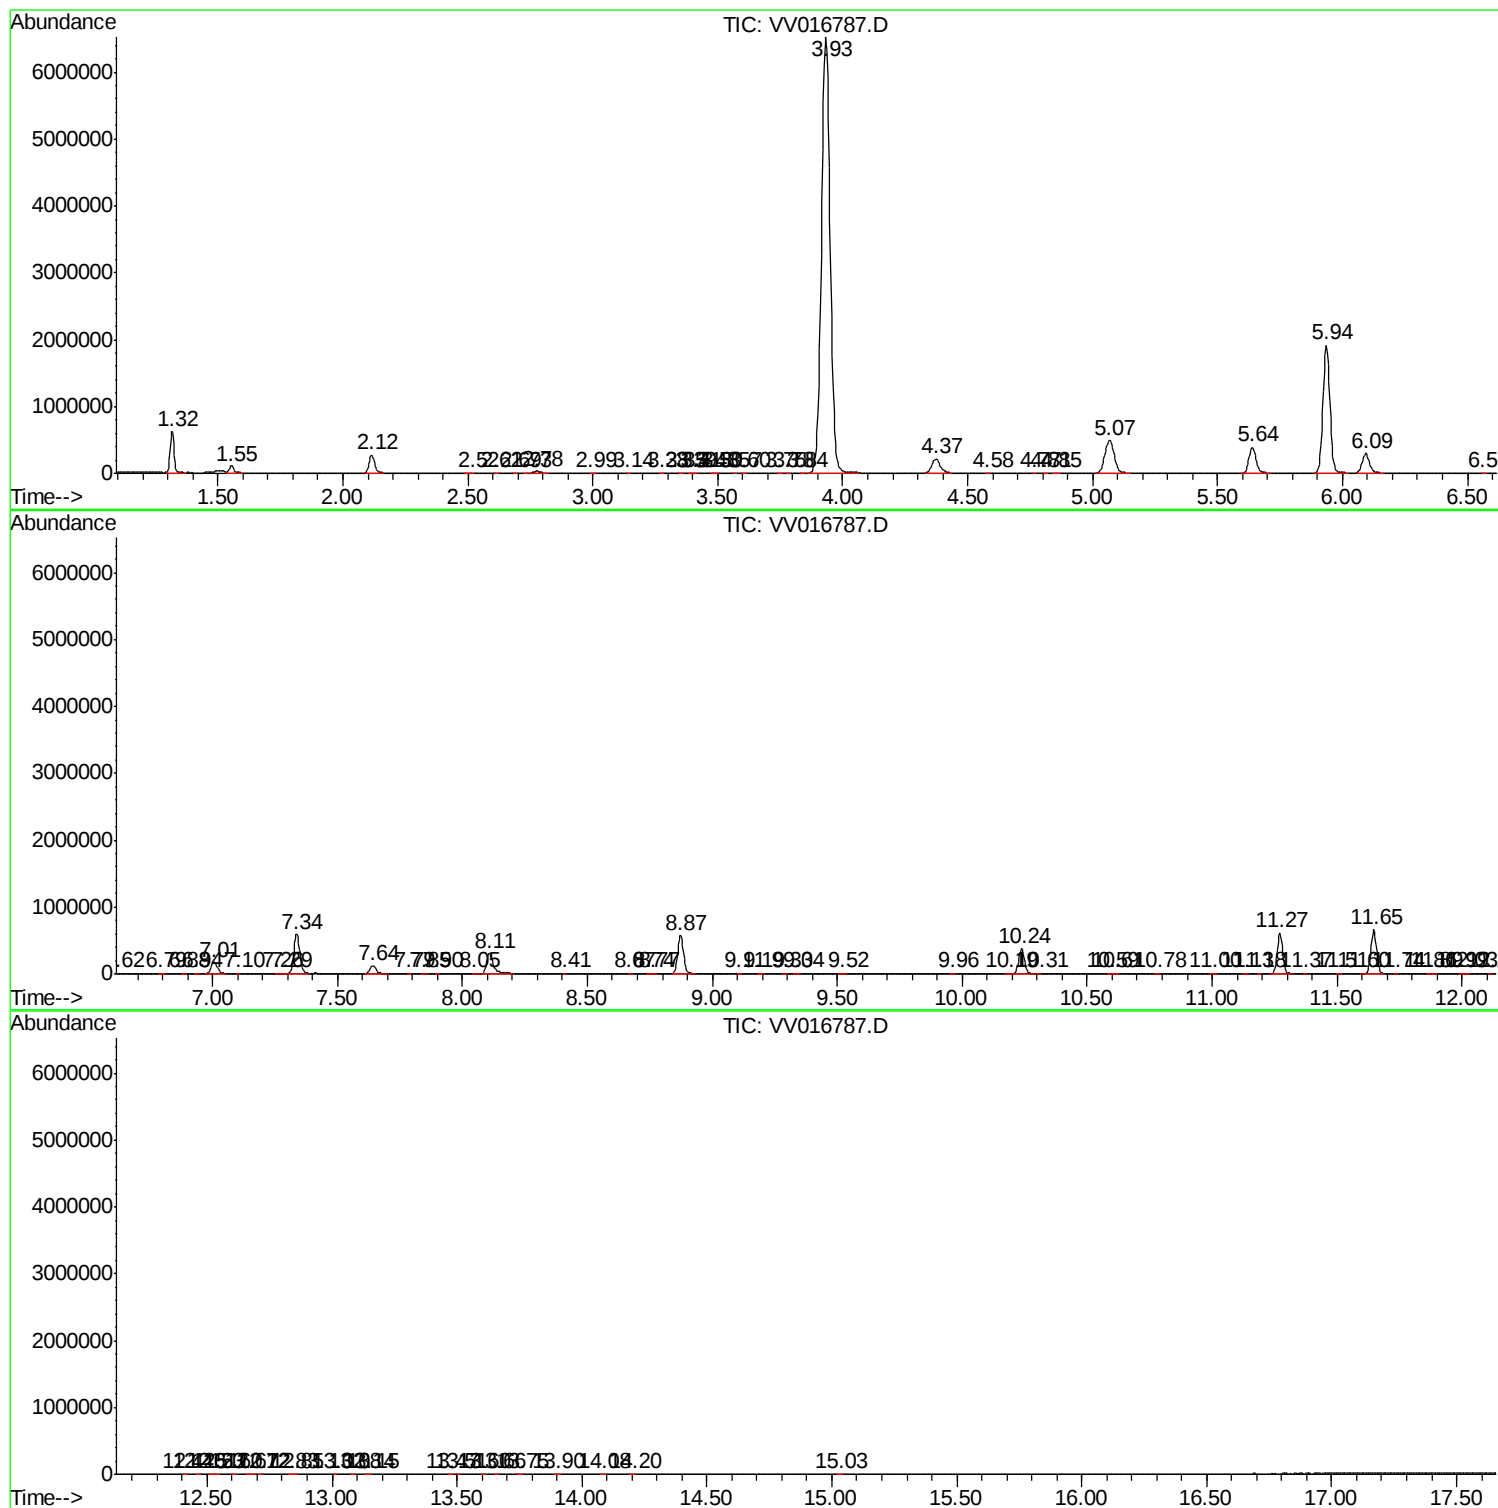

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV061020\
Data File : VV016787.D
Acq On : 10 Jun 2020 22:47
Operator : SY/MD
Sample : L2929-01 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTS5

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV061020\
Data File : VV016787.D
Acq On : 10 Jun 2020 22:47
Operator : SY/MD
Sample : L2929-01 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTS5

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc