

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061020\
 Data File : VV016788.D
 Acq On : 10 Jun 2020 23:11
 Operator : SY/MD
 Sample : L2929-02 100X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTW0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.312	63	69	80	rVB	170369	171550	13.11%	1.692%
2	1.557	139	145	162	rVB	110731	137340	10.50%	1.354%
3	2.116	309	319	333	rBV	255143	383321	29.30%	3.780%
4	2.364	392	396	399	rBV6	1317	904	0.07%	0.009%
5	2.486	432	434	436	rBV3	1615	969	0.07%	0.010%
6	2.608	470	472	473	rBV2	1310	721	0.06%	0.007%
7	2.692	496	498	506	rVB8	2189	2265	0.17%	0.022%
8	2.730	506	510	515	rBV8	1899	1989	0.15%	0.020%
9	2.830	538	541	545	rVB6	1523	1003	0.08%	0.010%
10	2.926	568	571	572	rBV3	1838	897	0.07%	0.009%
11	3.033	602	604	608	rVB4	1125	822	0.06%	0.008%
12	3.068	612	615	617	rBV3	1686	1147	0.09%	0.011%
13	3.119	629	631	635	rVB4	2427	1441	0.11%	0.014%
14	3.193	651	654	656	rBV4	1305	701	0.05%	0.007%
15	3.303	684	688	692	rBV6	1440	1380	0.11%	0.014%
16	3.402	717	719	722	rBV4	1492	1105	0.08%	0.011%
17	3.505	748	751	754	rBV4	1431	1175	0.09%	0.012%
18	3.547	762	764	766	rBV3	1594	931	0.07%	0.009%
19	3.685	805	807	809	rBV3	1574	908	0.07%	0.009%
20	3.897	862	873	908	rBV	105319	320488	24.49%	3.161%
21	4.055	920	922	925	rVB3	1690	707	0.05%	0.007%
22	4.251	981	983	988	rVB6	1314	972	0.07%	0.010%
23	4.370	1003	1020	1044	rBV	212010	523513	40.01%	5.163%
24	4.778	1143	1147	1150	rBV5	1458	1009	0.08%	0.010%
25	4.971	1204	1207	1211	rBV5	1282	1183	0.09%	0.012%
26	4.997	1211	1215	1218	rVV5	1250	1270	0.10%	0.013%
27	5.068	1220	1237	1261	rBV2	513613	1308470	100.00%	12.904%
28	5.319	1312	1315	1317	rBV4	1540	1114	0.09%	0.011%
29	5.483	1362	1366	1368	rBV4	2266	1363	0.10%	0.013%
30	5.579	1392	1396	1397	rBV4	1437	1025	0.08%	0.010%
31	5.637	1402	1414	1431	rVV	398083	784946	59.99%	7.741%
32	5.930	1493	1505	1519	rBV8	19143	45617	3.49%	0.450%
33	6.090	1543	1555	1578	rVB	291444	588051	44.94%	5.799%
34	6.434	1659	1662	1664	rBV4	1666	1072	0.08%	0.011%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061020\
 Data File : VV016788.D
 Acq On : 10 Jun 2020 23:11
 Operator : SY/MD
 Sample : L2929-02 100X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTW0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

35	6.518	1685	1688	1690	rBV3	1348	946	0.07%	0.009%
36	6.576	1702	1706	1707	rBV4	1331	719	0.05%	0.007%
37	6.585	1707	1709	1713	rVV5	1217	789	0.06%	0.008%
38	6.717	1747	1750	1752	rBV4	1825	1062	0.08%	0.010%
39	6.801	1774	1776	1780	rBV5	1443	1041	0.08%	0.010%
40	6.859	1790	1794	1796	rBV4	1486	794	0.06%	0.008%
41	7.007	1829	1840	1859	rBV	164659	295648	22.59%	2.916%
42	7.338	1929	1943	1959	rBV	603377	1044763	79.85%	10.303%
43	7.640	2026	2037	2053	rBV	117927	200054	15.29%	1.973%
44	7.804	2081	2088	2091	rBV8	1889	2364	0.18%	0.023%
45	8.068	2167	2170	2172	rBV3	2299	1464	0.11%	0.014%
46	8.106	2172	2182	2211	rVV	312357	599482	45.82%	5.912%
47	8.312	2244	2246	2250	rBV4	1633	1201	0.09%	0.012%
48	8.434	2279	2284	2291	rBV8	3493	4948	0.38%	0.049%
49	8.669	2354	2357	2358	rBV3	1397	792	0.06%	0.008%
50	8.798	2395	2397	2402	rBV6	1391	773	0.06%	0.008%
51	8.872	2409	2420	2437	rBV	602815	975738	74.57%	9.623%
52	9.154	2506	2508	2512	rBV5	1482	890	0.07%	0.009%
53	9.344	2562	2567	2568	rBV4	2274	1929	0.15%	0.019%
54	9.386	2577	2580	2584	rBV6	1143	1005	0.08%	0.010%
55	9.579	2635	2640	2643	rBV6	2468	2344	0.18%	0.023%
56	9.669	2665	2668	2672	rVB5	1640	1128	0.09%	0.011%
57	9.717	2681	2683	2685	rBV3	1763	1034	0.08%	0.010%
58	9.994	2767	2769	2772	rVB3	2196	1137	0.09%	0.011%
59	10.064	2790	2791	2794	rVV3	1234	764	0.06%	0.008%
60	10.093	2798	2800	2802	rBV3	1250	745	0.06%	0.007%
61	10.238	2834	2845	2863	rVB	389640	613752	46.91%	6.053%
62	10.466	2914	2916	2920	rVB5	2093	1189	0.09%	0.012%
63	10.486	2920	2922	2925	rVB4	1838	855	0.07%	0.008%
64	10.518	2930	2932	2935	rBV3	1047	732	0.06%	0.007%
65	10.563	2943	2946	2948	rBV4	1406	1029	0.08%	0.010%
66	10.630	2963	2967	2971	rBV7	1230	1385	0.11%	0.014%
67	10.688	2982	2985	2986	rBV3	1370	767	0.06%	0.008%
68	10.817	3021	3025	3026	rBV4	1637	891	0.07%	0.009%
69	11.055	3096	3099	3101	rBV5	1152	760	0.06%	0.007%
70	11.097	3108	3112	3116	rBV7	1591	1387	0.11%	0.014%
71	11.270	3153	3166	3180	rBV	652482	1000185	76.44%	9.864%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061020\
 Data File : VV016788.D
 Acq On : 10 Jun 2020 23:11
 Operator : SY/MD
 Sample : L2929-02 100X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTW0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

72	11.370	3193	3197	3201	rBV7	2698	2922	0.22%	0.029%
73	11.444	3217	3220	3222	rVB3	2100	1057	0.08%	0.010%
74	11.646	3271	3283	3299	rBV	675840	1046324	79.97%	10.319%
75	11.926	3365	3370	3371	rBV5	1731	1399	0.11%	0.014%
76	12.090	3419	3421	3424	rBV2	1652	1083	0.08%	0.011%
77	12.341	3495	3499	3501	rBV4	1263	984	0.08%	0.010%
78	12.424	3521	3525	3526	rBV4	1665	892	0.07%	0.009%
79	12.473	3538	3540	3542	rBV3	1417	910	0.07%	0.009%
80	12.514	3552	3553	3559	rBV5	1426	1213	0.09%	0.012%
81	12.569	3564	3570	3571	rBV6	1654	917	0.07%	0.009%
82	12.669	3598	3601	3605	rVB4	2066	1618	0.12%	0.016%
83	12.788	3632	3638	3641	rBV7	2006	1816	0.14%	0.018%
84	12.881	3663	3667	3668	rBV3	1653	841	0.06%	0.008%
85	13.113	3734	3739	3742	rVB6	1471	1171	0.09%	0.012%
86	13.212	3767	3770	3771	rBV3	1209	749	0.06%	0.007%
87	13.344	3804	3811	3813	rBV7	2415	2860	0.22%	0.028%
88	13.691	3913	3919	3920	rBV5	1561	1417	0.11%	0.014%
89	13.711	3923	3925	3928	rBV4	1094	712	0.05%	0.007%
90	13.788	3947	3949	3953	rBV3	1310	968	0.07%	0.010%
91	13.826	3958	3961	3963	rVB5	1305	760	0.06%	0.007%
92	14.013	4016	4019	4021	rBV3	2240	1147	0.09%	0.011%
93	14.267	4095	4098	4100	rBV3	2450	1386	0.11%	0.014%
94	14.537	4178	4182	4185	rBV5	1510	1283	0.10%	0.013%
95	14.569	4185	4192	4194	rBV8	1671	1907	0.15%	0.019%
96	14.791	4258	4261	4262	rBV3	1879	896	0.07%	0.009%
97	14.833	4272	4274	4278	rBV4	1607	1185	0.09%	0.012%
98	15.112	4359	4361	4364	rVB4	1733	1014	0.08%	0.010%
99	15.524	4487	4489	4494	rBV4	2393	1750	0.13%	0.017%
100	15.547	4494	4496	4497	rBV2	2256	1047	0.08%	0.010%


Sum of corrected areas: 10140083

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV061020\
Data File : VV016788.D
Acq On : 10 Jun 2020 23:11
Operator : SY/MD
Sample : L2929-02 100X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampled :
ETTW0

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

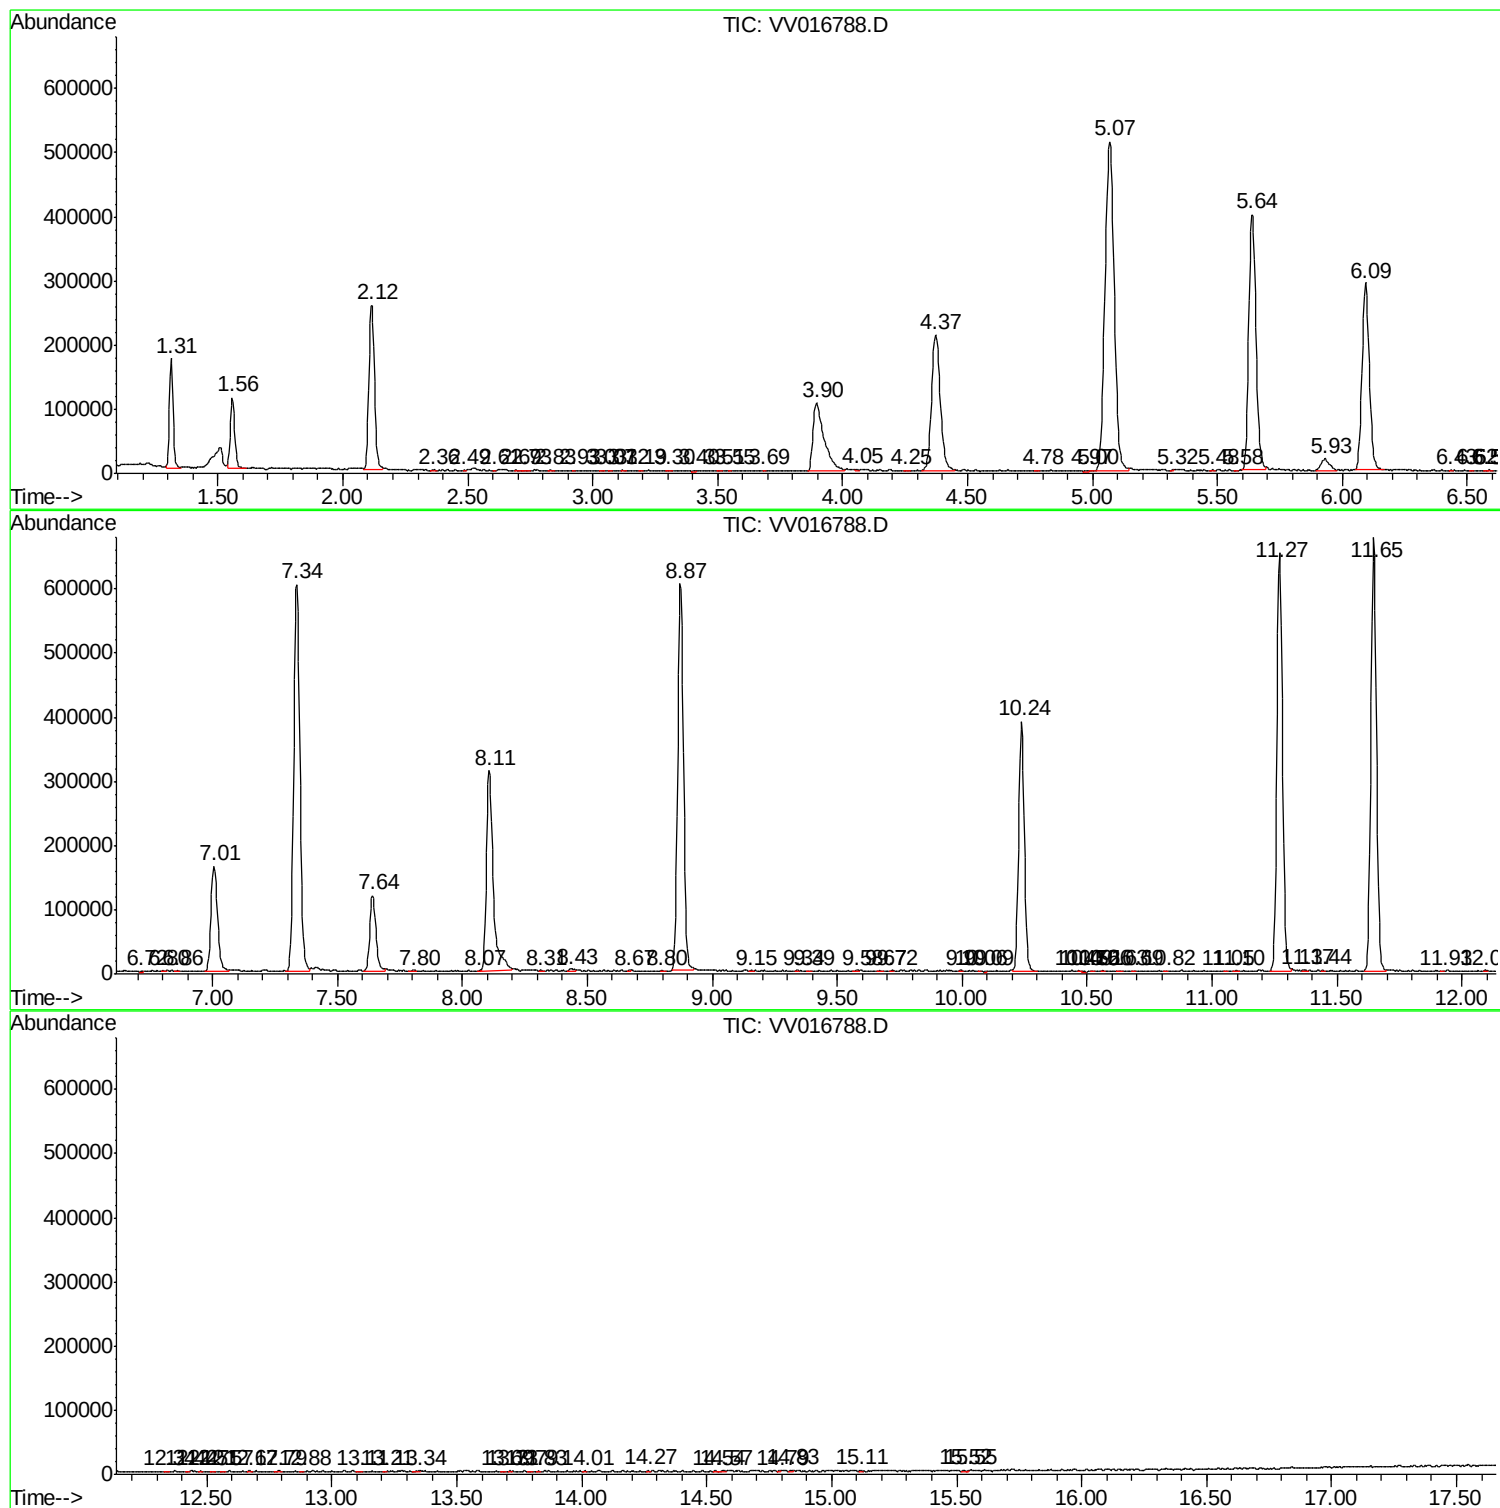

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV061020\
Data File : VV016788.D
Acq On : 10 Jun 2020 23:11
Operator : SY/MD
Sample : L2929-02 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTW0

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV061020\
Data File : VV016788.D
Acq On : 10 Jun 2020 23:11
Operator : SY/MD
Sample : L2929-02 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTW0

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc