

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061020\
 Data File : VV016790.D
 Acq On : 10 Jun 2020 23:59
 Operator : SY/MD
 Sample : L2929-04 100X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTW2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.312	63	69	83	rVB	167816	171299	13.61%	1.777%
2	1.553	138	144	159	rVB	111520	134531	10.69%	1.395%
3	2.113	309	318	333	rBV	243991	366867	29.15%	3.805%
4	2.511	436	442	444	rBV7	2823	2926	0.23%	0.030%
5	2.733	506	511	516	rBV8	2305	2441	0.19%	0.025%
6	2.759	516	519	523	rBV5	2089	2111	0.17%	0.022%
7	2.846	542	546	547	rVV3	1558	956	0.08%	0.010%
8	3.116	627	630	633	rBV5	2058	1117	0.09%	0.012%
9	3.180	645	650	652	rBV4	1093	806	0.06%	0.008%
10	3.412	720	722	725	rBV4	1806	976	0.08%	0.010%
11	3.553	764	766	769	rVB4	1689	776	0.06%	0.008%
12	3.663	796	800	803	rBV6	754	769	0.06%	0.008%
13	3.685	804	807	813	rVB8	1588	1173	0.09%	0.012%
14	3.711	813	815	818	rVB4	1507	763	0.06%	0.008%
15	3.727	818	820	822	rBV3	1737	1083	0.09%	0.011%
16	3.897	861	873	902	rVV	98464	283236	22.50%	2.938%
17	4.373	1005	1021	1041	rVV	200110	495190	39.34%	5.136%
18	4.589	1084	1088	1091	rBV5	1969	1437	0.11%	0.015%
19	4.733	1130	1133	1138	rVV7	1724	1683	0.13%	0.017%
20	4.984	1208	1211	1217	rBV8	1473	1677	0.13%	0.017%
21	5.068	1219	1237	1264	rBV2	490183	1258727	100.00%	13.056%
22	5.444	1352	1354	1358	rBV3	1817	1646	0.13%	0.017%
23	5.527	1378	1380	1382	rBV3	1259	781	0.06%	0.008%
24	5.637	1401	1414	1435	rBV	386354	769004	61.09%	7.977%
25	5.807	1465	1467	1469	rVB3	2001	790	0.06%	0.008%
26	6.090	1543	1555	1574	rBV	275821	554544	44.06%	5.752%
27	6.283	1614	1615	1619	rVB3	2814	1467	0.12%	0.015%
28	6.521	1687	1689	1693	rVB4	1896	1257	0.10%	0.013%
29	6.553	1693	1699	1701	rBV6	1906	1804	0.14%	0.019%
30	6.608	1712	1716	1718	rBV4	1159	1186	0.09%	0.012%
31	6.688	1738	1741	1745	rBV4	1795	1254	0.10%	0.013%
32	6.839	1785	1788	1791	rBV4	1562	1134	0.09%	0.012%
33	6.862	1791	1795	1799	rBV7	1921	1924	0.15%	0.020%
34	6.920	1808	1813	1816	rBV6	2518	2221	0.18%	0.023%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061020\
 Data File : VV016790.D
 Acq On : 10 Jun 2020 23:59
 Operator : SY/MD
 Sample : L2929-04 100X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTW2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

35	7.007	1828	1840	1860	rBV	153887	281597	22.37%	2.921%
36	7.116	1871	1874	1876	rVB3	1860	1089	0.09%	0.011%
37	7.199	1898	1900	1901	rBV2	2007	773	0.06%	0.008%
38	7.338	1931	1943	1960	rBV	579553	992176	78.82%	10.291%
39	7.640	2024	2037	2056	rBV2	110520	190472	15.13%	1.976%
40	8.029	2155	2158	2161	rBV4	1395	908	0.07%	0.009%
41	8.071	2168	2171	2172	rBV3	2269	1240	0.10%	0.013%
42	8.109	2172	2183	2214	rVV2	293462	576356	45.79%	5.978%
43	8.656	2351	2353	2355	rBV3	1466	759	0.06%	0.008%
44	8.762	2384	2386	2391	rBV6	1176	935	0.07%	0.010%
45	8.871	2408	2420	2440	rBV	578462	936155	74.37%	9.710%
46	9.235	2530	2533	2539	rVB7	2425	1972	0.16%	0.020%
47	9.264	2539	2542	2545	rBV3	1347	1065	0.08%	0.011%
48	9.305	2550	2555	2556	rBV4	1259	890	0.07%	0.009%
49	9.428	2589	2593	2595	rVB5	1878	1294	0.10%	0.013%
50	9.447	2595	2599	2601	rBV5	1005	769	0.06%	0.008%
51	9.595	2641	2645	2647	rBV4	1585	1420	0.11%	0.015%
52	9.865	2724	2729	2732	rBV5	1904	1396	0.11%	0.014%
53	10.077	2792	2795	2798	rBV5	1483	985	0.08%	0.010%
54	10.170	2820	2824	2827	rVB5	1479	1369	0.11%	0.014%
55	10.190	2827	2830	2833	rBV4	1165	1034	0.08%	0.011%
56	10.238	2833	2845	2858	rBV	366282	575307	45.71%	5.967%
57	10.350	2878	2880	2882	rBV2	1587	764	0.06%	0.008%
58	10.457	2910	2913	2917	rBV5	1596	1066	0.08%	0.011%
59	10.752	3003	3005	3008	rVB4	1752	954	0.08%	0.010%
60	10.865	3038	3040	3042	rBV3	1879	844	0.07%	0.009%
61	10.942	3060	3064	3069	rBV9	1623	1497	0.12%	0.016%
62	11.010	3079	3085	3087	rBV7	2324	2513	0.20%	0.026%
63	11.215	3146	3149	3151	rVB4	1458	915	0.07%	0.009%
64	11.231	3151	3154	3155	rBV3	1157	778	0.06%	0.008%
65	11.270	3155	3166	3186	rBV	617909	944378	75.03%	9.796%
66	11.521	3242	3244	3249	rBV6	1077	951	0.08%	0.010%
67	11.553	3252	3254	3258	rVB5	1685	1210	0.10%	0.013%
68	11.575	3258	3261	3263	rBV2	1245	862	0.07%	0.009%
69	11.646	3271	3283	3302	rBV	641850	1003979	79.76%	10.414%
70	11.804	3328	3332	3336	rVB7	2381	1744	0.14%	0.018%
71	12.022	3389	3400	3402	rBV7	2078	2891	0.23%	0.030%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061020\
 Data File : VV016790.D
 Acq On : 10 Jun 2020 23:59
 Operator : SY/MD
 Sample : L2929-04 100X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTW2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

72	12.116	3425	3429	3431	rBV3	1798	1407	0.11%	0.015%
73	12.196	3448	3454	3459	rVB8	2219	3008	0.24%	0.031%
74	12.238	3465	3467	3472	rVV4	1508	1023	0.08%	0.011%
75	12.260	3472	3474	3479	rVV6	1424	1230	0.10%	0.013%
76	12.354	3501	3503	3505	rBV2	1521	838	0.07%	0.009%
77	12.405	3517	3519	3524	rVB5	2231	1655	0.13%	0.017%
78	12.527	3555	3557	3560	rBV4	1533	1288	0.10%	0.013%
79	12.630	3585	3589	3592	rBV5	2537	2065	0.16%	0.021%
80	12.717	3614	3616	3620	rVB3	1645	1116	0.09%	0.012%
81	12.739	3620	3623	3625	rBV4	1366	958	0.08%	0.010%
82	12.791	3636	3639	3641	rBV3	1563	1044	0.08%	0.011%
83	12.903	3672	3674	3679	rBV5	1887	1423	0.11%	0.015%
84	12.971	3692	3695	3697	rBV3	1219	791	0.06%	0.008%
85	13.054	3719	3721	3723	rBV3	1561	845	0.07%	0.009%
86	13.109	3734	3738	3742	rBV6	1418	1411	0.11%	0.015%
87	13.151	3748	3751	3754	rBV5	1244	868	0.07%	0.009%
88	13.183	3758	3761	3763	rBV5	1680	786	0.06%	0.008%
89	13.231	3772	3776	3778	rBV3	1471	1134	0.09%	0.012%
90	13.411	3829	3832	3835	rBV5	1698	1303	0.10%	0.014%
91	13.530	3865	3869	3871	rBV4	1245	1035	0.08%	0.011%
92	13.649	3902	3906	3908	rBV4	1757	1317	0.10%	0.014%
93	13.681	3914	3916	3918	rBV3	1632	901	0.07%	0.009%
94	14.270	4096	4099	4102	rBV4	1409	975	0.08%	0.010%
95	14.424	4145	4147	4151	rBV3	1550	829	0.07%	0.009%
96	14.527	4177	4179	4184	rVB6	2303	1429	0.11%	0.015%
97	14.550	4184	4186	4190	rVB5	1673	1118	0.09%	0.012%
98	14.572	4190	4193	4196	rBV4	1790	1386	0.11%	0.014%
99	14.640	4212	4214	4216	rBV3	1307	826	0.07%	0.009%
100	15.517	4485	4487	4492	rBV5	1977	1965	0.16%	0.020%


Sum of corrected areas: 9640837

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV061020\
Data File : VV016790.D
Acq On : 10 Jun 2020 23:59
Operator : SY/MD
Sample : L2929-04 100X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampled :
ETTW2

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

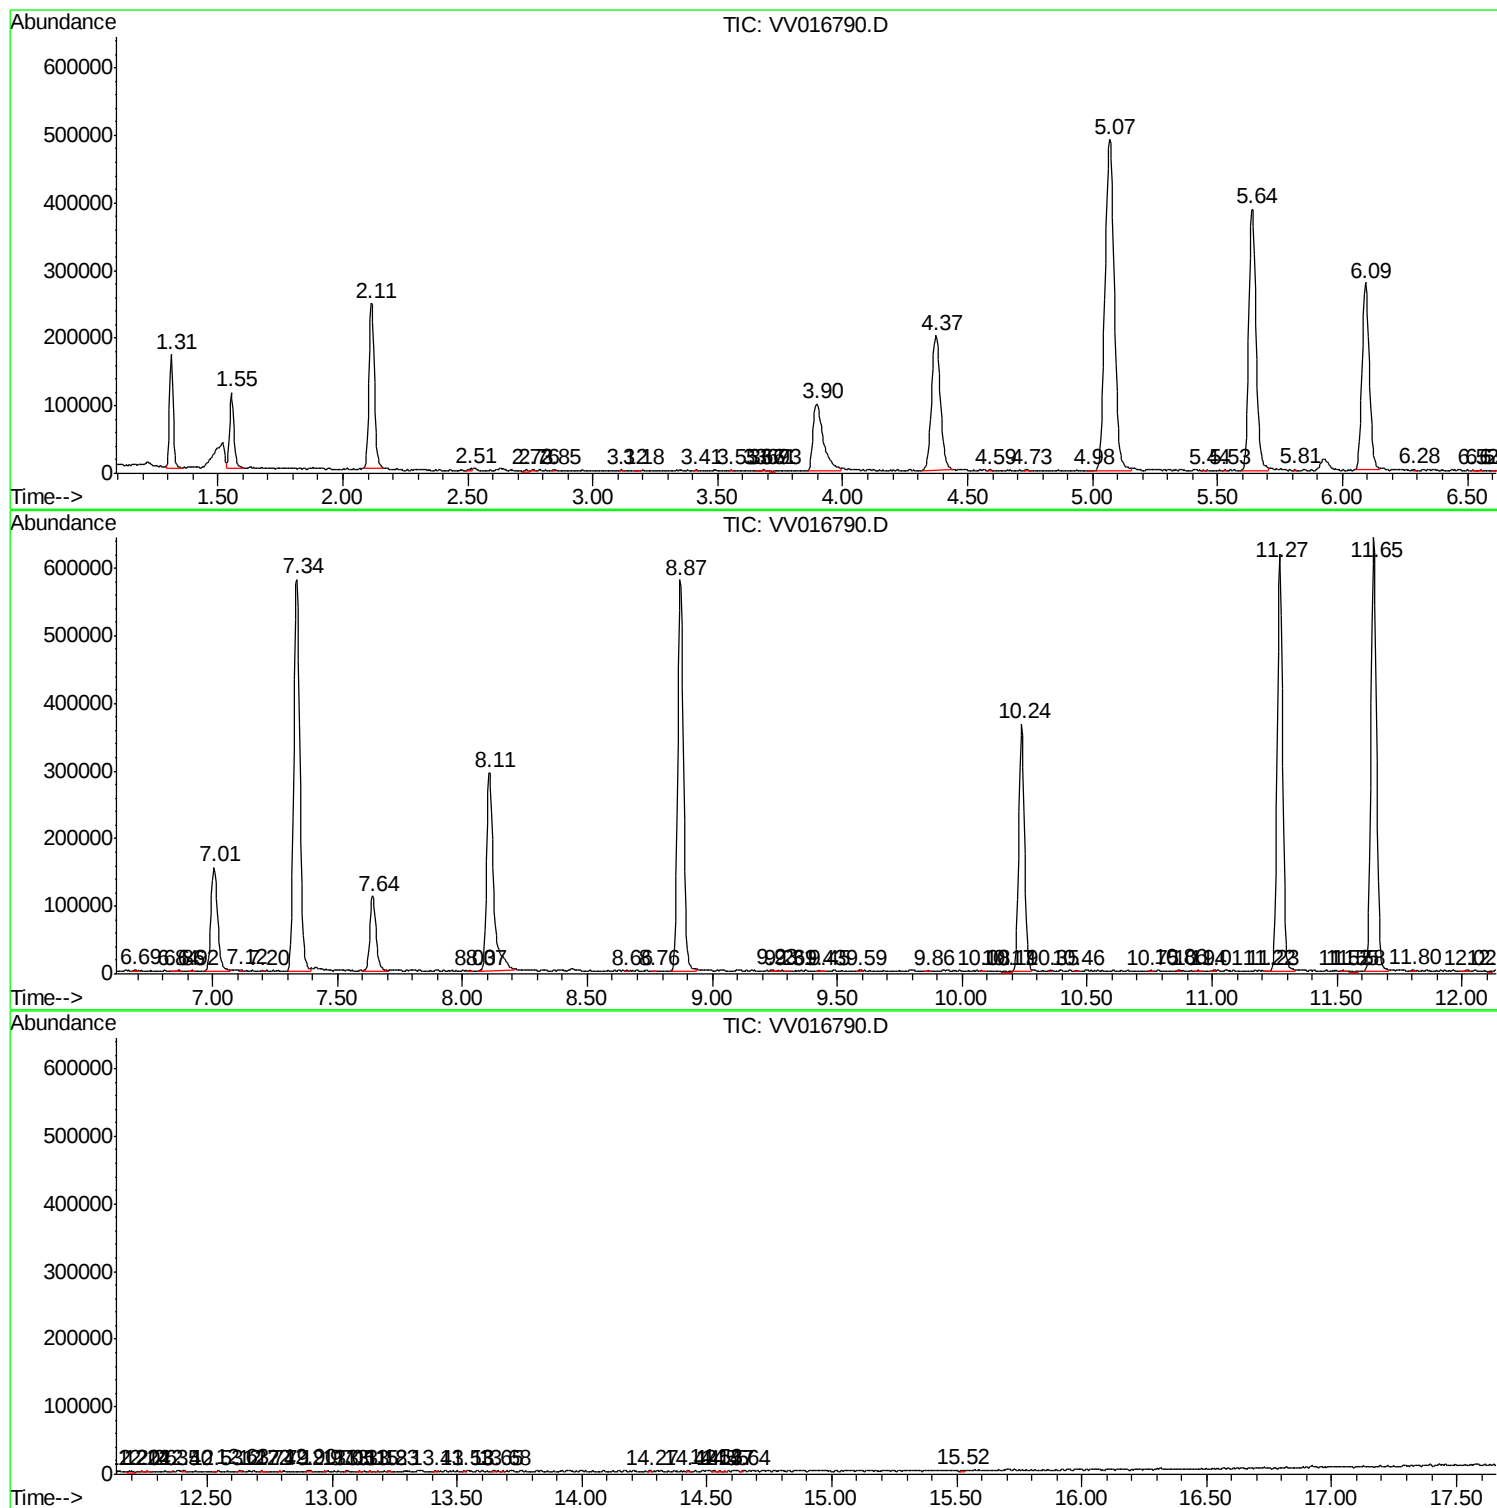

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV061020\
Data File : VV016790.D
Acq On : 10 Jun 2020 23:59
Operator : SY/MD
Sample : L2929-04 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTW2

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV061020\
Data File : VV016790.D
Acq On : 10 Jun 2020 23:59
Operator : SY/MD
Sample : L2929-04 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTW2

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc