

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061020\
 Data File : VV016791.D
 Acq On : 11 Jun 2020 00:23
 Operator : SY/MD
 Sample : L2929-05 100X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTW3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.312	63	69	80	rVB	174725	178213	13.83%	1.839%
2	2.113	309	318	334	rVB	252400	371068	28.79%	3.830%
3	2.460	424	426	428	rBV3	1406	839	0.07%	0.009%
4	2.765	518	521	522	rBV3	1109	761	0.06%	0.008%
5	2.868	550	553	555	rBV3	1185	757	0.06%	0.008%
6	2.997	590	593	598	rBV7	1868	1713	0.13%	0.018%
7	3.087	619	621	624	rBV4	1350	893	0.07%	0.009%
8	3.138	634	637	641	rBV5	2020	1919	0.15%	0.020%
9	3.161	641	644	647	rVV4	1534	1017	0.08%	0.010%
10	3.225	659	664	665	rBV5	1663	1284	0.10%	0.013%
11	3.293	681	685	687	rVV5	1576	1338	0.10%	0.014%
12	3.373	707	710	712	rVB3	1570	714	0.06%	0.007%
13	3.534	757	760	763	rVB3	1612	856	0.07%	0.009%
14	3.582	771	775	778	rBV5	1222	1012	0.08%	0.010%
15	3.730	816	821	824	rBV7	1439	1189	0.09%	0.012%
16	3.769	829	833	836	rVV5	1362	969	0.08%	0.010%
17	3.804	842	844	847	rVB3	1333	905	0.07%	0.009%
18	3.849	854	858	861	rBV5	1815	1768	0.14%	0.018%
19	3.894	861	872	904	rBV	101293	288934	22.42%	2.982%
20	4.171	955	958	960	rBV3	1464	857	0.07%	0.009%
21	4.257	982	985	987	rBV3	1506	1065	0.08%	0.011%
22	4.373	1006	1021	1042	rVB	208388	503969	39.10%	5.201%
23	4.531	1068	1070	1071	rBV2	1679	693	0.05%	0.007%
24	4.634	1100	1102	1106	rBV5	1289	1041	0.08%	0.011%
25	4.765	1139	1143	1145	rBV4	2379	1298	0.10%	0.013%
26	4.785	1147	1149	1152	rVB4	2074	1041	0.08%	0.011%
27	4.817	1156	1159	1161	rBV4	2351	1184	0.09%	0.012%
28	4.891	1179	1182	1188	rBV6	2005	1314	0.10%	0.014%
29	5.068	1219	1237	1260	rBV2	505859	1288913	100.00%	13.302%
30	5.219	1282	1284	1286	rBV3	1735	917	0.07%	0.009%
31	5.553	1384	1388	1391	rBV6	1671	1139	0.09%	0.012%
32	5.637	1402	1414	1437	rVV	385518	777346	60.31%	8.022%
33	5.775	1454	1457	1459	rBV3	1419	928	0.07%	0.010%
34	6.090	1541	1555	1580	rBV	288485	585793	45.45%	6.046%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061020\
 Data File : VV016791.D
 Acq On : 11 Jun 2020 00:23
 Operator : SY/MD
 Sample : L2929-05 100X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTW3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

35	6.260	1606	1608	1613	rVB5	2154	1556	0.12%	0.016%
36	6.286	1613	1616	1617	rBV3	1343	818	0.06%	0.008%
37	6.344	1631	1634	1636	rBV4	1227	726	0.06%	0.007%
38	6.415	1652	1656	1659	rBV6	2058	1691	0.13%	0.017%
39	6.547	1693	1697	1698	rBV3	2222	1599	0.12%	0.017%
40	6.630	1718	1723	1724	rBV5	1428	1227	0.10%	0.013%
41	6.743	1755	1758	1760	rBV3	1462	795	0.06%	0.008%
42	7.006	1829	1840	1855	rBV	161894	282666	21.93%	2.917%
43	7.199	1898	1900	1902	rVB3	1685	707	0.05%	0.007%
44	7.219	1902	1906	1907	rBV3	1322	832	0.06%	0.009%
45	7.338	1928	1943	1960	rBV	591745	1020342	79.16%	10.530%
46	7.566	2011	2014	2017	rBV5	1644	897	0.07%	0.009%
47	7.640	2026	2037	2051	rBV	120057	199895	15.51%	2.063%
48	7.723	2061	2063	2069	rVB6	2353	1428	0.11%	0.015%
49	7.752	2069	2072	2073	rBV2	1454	887	0.07%	0.009%
50	7.923	2123	2125	2130	rVB6	1984	1007	0.08%	0.010%
51	7.949	2130	2133	2134	rBV2	1162	819	0.06%	0.008%
52	8.042	2159	2162	2164	rBV4	1663	831	0.06%	0.009%
53	8.109	2172	2183	2213	rBV	298960	599074	46.48%	6.183%
54	8.582	2327	2330	2331	rBV4	1475	819	0.06%	0.008%
55	8.871	2408	2420	2442	rBV	585656	952997	73.94%	9.835%
56	9.116	2494	2496	2499	rVB4	1900	984	0.08%	0.010%
57	9.141	2502	2504	2507	rBV3	1136	773	0.06%	0.008%
58	9.247	2534	2537	2539	rBV3	2091	1312	0.10%	0.014%
59	9.350	2567	2569	2573	rVB4	1279	799	0.06%	0.008%
60	9.585	2638	2642	2644	rBV4	1765	1239	0.10%	0.013%
61	9.701	2674	2678	2680	rBV4	1412	915	0.07%	0.009%
62	9.781	2701	2703	2707	rVB5	1095	860	0.07%	0.009%
63	9.804	2707	2710	2712	rBV3	1550	1248	0.10%	0.013%
64	9.871	2728	2731	2734	rBV4	1728	1516	0.12%	0.016%
65	10.048	2784	2786	2788	rBV3	1945	1095	0.08%	0.011%
66	10.103	2800	2803	2807	rBV5	1987	1428	0.11%	0.015%
67	10.164	2819	2822	2827	rVB6	1607	1037	0.08%	0.011%
68	10.238	2833	2845	2858	rVV	374749	587474	45.58%	6.063%
69	10.485	2919	2922	2923	rBV3	1420	709	0.06%	0.007%
70	10.518	2927	2932	2934	rBV5	1307	1095	0.08%	0.011%
71	10.608	2953	2960	2963	rBV8	2175	2711	0.21%	0.028%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061020\
 Data File : VV016791.D
 Acq On : 11 Jun 2020 00:23
 Operator : SY/MD
 Sample : L2929-05 100X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTW3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

72	10.964	3068	3071	3074	rBV4	1955	1478	0.11%	0.015%
73	11.077	3103	3106	3109	rBV5	1367	812	0.06%	0.008%
74	11.106	3109	3115	3117	rVV6	1491	1284	0.10%	0.013%
75	11.122	3117	3120	3122	rVB5	1312	718	0.06%	0.007%
76	11.148	3124	3128	3130	rBV5	947	784	0.06%	0.008%
77	11.270	3155	3166	3186	rVB	622987	936700	72.67%	9.667%
78	11.402	3200	3207	3210	rBV7	1700	1747	0.14%	0.018%
79	11.421	3210	3213	3215	rBV3	1437	1026	0.08%	0.011%
80	11.489	3231	3234	3237	rVV4	1477	775	0.06%	0.008%
81	11.534	3242	3248	3252	rVB10	2289	2599	0.20%	0.027%
82	11.646	3271	3283	3299	rBV	648198	1021017	79.22%	10.537%
83	11.804	3331	3332	3335	rBV3	1416	939	0.07%	0.010%
84	12.164	3440	3444	3448	rVV5	2008	1368	0.11%	0.014%
85	12.199	3451	3455	3458	rBV4	1255	1098	0.09%	0.011%
86	12.341	3495	3499	3501	rVV4	1104	842	0.07%	0.009%
87	12.437	3523	3529	3531	rBV5	2015	1824	0.14%	0.019%
88	12.646	3591	3594	3596	rBV3	1797	1149	0.09%	0.012%
89	12.733	3618	3621	3624	rBV5	1471	757	0.06%	0.008%
90	12.826	3645	3650	3651	rBV4	1320	731	0.06%	0.008%
91	13.003	3703	3705	3708	rBV4	1353	797	0.06%	0.008%
92	13.032	3712	3714	3717	rBV4	1363	880	0.07%	0.009%
93	13.048	3717	3719	3723	rVB5	1314	709	0.06%	0.007%
94	13.254	3781	3783	3786	rVB4	2047	723	0.06%	0.007%
95	13.270	3786	3788	3791	rBV3	1162	877	0.07%	0.009%
96	13.601	3888	3891	3893	rBV3	1303	877	0.07%	0.009%
97	13.649	3900	3906	3910	rBV9	2526	2930	0.23%	0.030%
98	13.688	3914	3918	3919	rBV4	1086	829	0.06%	0.009%
99	14.296	4104	4107	4110	rBV4	1476	1233	0.10%	0.013%
100	14.694	4228	4231	4233	rBV4	2359	1628	0.13%	0.017%


Sum of corrected areas: 9689586

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV061020\
Data File : VV016791.D
Acq On : 11 Jun 2020 00:23
Operator : SY/MD
Sample : L2929-05 100X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTW3

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

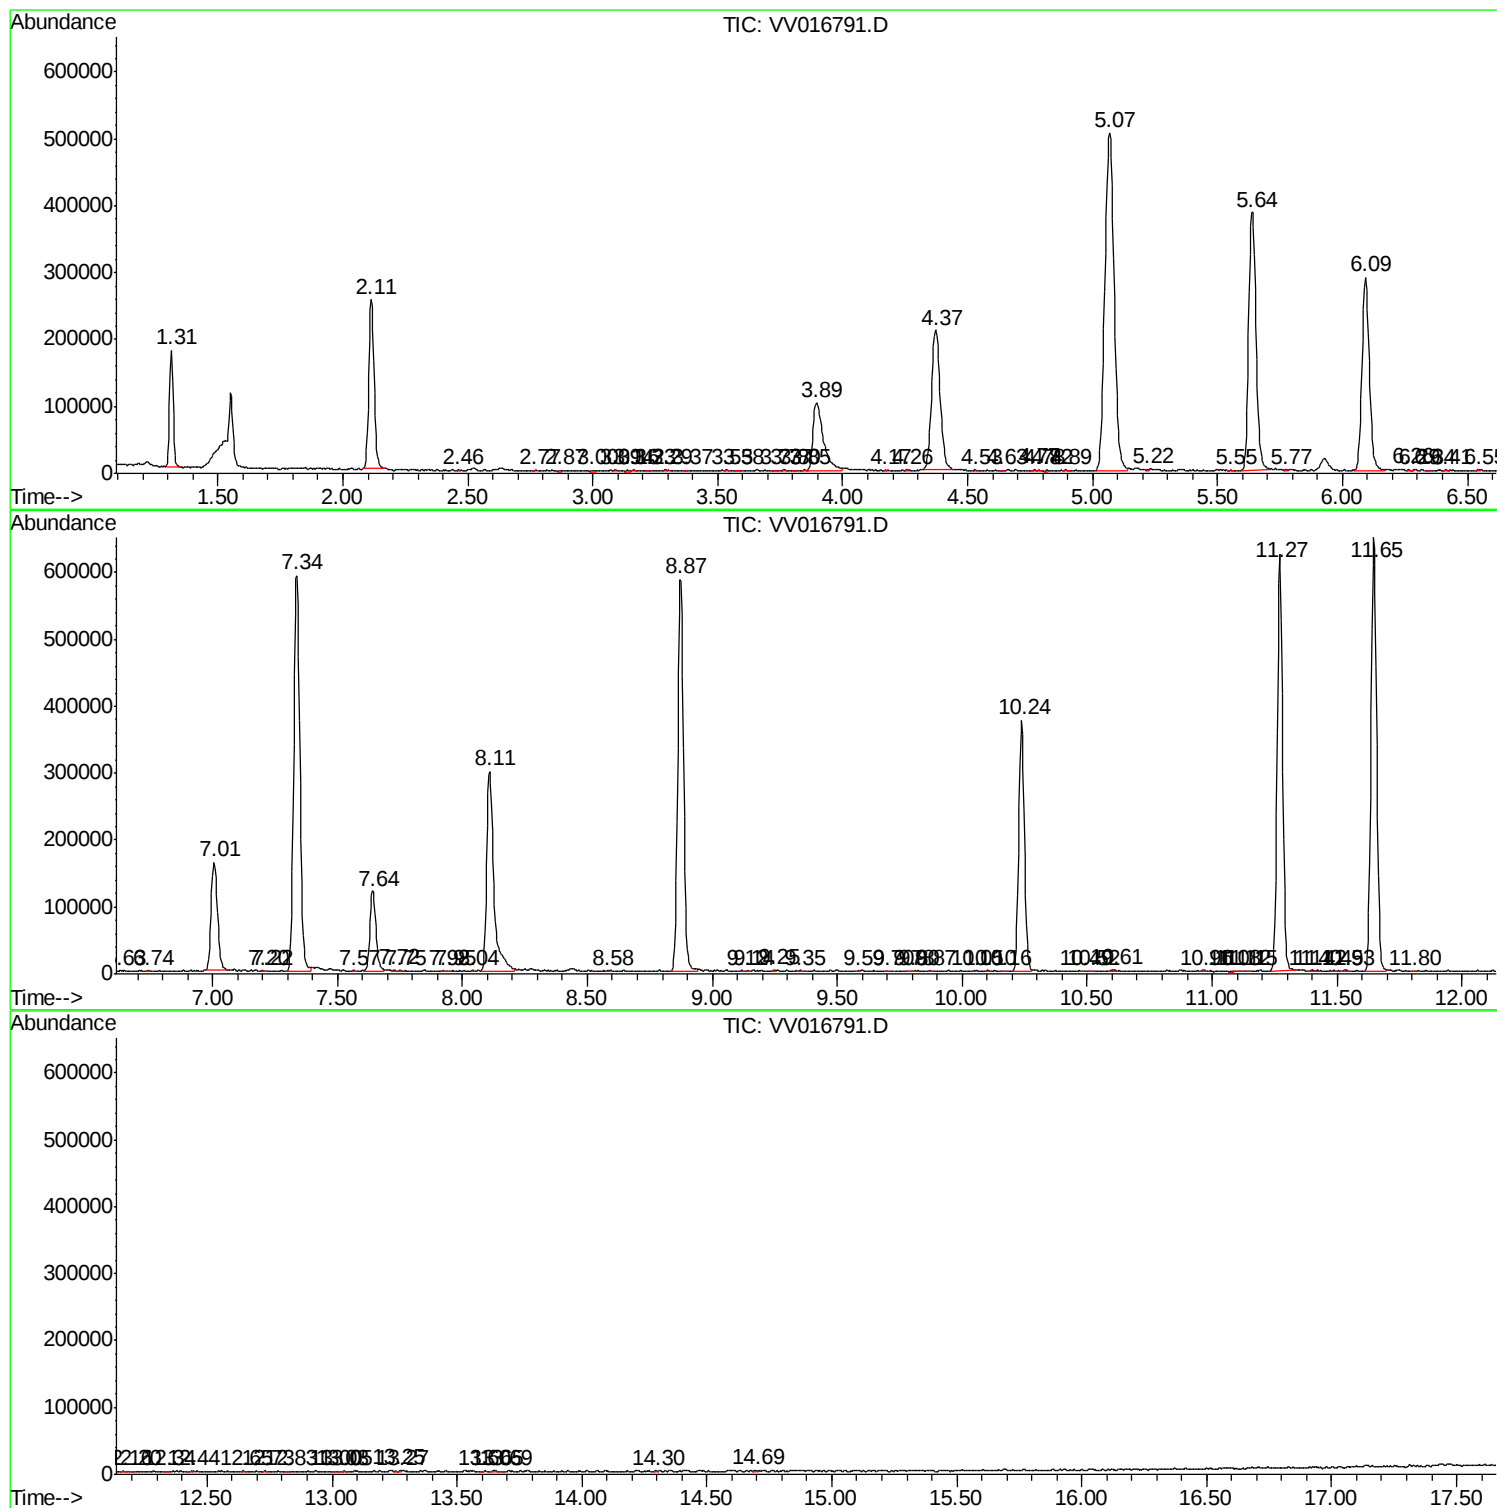

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV061020\
Data File : VV016791.D
Acq On : 11 Jun 2020 00:23
Operator : SY/MD
Sample : L2929-05 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTW3

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV061020\
Data File : VV016791.D
Acq On : 11 Jun 2020 00:23
Operator : SY/MD
Sample : L2929-05 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTW3

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc