

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061020\
 Data File : VV016792.D
 Acq On : 11 Jun 2020 00:46
 Operator : SY/MD
 Sample : L2929-06 100X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTW4

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.312	64	69	84	rVB	168899	170444	13.43%	1.763%
2	1.556	139	145	160	rVB	111865	135730	10.69%	1.404%
3	2.116	309	319	342	rVB	252261	379829	29.92%	3.928%
4	2.618	472	475	476	rBV4	1704	1033	0.08%	0.011%
5	2.698	497	500	502	rBV2	1084	575	0.05%	0.006%
6	2.711	502	504	509	rBV5	1969	1259	0.10%	0.013%
7	2.736	509	512	515	rBV5	2131	1408	0.11%	0.015%
8	2.923	568	570	571	rBV	1105	576	0.05%	0.006%
9	2.987	586	590	594	rBV7	2134	1444	0.11%	0.015%
10	3.061	611	613	616	rVB4	1416	675	0.05%	0.007%
11	3.222	662	663	665	rBV2	1559	751	0.06%	0.008%
12	3.251	671	672	674	rBV2	726	330	0.03%	0.003%
13	3.335	696	698	703	rBV5	1943	1386	0.11%	0.014%
14	3.608	781	783	787	rBV3	984	503	0.04%	0.005%
15	3.663	798	800	802	rBV4	1487	752	0.06%	0.008%
16	3.810	842	846	848	rBV4	1538	1469	0.12%	0.015%
17	3.897	862	873	896	rBV2	101138	277912	21.89%	2.874%
18	4.283	990	993	995	rBV3	1485	704	0.06%	0.007%
19	4.373	1003	1021	1040	rBV	206835	507247	39.96%	5.246%
20	4.563	1078	1080	1081	rBV2	1352	485	0.04%	0.005%
21	4.608	1093	1094	1095	rBV	1122	345	0.03%	0.004%
22	4.778	1144	1147	1150	rVB4	1332	912	0.07%	0.009%
23	4.826	1160	1162	1169	rVB6	2311	1651	0.13%	0.017%
24	4.862	1169	1173	1174	rBV4	2908	1736	0.14%	0.018%
25	4.971	1205	1207	1209	rBV3	1292	568	0.04%	0.006%
26	5.068	1221	1237	1259	rBV2	497589	1269537	100.00%	13.130%
27	5.640	1402	1415	1435	rBV	371705	751956	59.23%	7.777%
28	6.093	1543	1556	1581	rVB	285091	580822	45.75%	6.007%
29	6.328	1627	1629	1632	rBV3	1915	1114	0.09%	0.012%
30	6.505	1683	1684	1685	rBV	1315	394	0.03%	0.004%
31	6.961	1823	1826	1829	rBV4	1534	1415	0.11%	0.015%
32	7.006	1829	1840	1855	rVV	158929	285024	22.45%	2.948%
33	7.170	1889	1891	1892	rBV2	1151	490	0.04%	0.005%
34	7.196	1897	1899	1900	rBV2	2197	931	0.07%	0.010%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061020\
 Data File : VV016792.D
 Acq On : 11 Jun 2020 00:46
 Operator : SY/MD
 Sample : L2929-06 100X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTW4

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

35	7.238	1905	1912	1914	rBV7	1675	1738	0.14%	0.018%
36	7.338	1931	1943	1963	rBV	587093	1006280	79.26%	10.407%
37	7.640	2028	2037	2054	rBV2	113269	188736	14.87%	1.952%
38	7.804	2085	2088	2090	rBV4	1495	1216	0.10%	0.013%
39	7.858	2103	2105	2106	rVB2	1483	380	0.03%	0.004%
40	7.868	2106	2108	2109	rBV	1983	1096	0.09%	0.011%
41	8.032	2156	2159	2160	rBV3	1266	791	0.06%	0.008%
42	8.106	2172	2182	2215	rBV2	297778	592379	46.66%	6.126%
43	8.530	2310	2314	2318	rBV6	1772	1527	0.12%	0.016%
44	8.592	2331	2333	2336	rBV3	1348	872	0.07%	0.009%
45	8.765	2385	2387	2390	rVB4	1577	723	0.06%	0.007%
46	8.820	2403	2404	2405	rBV	961	349	0.03%	0.004%
47	8.871	2409	2420	2438	rVV	561976	920208	72.48%	9.517%
48	9.122	2495	2498	2499	rBV3	1567	978	0.08%	0.010%
49	9.157	2504	2509	2513	rBV7	1618	1760	0.14%	0.018%
50	9.334	2561	2564	2568	rVB6	1927	1228	0.10%	0.013%
51	9.357	2568	2571	2574	rBV4	1925	1261	0.10%	0.013%
52	9.405	2584	2586	2588	rBV3	1386	622	0.05%	0.006%
53	9.418	2588	2590	2592	rBV2	1469	834	0.07%	0.009%
54	9.646	2658	2661	2663	rBV3	1032	583	0.05%	0.006%
55	9.710	2677	2681	2684	rBV5	1712	1544	0.12%	0.016%
56	9.794	2705	2707	2710	rVB3	1381	538	0.04%	0.006%
57	9.887	2735	2736	2738	rBV2	1119	489	0.04%	0.005%
58	10.022	2774	2778	2781	rBV6	1672	1547	0.12%	0.016%
59	10.122	2806	2809	2810	rBV3	1659	968	0.08%	0.010%
60	10.180	2824	2827	2830	rVB5	2178	1247	0.10%	0.013%
61	10.238	2830	2845	2862	rBV	381429	596471	46.98%	6.169%
62	10.386	2887	2891	2895	rBV6	2056	2324	0.18%	0.024%
63	10.698	2985	2988	2990	rBV4	1286	673	0.05%	0.007%
64	10.736	2998	3000	3003	rBV3	847	589	0.05%	0.006%
65	10.839	3028	3032	3035	rVB5	1012	725	0.06%	0.007%
66	10.910	3052	3054	3060	rBV8	1206	899	0.07%	0.009%
67	11.029	3089	3091	3095	rBV5	1391	1238	0.10%	0.013%
68	11.074	3103	3105	3108	rBV4	1223	945	0.07%	0.010%
69	11.106	3112	3115	3119	rBV4	1885	1524	0.12%	0.016%
70	11.157	3129	3131	3133	rVB3	1482	497	0.04%	0.005%
71	11.212	3145	3148	3150	rBV4	1109	775	0.06%	0.008%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061020\
 Data File : VV016792.D
 Acq On : 11 Jun 2020 00:46
 Operator : SY/MD
 Sample : L2929-06 100X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTW4

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

72	11.270	3154	3166	3181	rBV	599042	912795	71.90%	9.440%
73	11.527	3243	3246	3247	rBV3	1176	618	0.05%	0.006%
74	11.646	3271	3283	3301	rBV	652484	1010804	79.62%	10.454%
75	11.862	3349	3350	3352	rBV2	762	325	0.03%	0.003%
76	11.874	3352	3354	3359	rVV4	2092	1873	0.15%	0.019%
77	11.919	3366	3368	3372	rBV4	1035	662	0.05%	0.007%
78	11.968	3380	3383	3386	rBV3	1260	1125	0.09%	0.012%
79	12.077	3415	3417	3421	rBV5	904	734	0.06%	0.008%
80	12.122	3428	3431	3432	rBV3	1065	693	0.05%	0.007%
81	12.128	3432	3433	3436	rVB3	1179	594	0.05%	0.006%
82	12.292	3482	3484	3486	rBV3	1320	677	0.05%	0.007%
83	12.325	3491	3494	3496	rBV4	1840	1174	0.09%	0.012%
84	12.447	3530	3532	3534	rVB3	1291	502	0.04%	0.005%
85	12.463	3534	3537	3539	rBV3	1085	540	0.04%	0.006%
86	12.534	3556	3559	3565	rVB8	1797	1838	0.14%	0.019%
87	12.804	3641	3643	3649	rVB6	1607	1323	0.10%	0.014%
88	13.109	3737	3738	3744	rVB5	1754	1413	0.11%	0.015%
89	13.218	3770	3772	3773	rBV2	1619	463	0.04%	0.005%
90	13.254	3780	3783	3786	rBV5	1454	968	0.08%	0.010%
91	13.595	3887	3889	3892	rBV3	1602	937	0.07%	0.010%
92	13.810	3953	3956	3961	rBV6	1487	1275	0.10%	0.013%
93	13.865	3971	3973	3976	rBV4	1351	664	0.05%	0.007%
94	13.939	3992	3996	3998	rVB3	1670	1080	0.09%	0.011%
95	14.112	4048	4050	4055	rBV5	1499	1266	0.10%	0.013%
96	14.202	4075	4078	4079	rBV3	1577	912	0.07%	0.009%
97	14.418	4142	4145	4149	rBV5	2191	1569	0.12%	0.016%
98	14.845	4276	4278	4281	rBV4	2072	929	0.07%	0.010%
99	14.987	4318	4322	4324	rBV4	1840	1556	0.12%	0.016%
100	15.183	4377	4383	4384	rBV5	1895	1859	0.15%	0.019%


Sum of corrected areas: 9669129

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV061020\
Data File : VV016792.D
Acq On : 11 Jun 2020 00:46
Operator : SY/MD
Sample : L2929-06 100X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTW4

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

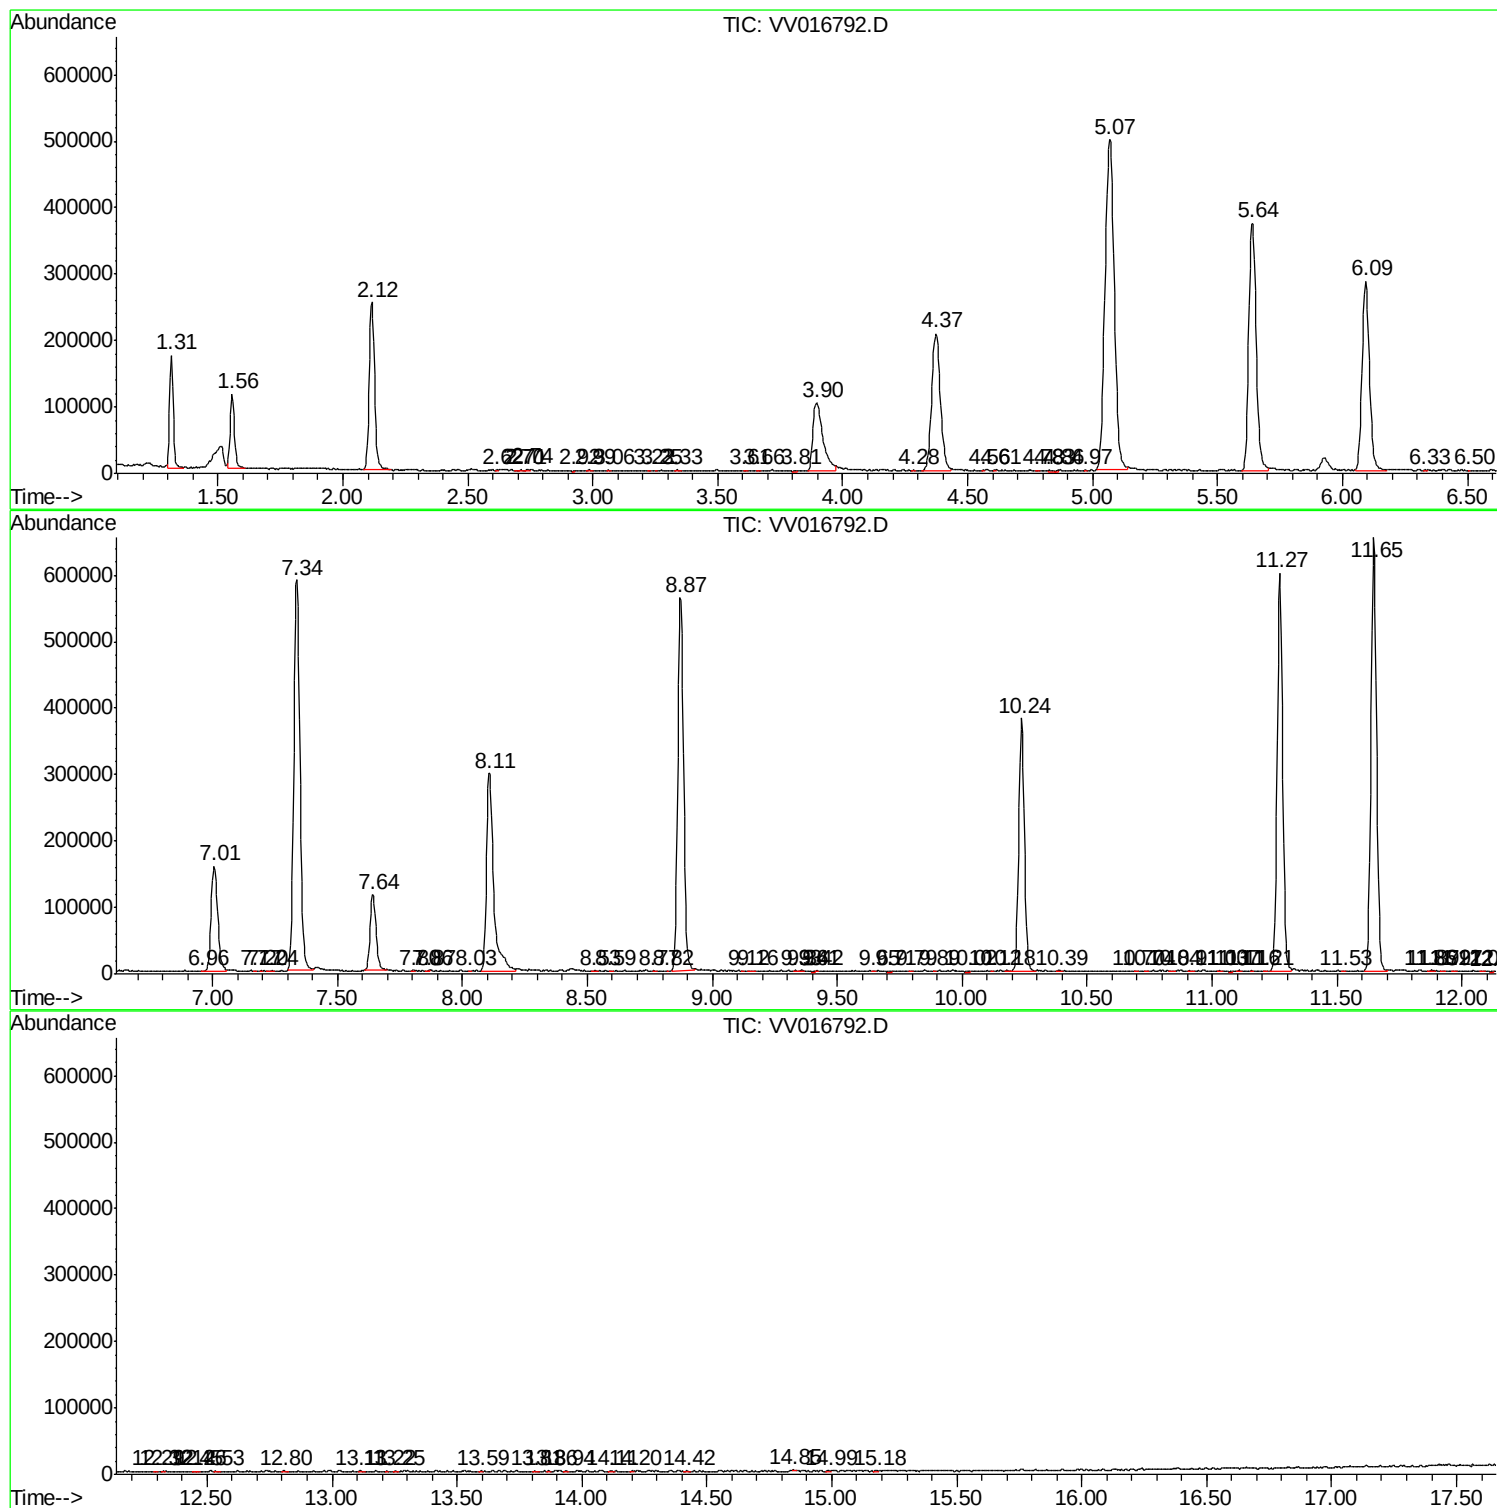

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV061020\
Data File : VV016792.D
Acq On : 11 Jun 2020 00:46
Operator : SY/MD
Sample : L2929-06 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTW4

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV061020\
Data File : VV016792.D
Acq On : 11 Jun 2020 00:46
Operator : SY/MD
Sample : L2929-06 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTW4

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc