

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061020\
 Data File : VV016793.D
 Acq On : 11 Jun 2020 01:10
 Operator : SY/MD
 Sample : L2929-07 100X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTW6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	63	70	78	rBV	163639	161952	12.55%	1.646%
2	1.556	139	145	157	rVB	111174	133540	10.34%	1.357%
3	2.116	310	319	337	rVB	255710	375587	29.09%	3.816%
4	2.228	351	354	358	rBV4	1976	1544	0.12%	0.016%
5	2.380	397	401	407	rVB8	1810	2195	0.17%	0.022%
6	2.418	408	413	414	rBV4	1063	857	0.07%	0.009%
7	2.515	434	443	444	rBV7	3494	3104	0.24%	0.032%
8	2.827	536	540	542	rBV4	1373	1109	0.09%	0.011%
9	2.872	552	554	556	rBV3	1691	930	0.07%	0.009%
10	3.138	633	637	639	rBV5	1479	1192	0.09%	0.012%
11	3.325	690	695	701	rBV9	1646	2437	0.19%	0.025%
12	3.399	715	718	721	rVB4	1698	1094	0.08%	0.011%
13	3.595	776	779	781	rBV4	1655	1025	0.08%	0.010%
14	3.637	788	792	796	rVB7	1446	1156	0.09%	0.012%
15	3.663	796	800	805	rBV6	2121	2496	0.19%	0.025%
16	3.846	854	857	858	rBV3	1716	962	0.07%	0.010%
17	3.894	862	872	907	rVV2	103400	297061	23.01%	3.019%
18	4.232	975	977	980	rBV4	1464	820	0.06%	0.008%
19	4.280	988	992	994	rBV4	1610	1230	0.10%	0.012%
20	4.373	1004	1021	1041	rBV	211269	516354	40.00%	5.247%
21	4.720	1125	1129	1130	rBV4	1099	730	0.06%	0.007%
22	4.804	1151	1155	1156	rBV3	1417	787	0.06%	0.008%
23	4.990	1209	1213	1217	rBV7	1706	1494	0.12%	0.015%
24	5.068	1217	1237	1264	rBV2	500581	1290955	100.00%	13.118%
25	5.376	1328	1333	1334	rBV5	1168	822	0.06%	0.008%
26	5.640	1400	1415	1433	rBV	392094	785174	60.82%	7.978%
27	6.093	1543	1556	1578	rBV	289243	582155	45.09%	5.915%
28	6.318	1624	1626	1631	rBV4	1264	829	0.06%	0.008%
29	6.453	1664	1668	1671	rBV4	1312	1337	0.10%	0.014%
30	6.537	1689	1694	1696	rBV5	1390	1157	0.09%	0.012%
31	6.720	1745	1751	1754	rBV7	1474	1601	0.12%	0.016%
32	6.775	1765	1768	1769	rVV3	1544	745	0.06%	0.008%
33	6.807	1775	1778	1779	rBV3	1705	1040	0.08%	0.011%
34	7.006	1828	1840	1861	rBV	163737	294153	22.79%	2.989%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061020\
 Data File : VV016793.D
 Acq On : 11 Jun 2020 01:10
 Operator : SY/MD
 Sample : L2929-07 100X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTW6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

35	7.148	1881	1884	1887	rVB3	1795	1126	0.09%	0.011%
36	7.228	1907	1909	1913	rVB4	2470	1705	0.13%	0.017%
37	7.248	1913	1915	1916	rBV2	1572	724	0.06%	0.007%
38	7.338	1929	1943	1961	rBV	585580	1021367	79.12%	10.378%
39	7.640	2028	2037	2053	rBV	113309	189844	14.71%	1.929%
40	7.772	2074	2078	2079	rBV4	1549	799	0.06%	0.008%
41	7.810	2087	2090	2092	rVB4	1586	843	0.07%	0.009%
42	7.961	2132	2137	2140	rBV6	2198	2099	0.16%	0.021%
43	8.010	2149	2152	2154	rBV3	1986	1204	0.09%	0.012%
44	8.109	2171	2183	2210	rBV2	296164	593237	45.95%	6.028%
45	8.723	2372	2374	2376	rBV3	1272	764	0.06%	0.008%
46	8.746	2376	2381	2384	rVV6	1338	1192	0.09%	0.012%
47	8.875	2408	2421	2441	rBV	595029	963493	74.63%	9.790%
48	9.048	2473	2475	2477	rBV3	1545	741	0.06%	0.008%
49	9.096	2486	2490	2493	rBV6	2263	2294	0.18%	0.023%
50	9.148	2503	2506	2508	rBV4	1751	904	0.07%	0.009%
51	9.264	2539	2542	2548	rVB7	1793	1594	0.12%	0.016%
52	9.289	2548	2550	2552	rBV3	1633	841	0.07%	0.009%
53	9.444	2595	2598	2604	rBV6	1621	1893	0.15%	0.019%
54	9.473	2604	2607	2611	rVV5	987	887	0.07%	0.009%
55	9.514	2615	2620	2621	rBV5	1596	925	0.07%	0.009%
56	9.566	2634	2636	2639	rVB3	2490	1300	0.10%	0.013%
57	9.675	2669	2670	2676	rVB5	1122	1072	0.08%	0.011%
58	9.739	2688	2690	2693	rBV3	1810	1057	0.08%	0.011%
59	9.788	2702	2705	2710	rBV7	1472	1076	0.08%	0.011%
60	9.820	2713	2715	2719	rBV4	958	756	0.06%	0.008%
61	9.862	2722	2728	2730	rBV7	1596	1271	0.10%	0.013%
62	9.884	2730	2735	2737	rBV3	1847	1179	0.09%	0.012%
63	10.096	2798	2801	2804	rVV4	1392	992	0.08%	0.010%
64	10.238	2834	2845	2861	rVB	370401	587740	45.53%	5.972%
65	10.337	2873	2876	2879	rBV4	1602	1398	0.11%	0.014%
66	10.485	2919	2922	2926	rBV5	1564	1022	0.08%	0.010%
67	10.691	2981	2986	2987	rBV3	1483	1108	0.09%	0.011%
68	10.752	3003	3005	3011	rVB7	1623	1436	0.11%	0.015%
69	10.813	3020	3024	3026	rBV5	1350	1077	0.08%	0.011%
70	11.090	3106	3110	3112	rVB5	1584	1018	0.08%	0.010%
71	11.164	3131	3133	3135	rBV3	1624	899	0.07%	0.009%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061020\
 Data File : VV016793.D
 Acq On : 11 Jun 2020 01:10
 Operator : SY/MD
 Sample : L2929-07 100X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTW6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

72	11.180	3135	3138	3141	rVB5	1745	1227	0.10%	0.012%
73	11.270	3156	3166	3183	rVB	609311	930924	72.11%	9.459%
74	11.646	3271	3283	3298	rBV	642665	1012108	78.40%	10.284%
75	11.855	3345	3348	3351	rBV5	1629	1173	0.09%	0.012%
76	11.878	3351	3355	3357	rVV4	1380	910	0.07%	0.009%
77	11.890	3357	3359	3367	rVB9	2088	2072	0.16%	0.021%
78	11.935	3370	3373	3375	rBV4	1828	1254	0.10%	0.013%
79	11.977	3381	3386	3389	rBV6	1379	1179	0.09%	0.012%
80	12.016	3395	3398	3403	rBV7	1374	1518	0.12%	0.015%
81	12.231	3463	3465	3470	rBV4	1034	1008	0.08%	0.010%
82	12.347	3499	3501	3506	rVB6	1372	982	0.08%	0.010%
83	12.373	3506	3509	3512	rBV4	1547	1286	0.10%	0.013%
84	12.402	3517	3518	3521	rBV3	1257	803	0.06%	0.008%
85	12.440	3527	3530	3534	rVB4	1381	978	0.08%	0.010%
86	12.469	3534	3539	3543	rVB7	1221	1099	0.09%	0.011%
87	12.614	3578	3584	3586	rBV7	1469	1421	0.11%	0.014%
88	12.653	3593	3596	3597	rBV3	2070	1505	0.12%	0.015%
89	13.363	3813	3817	3820	rBV5	1369	1366	0.11%	0.014%
90	13.453	3841	3845	3846	rBV3	2121	1356	0.11%	0.014%
91	13.505	3858	3861	3862	rBV2	2097	1108	0.09%	0.011%
92	13.697	3913	3921	3924	rBV7	3026	3144	0.24%	0.032%
93	13.884	3975	3979	3982	rBV4	1978	1936	0.15%	0.020%
94	14.070	4034	4037	4041	rBV5	1570	1234	0.10%	0.013%
95	14.241	4087	4090	4093	rBV5	1883	1168	0.09%	0.012%
96	14.414	4143	4144	4149	rBV4	1565	929	0.07%	0.009%
97	14.537	4179	4182	4186	rBV5	1120	914	0.07%	0.009%
98	14.588	4193	4198	4200	rBV5	1732	1765	0.14%	0.018%
99	14.636	4211	4213	4217	rBV5	1348	978	0.08%	0.010%
100	15.337	4427	4431	4432	rBV4	2112	1397	0.11%	0.014%


Sum of corrected areas: 9841243

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV061020\
Data File : VV016793.D
Acq On : 11 Jun 2020 01:10
Operator : SY/MD
Sample : L2929-07 100X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTW6

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

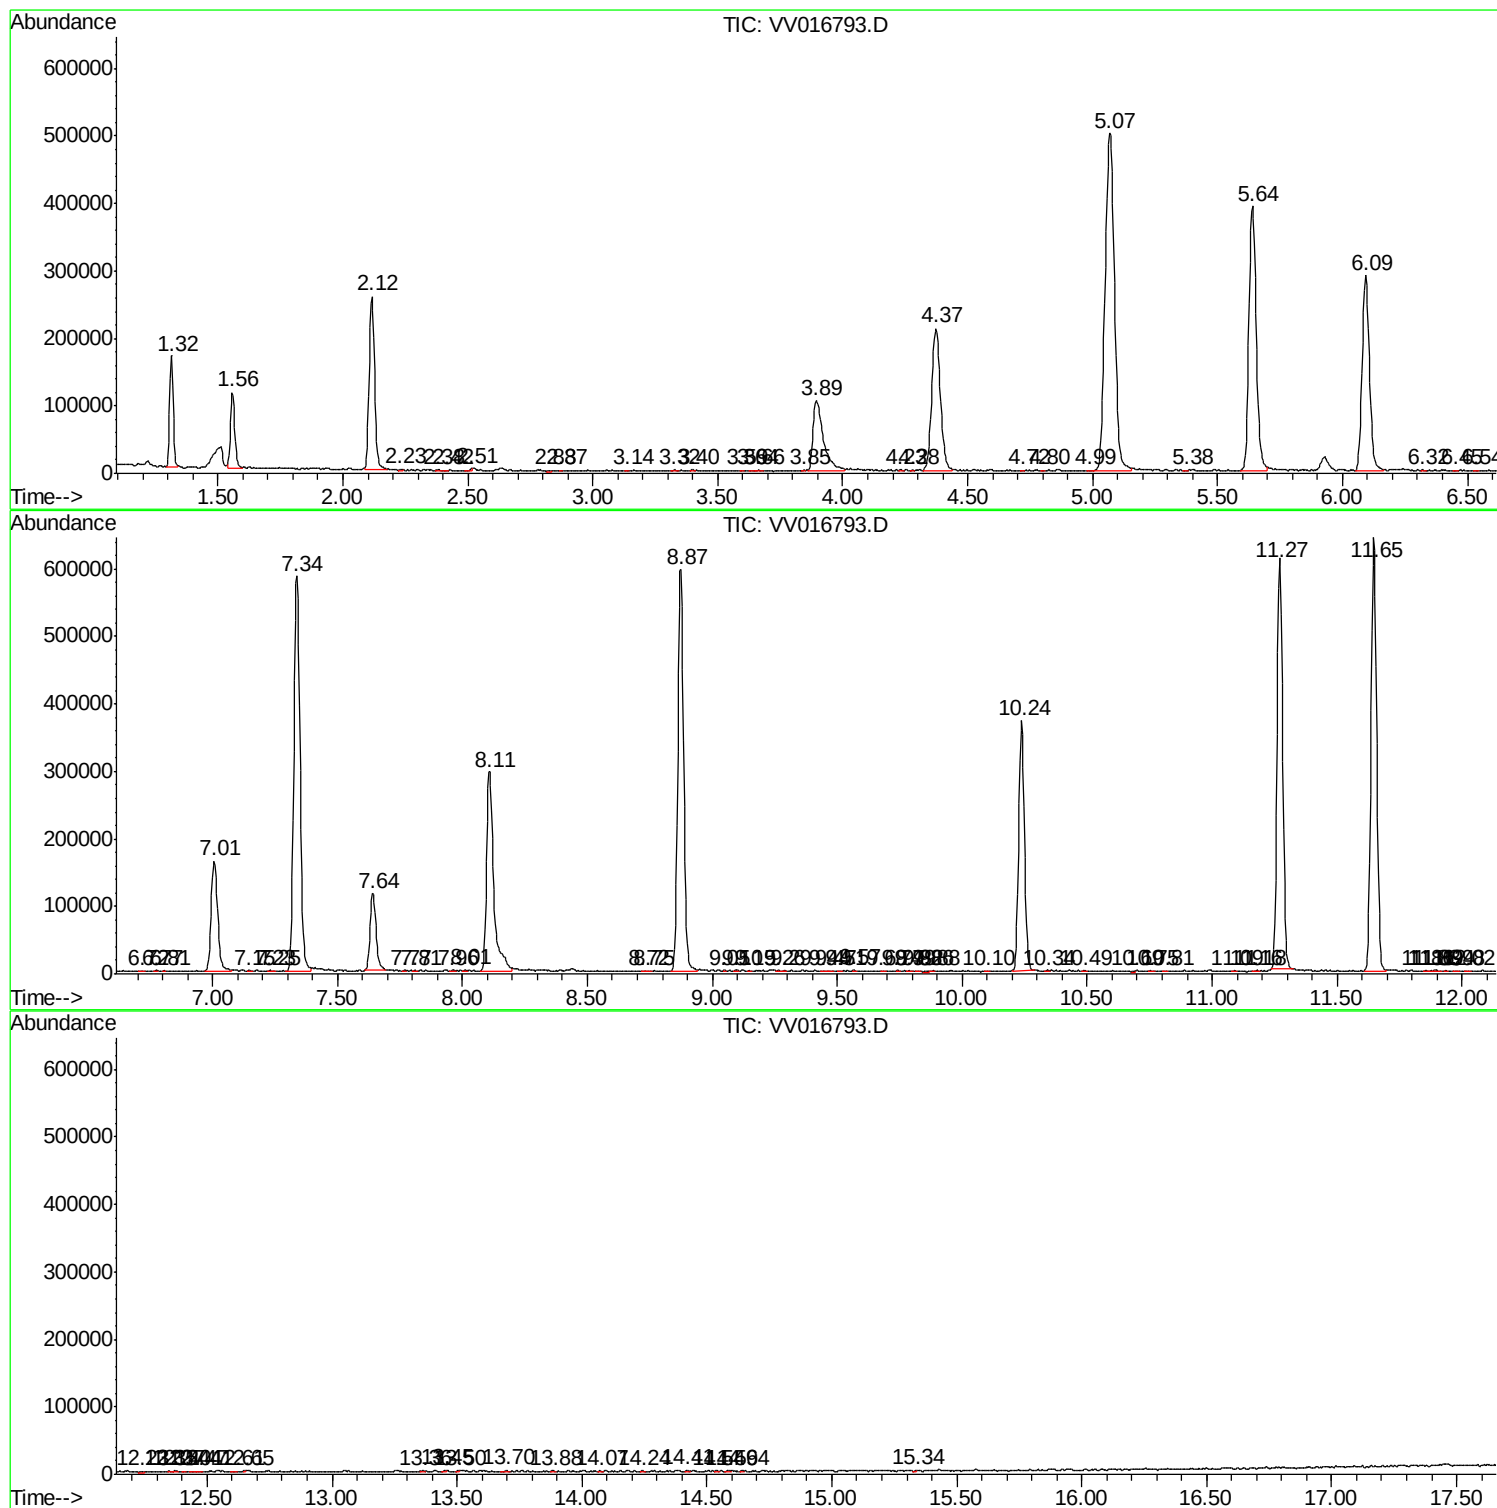

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV061020\
Data File : VV016793.D
Acq On : 11 Jun 2020 01:10
Operator : SY/MD
Sample : L2929-07 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTW6

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV061020\
Data File : VV016793.D
Acq On : 11 Jun 2020 01:10
Operator : SY/MD
Sample : L2929-07 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTW6

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc