

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061020\
 Data File : VV016794.D
 Acq On : 11 Jun 2020 01:34
 Operator : SY/MD
 Sample : L2929-08 100X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTW7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.312	64	69	83	rVB	164463	166041	13.18%	1.751%
2	1.557	139	145	155	rVB	109835	128502	10.20%	1.355%
3	2.113	308	318	334	rBV	245193	371834	29.51%	3.922%
4	2.759	515	519	524	rBV8	1679	1970	0.16%	0.021%
5	2.952	577	579	581	rBV3	1618	810	0.06%	0.009%
6	2.981	586	588	589	rBV2	1094	613	0.05%	0.006%
7	3.100	623	625	629	rVB4	1950	1094	0.09%	0.012%
8	3.132	629	635	638	rBV7	2218	1930	0.15%	0.020%
9	3.463	734	738	741	rBV4	1355	1371	0.11%	0.014%
10	3.553	764	766	770	rVB5	1287	710	0.06%	0.007%
11	3.579	773	774	778	rVB4	1451	647	0.05%	0.007%
12	3.598	778	780	783	rBV4	1060	850	0.07%	0.009%
13	3.756	827	829	833	rVB3	1525	755	0.06%	0.008%
14	3.827	847	851	852	rBV4	1294	850	0.07%	0.009%
15	3.840	852	855	857	rBV4	1914	1161	0.09%	0.012%
16	3.894	862	872	904	rVV	99243	285083	22.62%	3.007%
17	4.139	945	948	950	rBV3	1551	869	0.07%	0.009%
18	4.312	999	1002	1005	rBV4	1513	1301	0.10%	0.014%
19	4.370	1005	1020	1041	rVV2	204142	509960	40.47%	5.379%
20	4.537	1070	1072	1075	rBV4	1449	807	0.06%	0.009%
21	4.611	1091	1095	1096	rBV4	1660	1134	0.09%	0.012%
22	4.685	1115	1118	1123	rBV6	1912	1686	0.13%	0.018%
23	4.759	1138	1141	1144	rBV5	1720	1449	0.11%	0.015%
24	4.785	1147	1149	1153	rVV5	1136	869	0.07%	0.009%
25	4.936	1194	1196	1199	rBV4	1384	870	0.07%	0.009%
26	4.981	1208	1210	1214	rVB4	1315	923	0.07%	0.010%
27	5.003	1214	1217	1219	rBV3	1409	831	0.07%	0.009%
28	5.068	1221	1237	1261	rVV2	492690	1260061	100.00%	13.291%
29	5.386	1333	1336	1339	rBV3	1215	1003	0.08%	0.011%
30	5.640	1402	1415	1434	rBV	355527	714906	56.74%	7.541%
31	5.923	1495	1503	1518	rBV4	17315	35641	2.83%	0.376%
32	6.093	1543	1556	1575	rVB	280776	563551	44.72%	5.944%
33	6.341	1631	1633	1636	rBV4	1742	1118	0.09%	0.012%
34	6.421	1656	1658	1660	rBV3	1241	737	0.06%	0.008%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061020\
 Data File : VV016794.D
 Acq On : 11 Jun 2020 01:34
 Operator : SY/MD
 Sample : L2929-08 100X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTW7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

35	6.540	1690	1695	1698	rBV7	1771	1999	0.16%	0.021%
36	6.621	1718	1720	1722	rVB3	1640	641	0.05%	0.007%
37	6.650	1725	1729	1731	rBV5	2221	1436	0.11%	0.015%
38	6.704	1743	1746	1750	rBV5	1778	1342	0.11%	0.014%
39	7.007	1829	1840	1859	rBV	156430	278692	22.12%	2.940%
40	7.142	1878	1882	1884	rBV4	1518	903	0.07%	0.010%
41	7.235	1909	1911	1914	rBV3	1096	625	0.05%	0.007%
42	7.338	1926	1943	1965	rBV	573194	1015434	80.59%	10.710%
43	7.585	2017	2020	2023	rBV4	1501	1016	0.08%	0.011%
44	7.640	2028	2037	2051	rVV	113394	186553	14.81%	1.968%
45	7.753	2069	2072	2073	rBV3	1420	764	0.06%	0.008%
46	8.061	2166	2168	2170	rBV3	1237	658	0.05%	0.007%
47	8.109	2172	2183	2215	rVV2	292074	582148	46.20%	6.140%
48	8.347	2253	2257	2259	rBV5	1285	1220	0.10%	0.013%
49	8.585	2327	2331	2332	rBV3	1052	747	0.06%	0.008%
50	8.704	2366	2368	2372	rVB5	2199	1243	0.10%	0.013%
51	8.736	2376	2378	2381	rVV3	1478	775	0.06%	0.008%
52	8.814	2397	2402	2403	rBV4	1907	1674	0.13%	0.018%
53	8.872	2409	2420	2437	rBV	530811	860744	68.31%	9.079%
54	9.081	2483	2485	2488	rBV4	1865	1268	0.10%	0.013%
55	9.193	2518	2520	2523	rBV4	1198	714	0.06%	0.008%
56	9.302	2552	2554	2561	rBV6	1443	1170	0.09%	0.012%
57	9.335	2561	2564	2565	rBV3	1335	797	0.06%	0.008%
58	9.492	2611	2613	2615	rBV3	1072	636	0.05%	0.007%
59	9.569	2635	2637	2640	rBV4	1624	762	0.06%	0.008%
60	9.634	2653	2657	2659	rBV4	1750	1189	0.09%	0.013%
61	9.691	2670	2675	2678	rBV5	1799	1946	0.15%	0.021%
62	9.897	2736	2739	2741	rBV4	2210	1509	0.12%	0.016%
63	10.019	2774	2777	2781	rVB4	1827	1077	0.09%	0.011%
64	10.061	2787	2790	2792	rBV3	1564	803	0.06%	0.008%
65	10.129	2809	2811	2813	rBV3	1105	608	0.05%	0.006%
66	10.238	2833	2845	2866	rVB	363087	578365	45.90%	6.100%
67	10.476	2917	2919	2922	rBV3	1159	832	0.07%	0.009%
68	10.679	2979	2982	2984	rBV3	1563	1050	0.08%	0.011%
69	10.862	3034	3039	3040	rBV5	1981	1420	0.11%	0.015%
70	10.926	3057	3059	3062	rBV4	1053	811	0.06%	0.009%
71	10.955	3067	3068	3071	rBV3	1267	835	0.07%	0.009%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061020\
 Data File : VV016794.D
 Acq On : 11 Jun 2020 01:34
 Operator : SY/MD
 Sample : L2929-08 100X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTW7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

72	11.042	3092	3095	3099	rBV5	1333	1200	0.10%	0.013%
73	11.193	3140	3142	3144	rBV3	1509	857	0.07%	0.009%
74	11.270	3154	3166	3180	rBV	556189	849321	67.40%	8.958%
75	11.431	3214	3216	3219	rBV3	1807	1370	0.11%	0.014%
76	11.527	3244	3246	3248	rVB3	1521	754	0.06%	0.008%
77	11.646	3269	3283	3301	rVV	640134	1006272	79.86%	10.614%
78	11.772	3319	3322	3326	rBV5	2242	1758	0.14%	0.019%
79	11.974	3383	3385	3388	rVB3	1614	665	0.05%	0.007%
80	12.084	3416	3419	3424	rVB7	1692	1627	0.13%	0.017%
81	12.203	3454	3456	3460	rBV4	972	899	0.07%	0.009%
82	12.415	3517	3522	3524	rBV5	1254	1281	0.10%	0.014%
83	12.553	3563	3565	3568	rBV4	1353	1016	0.08%	0.011%
84	12.579	3571	3573	3576	rBV3	1547	1184	0.09%	0.012%
85	12.611	3580	3583	3584	rBV3	1232	688	0.05%	0.007%
86	12.842	3653	3655	3657	rBV3	1444	619	0.05%	0.007%
87	12.897	3670	3672	3674	rBV3	1874	1084	0.09%	0.011%
88	13.206	3766	3768	3770	rBV3	1992	805	0.06%	0.008%
89	13.360	3813	3816	3818	rBV3	1182	848	0.07%	0.009%
90	13.424	3833	3836	3838	rBV3	1348	831	0.07%	0.009%
91	13.498	3854	3859	3861	rBV5	1686	1414	0.11%	0.015%
92	13.656	3905	3908	3913	rVB6	1591	1496	0.12%	0.016%
93	13.739	3932	3934	3937	rBV3	1405	900	0.07%	0.009%
94	13.910	3983	3987	3989	rBV5	1503	1257	0.10%	0.013%
95	14.206	4075	4079	4082	rVB5	1146	921	0.07%	0.010%
96	14.309	4109	4111	4115	rVB5	1503	769	0.06%	0.008%
97	14.530	4178	4180	4183	rBV3	2038	1587	0.13%	0.017%
98	14.608	4202	4204	4207	rBV3	1674	998	0.08%	0.011%
99	14.711	4233	4236	4238	rBV4	1295	635	0.05%	0.007%
100	15.238	4397	4400	4402	rBV3	2289	1370	0.11%	0.014%


Sum of corrected areas: 9480769

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV061020\
Data File : VV016794.D
Acq On : 11 Jun 2020 01:34
Operator : SY/MD
Sample : L2929-08 100X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTW7

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

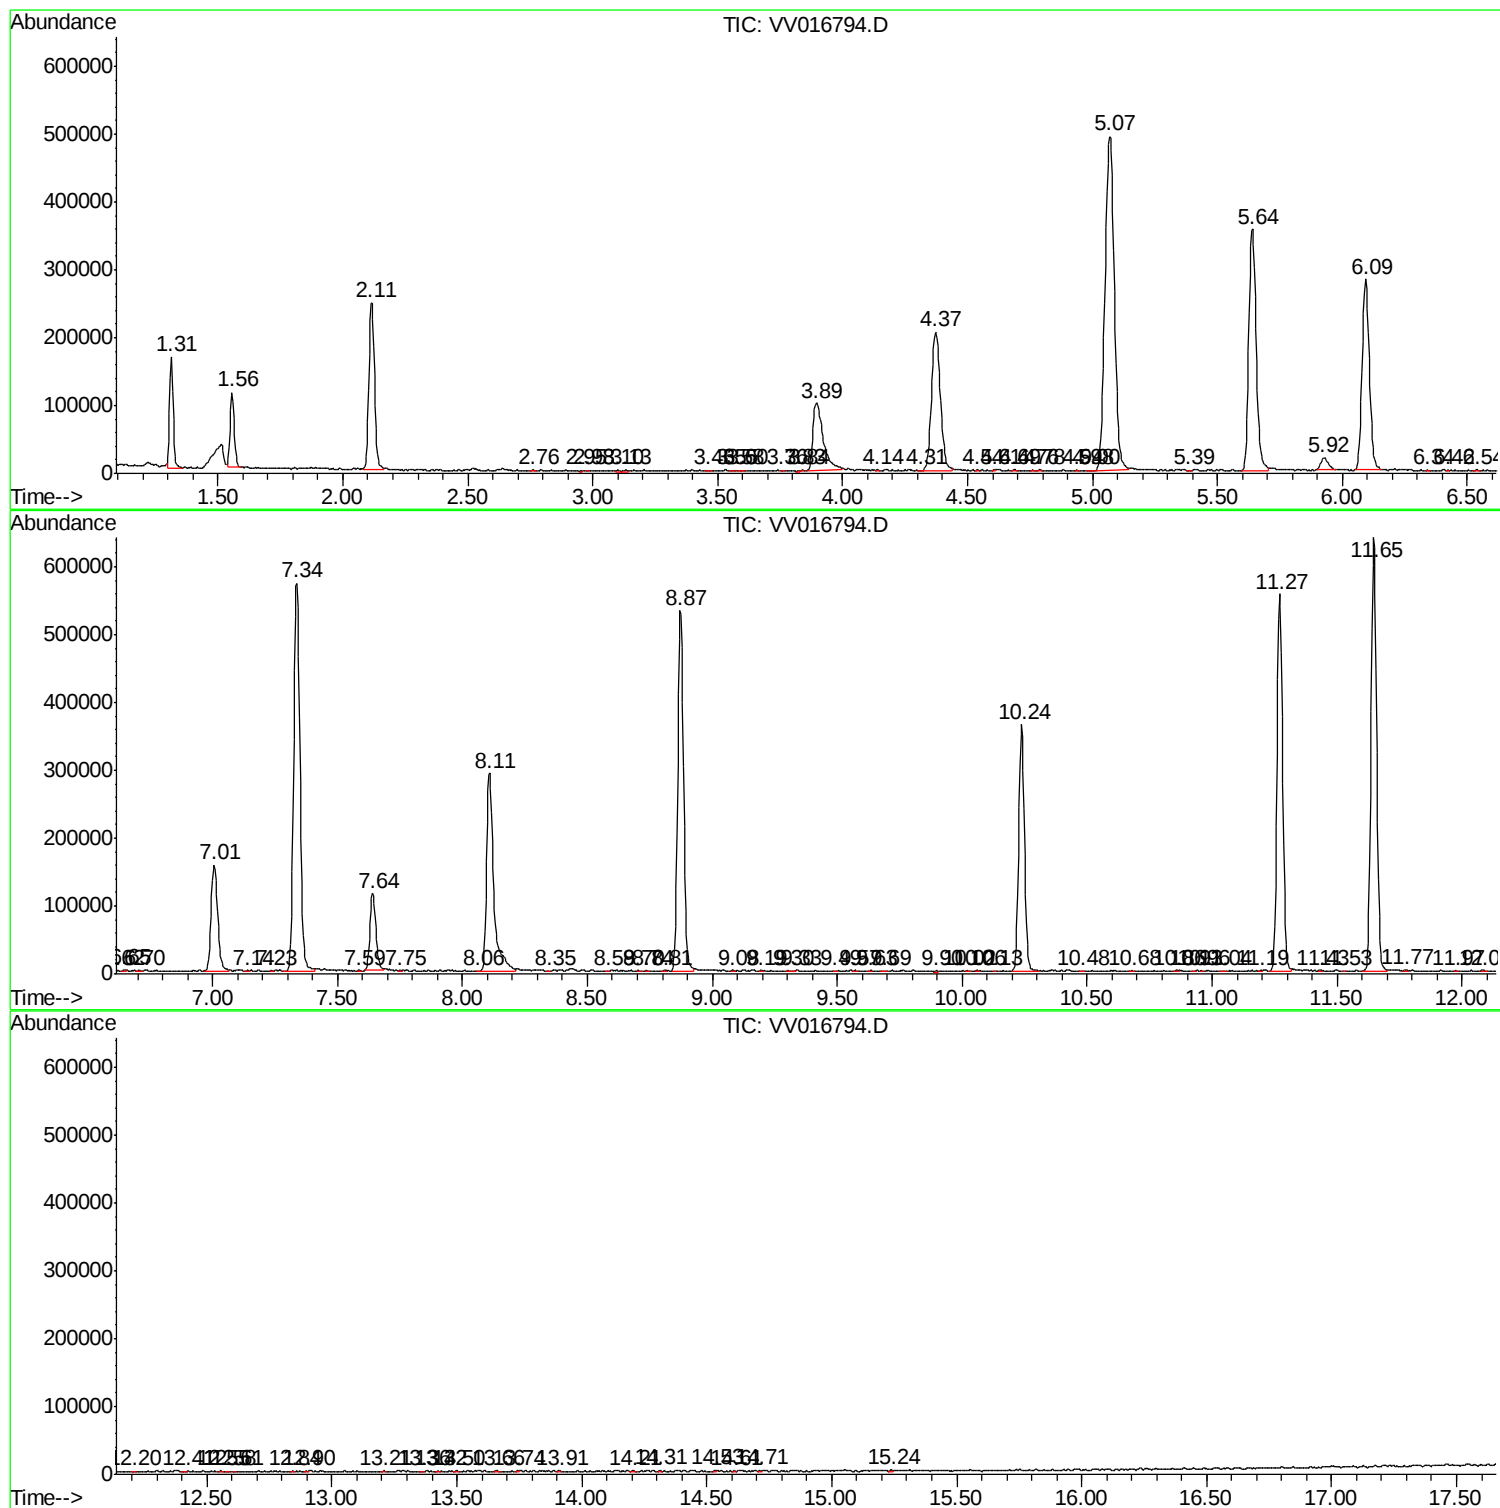

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV061020\
Data File : VV016794.D
Acq On : 11 Jun 2020 01:34
Operator : SY/MD
Sample : L2929-08 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTW7

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV061020\
Data File : VV016794.D
Acq On : 11 Jun 2020 01:34
Operator : SY/MD
Sample : L2929-08 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTW7

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc