

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061020\
 Data File : VV016796.D
 Acq On : 11 Jun 2020 02:22
 Operator : SY/MD
 Sample : L2929-10 100X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTW9

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.312	63	69	81	rVB	157326	155754	12.48%	1.646%
2	1.556	139	145	159	rVB	103184	125721	10.08%	1.329%
3	2.116	309	319	334	rBV	238294	357936	28.69%	3.783%
4	2.614	469	474	475	rBV4	3007	2456	0.20%	0.026%
5	2.855	545	549	551	rBV4	1317	1164	0.09%	0.012%
6	3.052	608	610	612	rBV3	1370	733	0.06%	0.008%
7	3.103	623	626	628	rVB4	1942	1144	0.09%	0.012%
8	3.122	628	632	635	rVB6	1543	1238	0.10%	0.013%
9	3.180	648	650	651	rBV2	1404	455	0.04%	0.005%
10	3.209	656	659	662	rBV5	1237	772	0.06%	0.008%
11	3.296	684	686	691	rVB6	1014	771	0.06%	0.008%
12	3.363	704	707	708	rBV2	1301	647	0.05%	0.007%
13	3.727	817	820	825	rBV6	1657	1590	0.13%	0.017%
14	3.820	847	849	850	rBV2	1191	457	0.04%	0.005%
15	3.894	863	872	898	rBV	95212	260270	20.86%	2.751%
16	4.280	989	992	993	rBV2	770	431	0.03%	0.005%
17	4.299	996	998	999	rBV2	1107	443	0.04%	0.005%
18	4.373	1007	1021	1039	rVB	197789	472788	37.89%	4.997%
19	4.502	1059	1061	1065	rBV4	1468	972	0.08%	0.010%
20	4.601	1088	1092	1096	rBV7	1621	1572	0.13%	0.017%
21	4.691	1117	1120	1124	rVB5	1727	1314	0.11%	0.014%
22	4.711	1124	1126	1128	rBV3	1252	460	0.04%	0.005%
23	4.727	1128	1131	1136	rBV7	1926	1356	0.11%	0.014%
24	4.769	1140	1144	1146	rBV5	2468	1958	0.16%	0.021%
25	4.817	1156	1159	1160	rBV2	1559	869	0.07%	0.009%
26	4.945	1196	1199	1201	rBV4	1482	1074	0.09%	0.011%
27	4.990	1211	1213	1215	rVB3	1330	482	0.04%	0.005%
28	5.068	1219	1237	1262	rBV3	488289	1247707	100.00%	13.187%
29	5.402	1338	1341	1344	rBV4	2702	2333	0.19%	0.025%
30	5.640	1402	1415	1438	rBV	380872	763055	61.16%	8.065%
31	6.093	1542	1556	1574	rBV	276739	562000	45.04%	5.940%
32	6.396	1647	1650	1654	rBV5	2086	1746	0.14%	0.018%
33	6.505	1679	1684	1685	rBV4	1576	1279	0.10%	0.014%
34	6.514	1685	1687	1690	rVB4	1343	690	0.06%	0.007%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061020\
 Data File : VV016796.D
 Acq On : 11 Jun 2020 02:22
 Operator : SY/MD
 Sample : L2929-10 100X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTW9

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

35	6.592	1708	1711	1712	rBV3	1307	750	0.06%	0.008%
36	6.624	1718	1721	1722	rBV3	1445	631	0.05%	0.007%
37	6.678	1735	1738	1739	rBV3	1607	963	0.08%	0.010%
38	6.768	1762	1766	1769	rBV5	1578	1475	0.12%	0.016%
39	6.949	1819	1822	1824	rBV4	2258	1666	0.13%	0.018%
40	7.006	1829	1840	1858	rVV	153722	277449	22.24%	2.932%
41	7.257	1916	1918	1922	rVB4	1524	866	0.07%	0.009%
42	7.338	1931	1943	1962	rBV	573875	984204	78.88%	10.402%
43	7.585	2018	2020	2022	rBV3	2357	1179	0.09%	0.012%
44	7.640	2027	2037	2055	rVV	110250	188929	15.14%	1.997%
45	7.778	2078	2080	2083	rBV4	1490	895	0.07%	0.009%
46	8.109	2173	2183	2213	rBV	286734	560845	44.95%	5.928%
47	8.431	2281	2283	2285	rBV3	2380	1204	0.10%	0.013%
48	8.579	2327	2329	2330	rBV3	1166	489	0.04%	0.005%
49	8.704	2365	2368	2371	rBV4	1535	1025	0.08%	0.011%
50	8.875	2410	2421	2436	rBV	578146	929986	74.54%	9.829%
51	9.376	2575	2577	2580	rBV4	1402	893	0.07%	0.009%
52	9.521	2620	2622	2624	rVB2	1524	596	0.05%	0.006%
53	9.540	2624	2628	2630	rBV4	1143	790	0.06%	0.008%
54	9.566	2633	2636	2637	rBV3	1593	832	0.07%	0.009%
55	9.604	2646	2648	2649	rBV2	1230	407	0.03%	0.004%
56	9.672	2667	2669	2670	rBV2	1265	406	0.03%	0.004%
57	9.710	2678	2681	2685	rBV5	1149	1019	0.08%	0.011%
58	9.752	2691	2694	2695	rBV2	1217	610	0.05%	0.006%
59	9.868	2728	2730	2733	rBV4	1325	949	0.08%	0.010%
60	10.016	2774	2776	2779	rBV3	1555	932	0.07%	0.010%
61	10.109	2803	2805	2807	rBV3	1474	782	0.06%	0.008%
62	10.238	2833	2845	2859	rBV	367414	566527	45.41%	5.988%
63	10.354	2878	2881	2883	rBV4	975	516	0.04%	0.005%
64	10.460	2911	2914	2915	rBV3	1095	722	0.06%	0.008%
65	10.495	2922	2925	2927	rBV4	1729	1123	0.09%	0.012%
66	10.537	2934	2938	2940	rBV3	1999	1544	0.12%	0.016%
67	10.627	2961	2966	2971	rBV8	1976	2797	0.22%	0.030%
68	10.730	2997	2998	3002	rVB3	1041	490	0.04%	0.005%
69	10.755	3002	3006	3009	rBV6	1892	1766	0.14%	0.019%
70	10.804	3019	3021	3024	rBV4	1169	612	0.05%	0.006%
71	10.842	3030	3033	3036	rBV5	1193	1030	0.08%	0.011%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061020\
 Data File : VV016796.D
 Acq On : 11 Jun 2020 02:22
 Operator : SY/MD
 Sample : L2929-10 100X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTW9

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

72	10.878	3042	3044	3048	rVB3	1147	610	0.05%	0.006%
73	10.919	3054	3057	3058	rBV2	1277	672	0.05%	0.007%
74	11.270	3155	3166	3183	rBV	610304	930352	74.56%	9.833%
75	11.411	3208	3210	3213	rVB4	1742	1120	0.09%	0.012%
76	11.434	3213	3217	3219	rBV4	2077	1809	0.14%	0.019%
77	11.463	3224	3226	3231	rVB4	1736	1080	0.09%	0.011%
78	11.485	3231	3233	3235	rBV3	1317	910	0.07%	0.010%
79	11.646	3272	3283	3306	rBV	642311	993129	79.60%	10.496%
80	11.968	3381	3383	3387	rVV5	1593	1146	0.09%	0.012%
81	11.987	3387	3389	3392	rVB4	1531	769	0.06%	0.008%
82	12.071	3413	3415	3417	rVB3	1403	510	0.04%	0.005%
83	12.135	3431	3435	3437	rBV4	1917	1241	0.10%	0.013%
84	12.228	3462	3464	3465	rBV3	1235	503	0.04%	0.005%
85	12.263	3471	3475	3477	rBV5	2288	2022	0.16%	0.021%
86	12.308	3487	3489	3492	rVB3	1203	523	0.04%	0.006%
87	12.424	3522	3525	3529	rVB5	2625	1846	0.15%	0.020%
88	12.444	3529	3531	3534	rBV4	1073	578	0.05%	0.006%
89	12.543	3560	3562	3567	rVB6	1616	1136	0.09%	0.012%
90	13.003	3702	3705	3707	rBV4	1341	604	0.05%	0.006%
91	13.032	3710	3714	3716	rVV4	1246	788	0.06%	0.008%
92	13.045	3716	3718	3722	rBV3	1389	795	0.06%	0.008%
93	13.376	3819	3821	3823	rBV3	1180	537	0.04%	0.006%
94	13.389	3823	3825	3828	rBV4	1541	1069	0.09%	0.011%
95	13.598	3888	3890	3892	rBV3	1312	868	0.07%	0.009%
96	14.019	4017	4021	4024	rBV4	1526	1246	0.10%	0.013%
97	14.173	4067	4069	4072	rBV2	1497	1021	0.08%	0.011%
98	14.341	4119	4121	4123	rBV3	1444	562	0.05%	0.006%
99	14.604	4201	4203	4205	rBV3	1828	1015	0.08%	0.011%
100	15.132	4362	4367	4368	rBV4	2103	1653	0.13%	0.017%


Sum of corrected areas: 9461650

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV061020\
Data File : VV016796.D
Acq On : 11 Jun 2020 02:22
Operator : SY/MD
Sample : L2929-10 100X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTW9

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

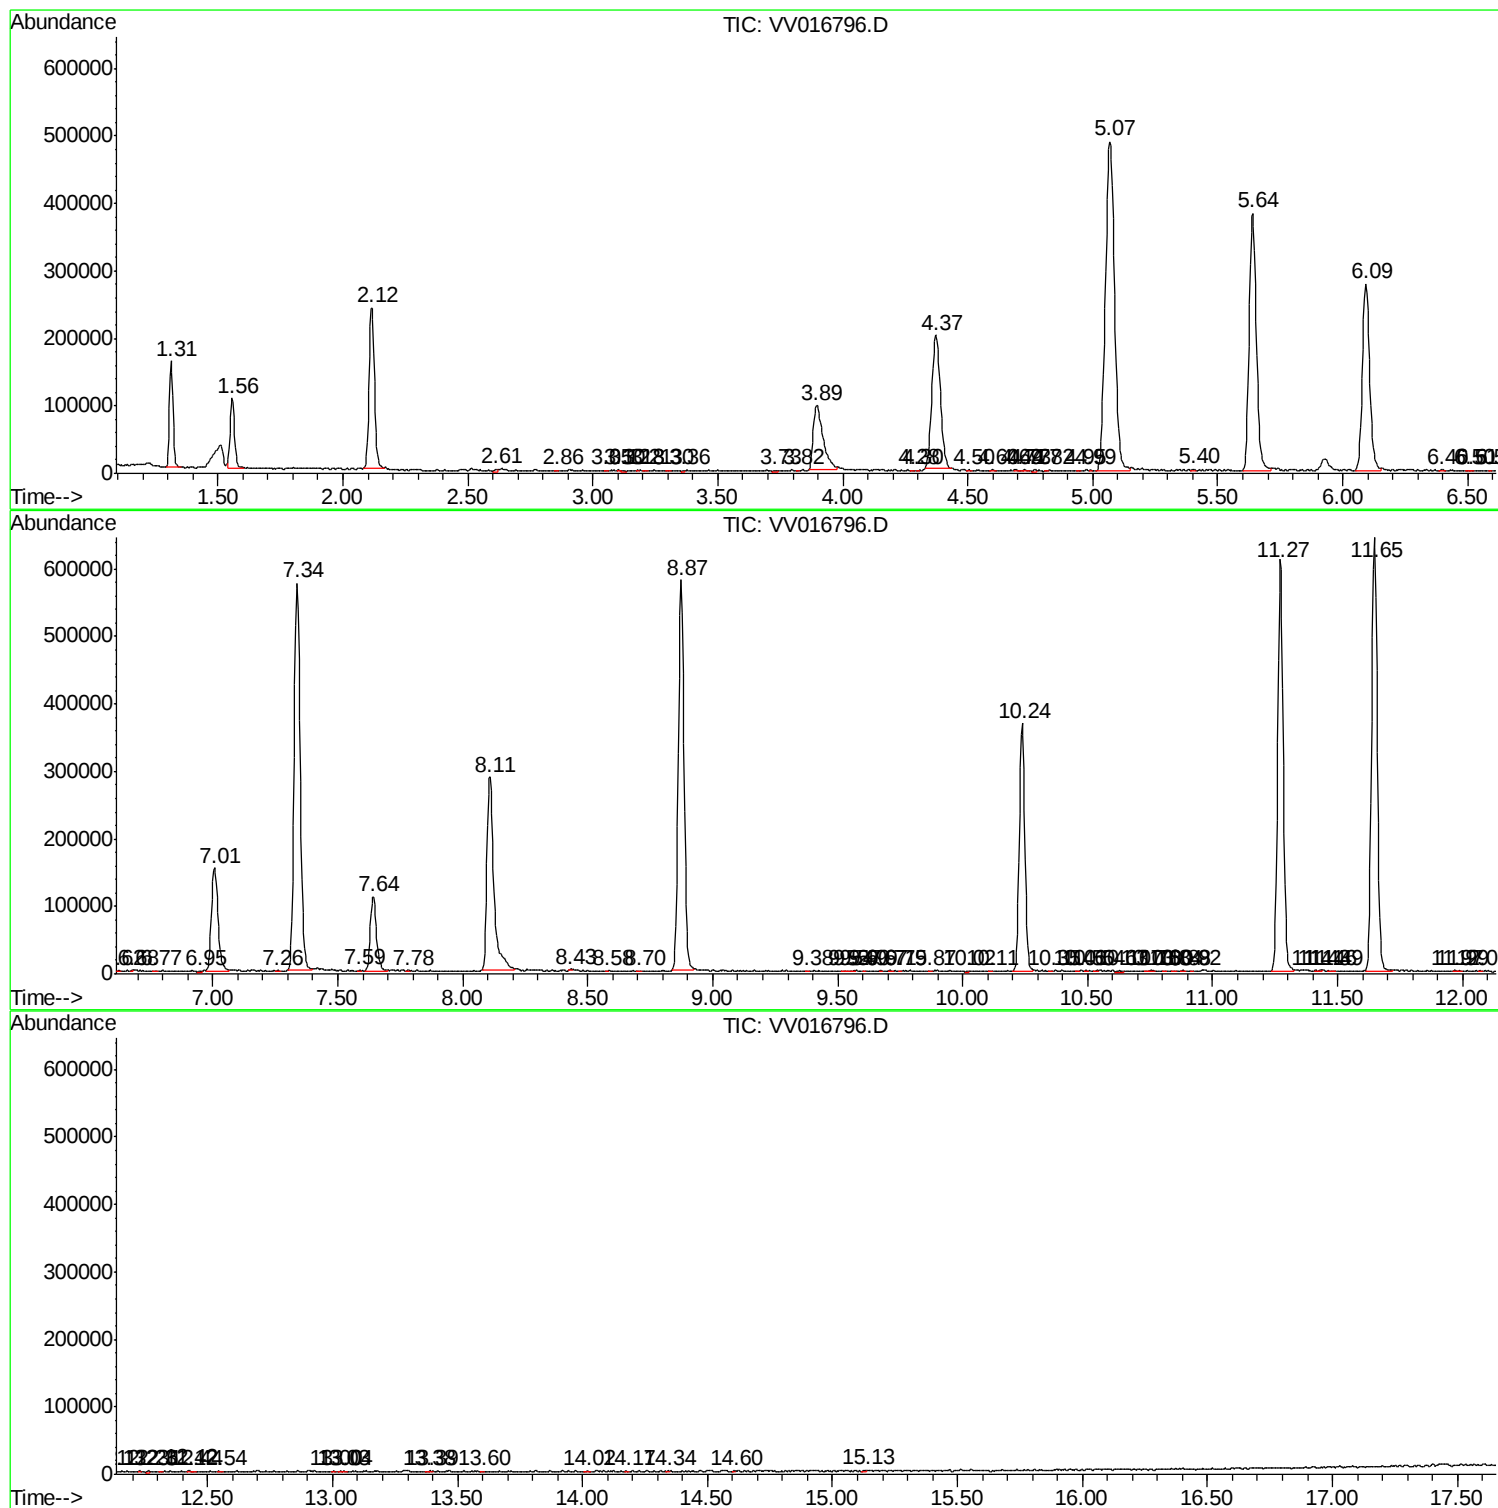

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV061020\
Data File : VV016796.D
Acq On : 11 Jun 2020 02:22
Operator : SY/MD
Sample : L2929-10 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTW9

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV061020\
Data File : VV016796.D
Acq On : 11 Jun 2020 02:22
Operator : SY/MD
Sample : L2929-10 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTW9

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc