

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061020\
 Data File : VV016797.D
 Acq On : 11 Jun 2020 02:45
 Operator : SY/MD
 Sample : L2929-11 100X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTX7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.312	63	69	78	rVB	159316	158985	12.53%	1.635%
2	1.557	139	145	158	rVB	110832	131559	10.37%	1.353%
3	2.116	310	319	337	rVB	251722	377307	29.74%	3.880%
4	2.553	452	455	460	rVB	11839	7143	0.56%	0.073%
5	2.631	470	479	480	rBV8	2895	3864	0.30%	0.040%
6	2.711	502	504	509	rVB6	1647	854	0.07%	0.009%
7	2.737	509	512	514	rBV3	1541	855	0.07%	0.009%
8	2.917	565	568	571	rBV3	1067	745	0.06%	0.008%
9	2.933	571	573	575	rBV3	1289	656	0.05%	0.007%
10	2.978	584	587	588	rBV3	1413	616	0.05%	0.006%
11	3.145	636	639	642	rBV4	2163	1212	0.10%	0.012%
12	3.206	655	658	661	rBV4	1421	930	0.07%	0.010%
13	3.248	667	671	672	rBV4	1291	970	0.08%	0.010%
14	3.579	768	774	778	rBV7	2172	2422	0.19%	0.025%
15	3.643	790	794	797	rVB5	1882	1385	0.11%	0.014%
16	3.663	797	800	801	rBV3	1456	636	0.05%	0.007%
17	3.685	805	807	810	rVB3	1656	950	0.07%	0.010%
18	3.733	818	822	825	rBV6	1193	1126	0.09%	0.012%
19	3.804	841	844	846	rBV4	1580	1043	0.08%	0.011%
20	3.894	862	872	904	rBV	103009	290919	22.93%	2.991%
21	4.373	1006	1021	1042	rBV	208940	508147	40.05%	5.225%
22	4.630	1099	1101	1108	rVB6	1812	1816	0.14%	0.019%
23	4.913	1186	1189	1195	rBV7	1484	1446	0.11%	0.015%
24	4.936	1195	1196	1199	rBV3	1116	600	0.05%	0.006%
25	5.071	1221	1238	1265	rBV2	494241	1268884	100.00%	13.047%
26	5.450	1354	1356	1360	rBV4	1694	1244	0.10%	0.013%
27	5.489	1363	1368	1370	rBV6	1820	1636	0.13%	0.017%
28	5.566	1389	1392	1394	rBV3	1018	591	0.05%	0.006%
29	5.582	1394	1397	1399	rBV4	1310	746	0.06%	0.008%
30	5.640	1403	1415	1434	rVV	375250	744354	58.66%	7.654%
31	5.926	1497	1504	1517	rVB4	18679	35246	2.78%	0.362%
32	6.090	1540	1555	1576	rBV	288855	582627	45.92%	5.991%
33	6.386	1644	1647	1649	rBV4	1525	959	0.08%	0.010%
34	6.479	1673	1676	1678	rBV3	1594	1044	0.08%	0.011%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061020\
 Data File : VV016797.D
 Acq On : 11 Jun 2020 02:45
 Operator : SY/MD
 Sample : L2929-11 100X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTX7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

35	6.505	1678	1684	1686	rVV6	1391	1541	0.12%	0.016%
36	6.598	1711	1713	1718	rBV5	972	646	0.05%	0.007%
37	6.679	1735	1738	1743	rBV7	1939	2009	0.16%	0.021%
38	6.904	1805	1808	1809	rBV3	1065	621	0.05%	0.006%
39	6.949	1820	1822	1823	rBV2	1538	636	0.05%	0.007%
40	6.962	1823	1826	1827	rBV3	1354	847	0.07%	0.009%
41	7.007	1830	1840	1858	rVB	161987	281423	22.18%	2.894%
42	7.187	1893	1896	1899	rBV5	1314	990	0.08%	0.010%
43	7.338	1930	1943	1958	rBV	590876	1018230	80.25%	10.470%
44	7.640	2028	2037	2054	rBV	112510	188688	14.87%	1.940%
45	7.910	2117	2121	2122	rBV4	1614	889	0.07%	0.009%
46	7.971	2137	2140	2145	rBV7	1667	1826	0.14%	0.019%
47	8.048	2160	2164	2166	rBV4	1283	992	0.08%	0.010%
48	8.106	2172	2182	2212	rBV	299063	584588	46.07%	6.011%
49	8.656	2350	2353	2354	rBV3	1192	660	0.05%	0.007%
50	8.698	2364	2366	2369	rVB3	2316	1055	0.08%	0.011%
51	8.714	2369	2371	2378	rBV8	2381	2379	0.19%	0.024%
52	8.871	2408	2420	2436	rBV	580280	930900	73.36%	9.572%
53	9.077	2482	2484	2490	rBV6	1574	1014	0.08%	0.010%
54	9.206	2519	2524	2526	rBV5	2087	1743	0.14%	0.018%
55	9.273	2543	2545	2546	rBV2	1528	621	0.05%	0.006%
56	9.518	2617	2621	2623	rBV4	1630	1116	0.09%	0.011%
57	9.650	2659	2662	2664	rVB4	1814	1037	0.08%	0.011%
58	9.662	2664	2666	2668	rBV3	1086	686	0.05%	0.007%
59	9.746	2687	2692	2694	rVB5	1907	1274	0.10%	0.013%
60	9.765	2696	2698	2703	rVB5	1838	1405	0.11%	0.014%
61	9.871	2726	2731	2734	rBV6	1855	1800	0.14%	0.019%
62	9.887	2734	2736	2739	rVB5	1635	968	0.08%	0.010%
63	9.904	2739	2741	2743	rBV2	1916	937	0.07%	0.010%
64	9.955	2755	2757	2761	rVB4	1434	673	0.05%	0.007%
65	10.010	2769	2774	2777	rBV6	1656	1614	0.13%	0.017%
66	10.151	2816	2818	2825	rBV7	1355	1003	0.08%	0.010%
67	10.238	2834	2845	2861	rVB	375101	592507	46.70%	6.092%
68	10.608	2957	2960	2961	rBV3	1437	871	0.07%	0.009%
69	10.653	2969	2974	2979	rBV9	1460	1779	0.14%	0.018%
70	11.000	3080	3082	3087	rVB4	1343	928	0.07%	0.010%
71	11.022	3087	3089	3092	rBV4	1137	828	0.07%	0.009%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061020\
 Data File : VV016797.D
 Acq On : 11 Jun 2020 02:45
 Operator : SY/MD
 Sample : L2929-11 100X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTX7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

72	11.270	3155	3166	3187	rVV	595239	909947	71.71%	9.356%
73	11.476	3227	3230	3233	rBV5	2283	1778	0.14%	0.018%
74	11.585	3261	3264	3266	rVB4	1126	651	0.05%	0.007%
75	11.646	3270	3283	3299	rVV	656790	1019271	80.33%	10.480%
76	11.817	3330	3336	3339	rBV8	1978	1691	0.13%	0.017%
77	11.878	3353	3355	3360	rVB3	1339	928	0.07%	0.010%
78	11.945	3373	3376	3379	rVB5	1596	890	0.07%	0.009%
79	12.048	3405	3408	3412	rBV6	1943	1613	0.13%	0.017%
80	12.116	3427	3429	3434	rVB5	1449	980	0.08%	0.010%
81	12.180	3447	3449	3452	rBV4	1065	712	0.06%	0.007%
82	12.231	3459	3465	3466	rBV7	1373	1212	0.10%	0.012%
83	12.305	3486	3488	3491	rBV3	1396	746	0.06%	0.008%
84	12.347	3499	3501	3504	rBV4	1210	901	0.07%	0.009%
85	12.379	3507	3511	3512	rBV3	1655	920	0.07%	0.009%
86	12.489	3542	3545	3547	rBV3	1056	738	0.06%	0.008%
87	12.566	3563	3569	3573	rBV8	2124	2553	0.20%	0.026%
88	12.637	3587	3591	3594	rVB4	1755	1229	0.10%	0.013%
89	13.026	3710	3712	3717	rVB5	1484	1153	0.09%	0.012%
90	13.061	3717	3723	3724	rBV4	2070	2313	0.18%	0.024%
91	13.321	3800	3804	3806	rBV4	1799	1300	0.10%	0.013%
92	13.495	3854	3858	3859	rBV3	1639	1325	0.10%	0.014%
93	13.566	3878	3880	3882	rBV3	1983	907	0.07%	0.009%
94	13.582	3883	3885	3888	rVV3	1349	645	0.05%	0.007%
95	13.778	3944	3946	3951	rBV5	1550	1414	0.11%	0.015%
96	14.321	4112	4115	4117	rBV3	1686	969	0.08%	0.010%
97	14.357	4123	4126	4128	rBV3	1516	959	0.08%	0.010%
98	14.717	4236	4238	4241	rBV3	1343	736	0.06%	0.008%
99	14.948	4308	4310	4312	rBV2	1648	785	0.06%	0.008%
100	14.980	4318	4320	4323	rBV3	1348	1019	0.08%	0.010%


Sum of corrected areas: 9725526

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV061020\
Data File : VV016797.D
Acq On : 11 Jun 2020 02:45
Operator : SY/MD
Sample : L2929-11 100X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTX7

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

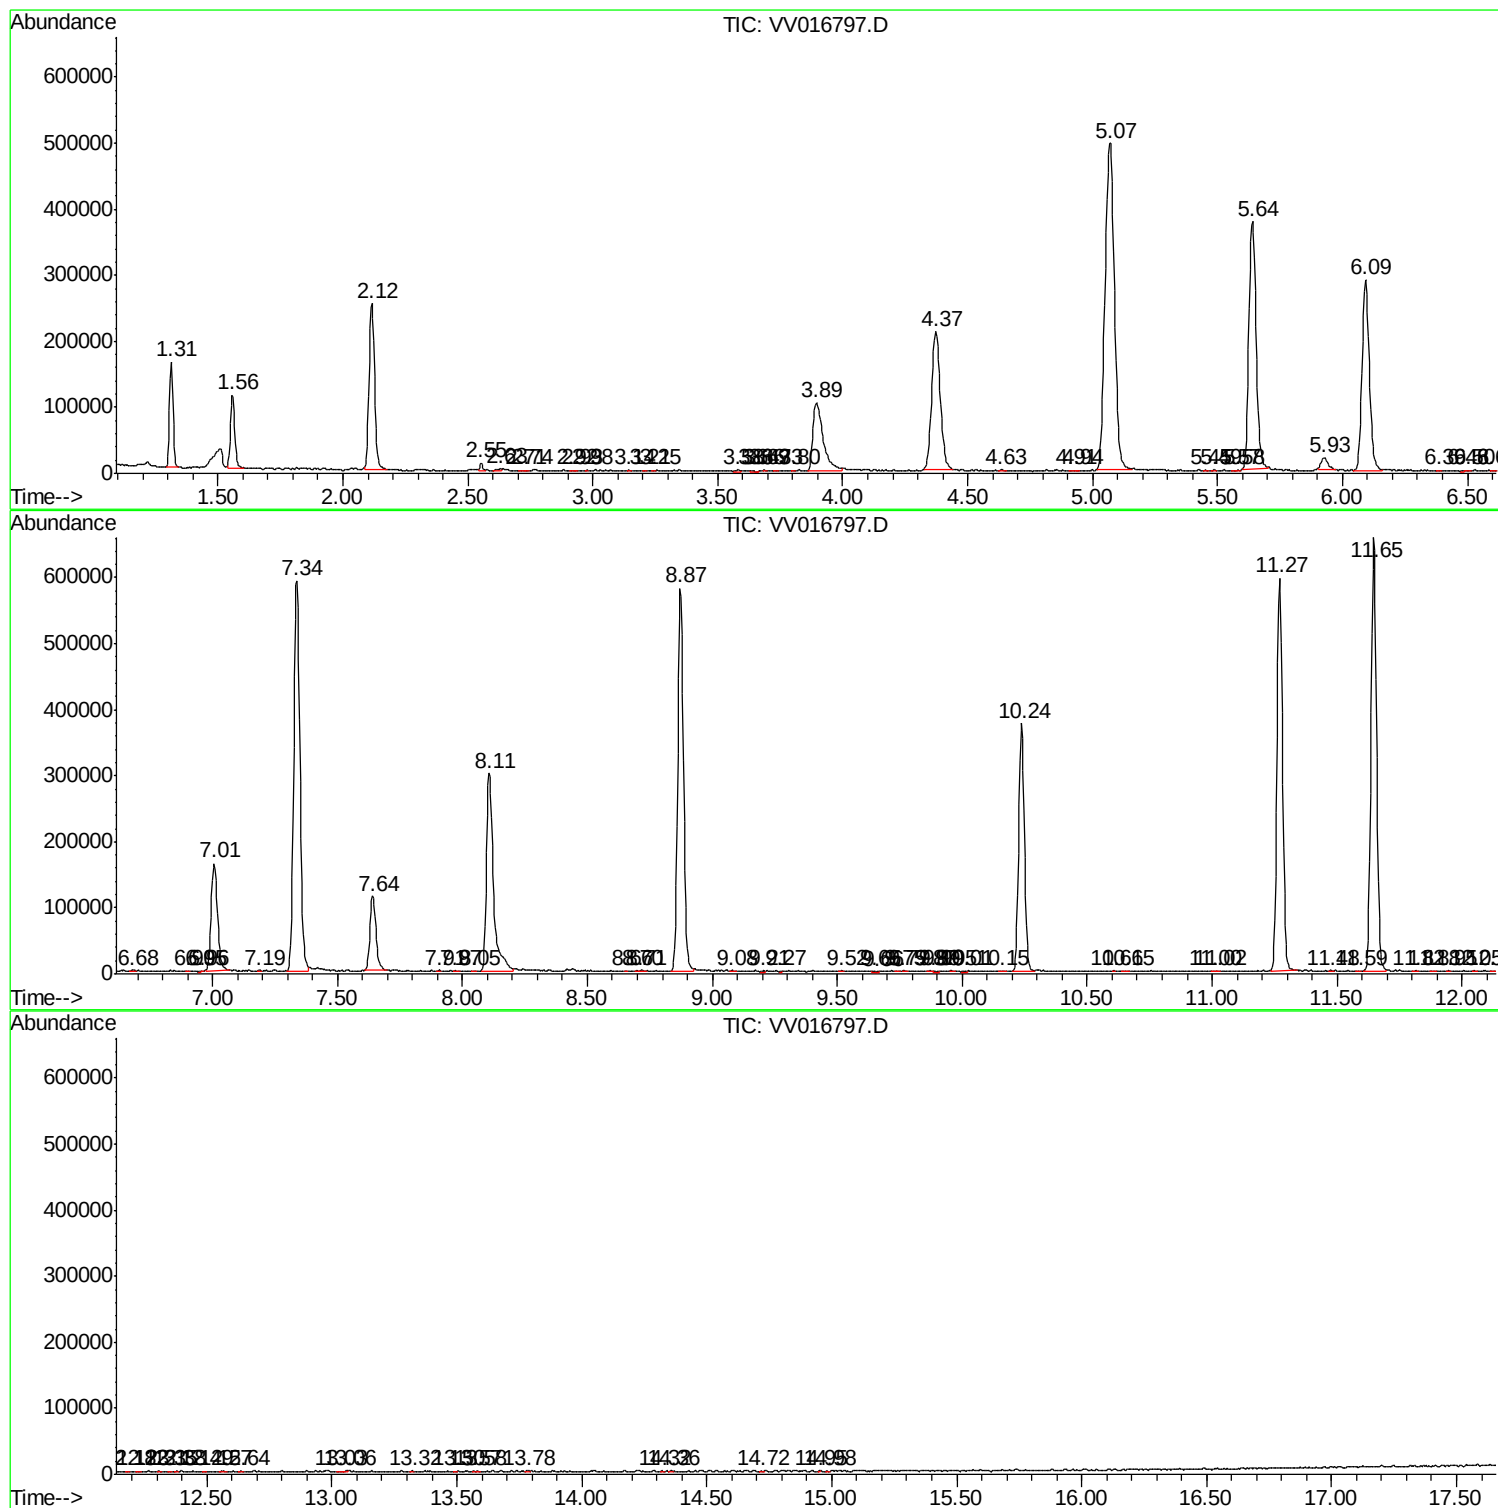

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV061020\
Data File : VV016797.D
Acq On : 11 Jun 2020 02:45
Operator : SY/MD
Sample : L2929-11 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTX7

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV061020\
Data File : VV016797.D
Acq On : 11 Jun 2020 02:45
Operator : SY/MD
Sample : L2929-11 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTX7

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc