

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061020\
 Data File : VV016798.D
 Acq On : 11 Jun 2020 03:09
 Operator : SY/MD
 Sample : L2929-12 100X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTX8

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.312	64	69	81	rVB	172793	168968	13.23%	1.733%
2	1.557	139	145	160	rVB	110570	135014	10.57%	1.385%
3	2.116	310	319	335	rVB	250694	371707	29.10%	3.812%
4	2.717	504	506	508	rBV3	1661	950	0.07%	0.010%
5	2.753	515	517	520	rVB4	1766	855	0.07%	0.009%
6	2.775	520	524	526	rBV5	2178	1704	0.13%	0.017%
7	2.868	549	553	558	rVB6	952	867	0.07%	0.009%
8	2.923	566	570	572	rBV3	1797	1170	0.09%	0.012%
9	3.155	639	642	647	rBV5	1890	1536	0.12%	0.016%
10	3.180	647	650	651	rBV3	897	631	0.05%	0.006%
11	3.209	657	659	660	rBV2	2052	899	0.07%	0.009%
12	3.376	706	711	714	rBV6	1507	1194	0.09%	0.012%
13	3.405	716	720	721	rBV4	1697	1050	0.08%	0.011%
14	3.431	724	728	730	rBV5	1394	1065	0.08%	0.011%
15	3.476	740	742	747	rVB5	1383	914	0.07%	0.009%
16	3.502	747	750	754	rBV5	1621	1097	0.09%	0.011%
17	3.576	768	773	774	rVB4	1540	1066	0.08%	0.011%
18	3.595	777	779	783	rBV3	1159	824	0.06%	0.008%
19	3.647	793	795	797	rBV3	1434	583	0.05%	0.006%
20	3.730	817	821	825	rBV6	2763	2270	0.18%	0.023%
21	3.766	829	832	834	rBV4	1273	589	0.05%	0.006%
22	3.894	862	872	893	rBV	103421	277844	21.75%	2.849%
23	4.286	991	994	995	rBV3	1275	768	0.06%	0.008%
24	4.373	1005	1021	1039	rBV	203382	503959	39.46%	5.168%
25	4.499	1058	1060	1064	rBV3	1860	1441	0.11%	0.015%
26	4.679	1114	1116	1118	rBV3	1610	630	0.05%	0.006%
27	4.714	1124	1127	1129	rBV2	1244	772	0.06%	0.008%
28	4.743	1133	1136	1138	rVB4	1442	815	0.06%	0.008%
29	4.756	1138	1140	1144	rBV5	942	805	0.06%	0.008%
30	4.881	1175	1179	1181	rBV3	1071	888	0.07%	0.009%
31	4.913	1185	1189	1194	rBV8	1506	1467	0.11%	0.015%
32	5.068	1221	1237	1261	rBV2	495504	1277206	100.00%	13.099%
33	5.492	1365	1369	1373	rBV6	1509	1201	0.09%	0.012%
34	5.637	1399	1414	1436	rBV	390659	787014	61.62%	8.071%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061020\
 Data File : VV016798.D
 Acq On : 11 Jun 2020 03:09
 Operator : SY/MD
 Sample : L2929-12 100X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTX8

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

35	5.827	1471	1473	1478	rBV6	1331	915	0.07%	0.009%
36	6.093	1543	1556	1579	rBV	280965	570106	44.64%	5.847%
37	6.309	1620	1623	1626	rBV5	1342	1049	0.08%	0.011%
38	6.380	1642	1645	1646	rBV2	1154	620	0.05%	0.006%
39	6.505	1681	1684	1688	rBV5	1413	1189	0.09%	0.012%
40	6.566	1698	1703	1708	rBV8	1621	2145	0.17%	0.022%
41	6.646	1725	1728	1731	rVV4	1131	787	0.06%	0.008%
42	6.759	1761	1763	1767	rBV3	805	699	0.05%	0.007%
43	6.884	1798	1802	1804	rBV4	1127	937	0.07%	0.010%
44	7.007	1829	1840	1860	rVV	162421	283366	22.19%	2.906%
45	7.193	1895	1898	1900	rBV4	1242	596	0.05%	0.006%
46	7.203	1900	1901	1904	rBV3	1524	933	0.07%	0.010%
47	7.338	1931	1943	1968	rBV	587436	1017360	79.66%	10.434%
48	7.556	2008	2011	2012	rBV3	1661	1080	0.08%	0.011%
49	7.640	2028	2037	2055	rBV	113770	189073	14.80%	1.939%
50	7.852	2101	2103	2106	rBV4	1401	1090	0.09%	0.011%
51	8.013	2151	2153	2158	rVB3	1664	1239	0.10%	0.013%
52	8.106	2172	2182	2215	rBV2	296887	579640	45.38%	5.945%
53	8.691	2362	2364	2366	rBV2	933	596	0.05%	0.006%
54	8.749	2380	2382	2385	rBV3	1563	725	0.06%	0.007%
55	8.826	2404	2406	2408	rBV3	1691	781	0.06%	0.008%
56	8.871	2409	2420	2440	rVV	605630	962676	75.37%	9.873%
57	9.103	2489	2492	2494	rBV5	1953	1533	0.12%	0.016%
58	9.283	2543	2548	2549	rBV4	1300	1219	0.10%	0.013%
59	9.354	2568	2570	2573	rBV4	1572	770	0.06%	0.008%
60	9.415	2586	2589	2590	rBV3	1164	617	0.05%	0.006%
61	9.518	2618	2621	2623	rBV3	1842	1172	0.09%	0.012%
62	9.717	2681	2683	2686	rBV4	1285	892	0.07%	0.009%
63	9.733	2686	2688	2690	rVB3	1341	572	0.04%	0.006%
64	9.810	2707	2712	2714	rBV5	2206	1825	0.14%	0.019%
65	9.871	2725	2731	2734	rBV7	1566	1595	0.12%	0.016%
66	9.897	2737	2739	2740	rBV2	1308	583	0.05%	0.006%
67	9.977	2762	2764	2768	rVB4	1476	892	0.07%	0.009%
68	10.000	2768	2771	2773	rBV3	1940	1023	0.08%	0.010%
69	10.177	2824	2826	2830	rVB5	2047	1173	0.09%	0.012%
70	10.238	2833	2845	2867	rVB	372499	586337	45.91%	6.013%
71	10.453	2909	2912	2913	rBV2	1202	778	0.06%	0.008%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061020\
 Data File : VV016798.D
 Acq On : 11 Jun 2020 03:09
 Operator : SY/MD
 Sample : L2929-12 100X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTX8

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

72	10.669	2975	2979	2980	rBV3	1638	914	0.07%	0.009%
73	10.711	2990	2992	2994	rBV3	1828	983	0.08%	0.010%
74	10.778	3010	3013	3015	rBV3	1214	856	0.07%	0.009%
75	10.830	3025	3029	3030	rBV4	1224	879	0.07%	0.009%
76	10.875	3041	3043	3049	rVV5	1605	1211	0.09%	0.012%
77	10.900	3049	3051	3056	rVB5	1412	999	0.08%	0.010%
78	10.952	3065	3067	3071	rBV4	1447	1259	0.10%	0.013%
79	11.058	3096	3100	3101	rBV3	1570	1212	0.09%	0.012%
80	11.119	3117	3119	3122	rBV3	1479	616	0.05%	0.006%
81	11.270	3154	3166	3186	rVV	616268	944397	73.94%	9.685%
82	11.582	3261	3263	3266	rBV3	1973	1233	0.10%	0.013%
83	11.646	3272	3283	3300	rBV	655640	1008104	78.93%	10.339%
84	12.000	3391	3393	3400	rVB7	2172	1902	0.15%	0.020%
85	12.029	3400	3402	3405	rBV4	789	632	0.05%	0.006%
86	12.048	3406	3408	3410	rBV2	1249	637	0.05%	0.007%
87	12.132	3432	3434	3436	rBV3	2120	1437	0.11%	0.015%
88	12.177	3444	3448	3449	rBV4	1702	1353	0.11%	0.014%
89	12.231	3462	3465	3467	rVB3	1202	637	0.05%	0.007%
90	12.514	3549	3553	3555	rBV6	1131	830	0.06%	0.009%
91	12.620	3583	3586	3590	rBV3	1813	1411	0.11%	0.014%
92	12.643	3590	3593	3597	rBV4	1252	621	0.05%	0.006%
93	12.846	3653	3656	3659	rBV3	1243	1140	0.09%	0.012%
94	12.900	3670	3673	3676	rBV4	1599	1379	0.11%	0.014%
95	13.006	3703	3706	3709	rBV5	1755	1400	0.11%	0.014%
96	13.116	3737	3740	3742	rBV4	1361	984	0.08%	0.010%
97	13.569	3879	3881	3883	rBV2	1547	978	0.08%	0.010%
98	13.624	3896	3898	3900	rBV2	2189	1046	0.08%	0.011%
99	14.029	4020	4024	4026	rBV4	1648	1389	0.11%	0.014%
100	14.813	4264	4268	4272	rBV7	1747	1898	0.15%	0.019%


Sum of corrected areas: 9750683

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV061020\
Data File : VV016798.D
Acq On : 11 Jun 2020 03:09
Operator : SY/MD
Sample : L2929-12 100X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTX8

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

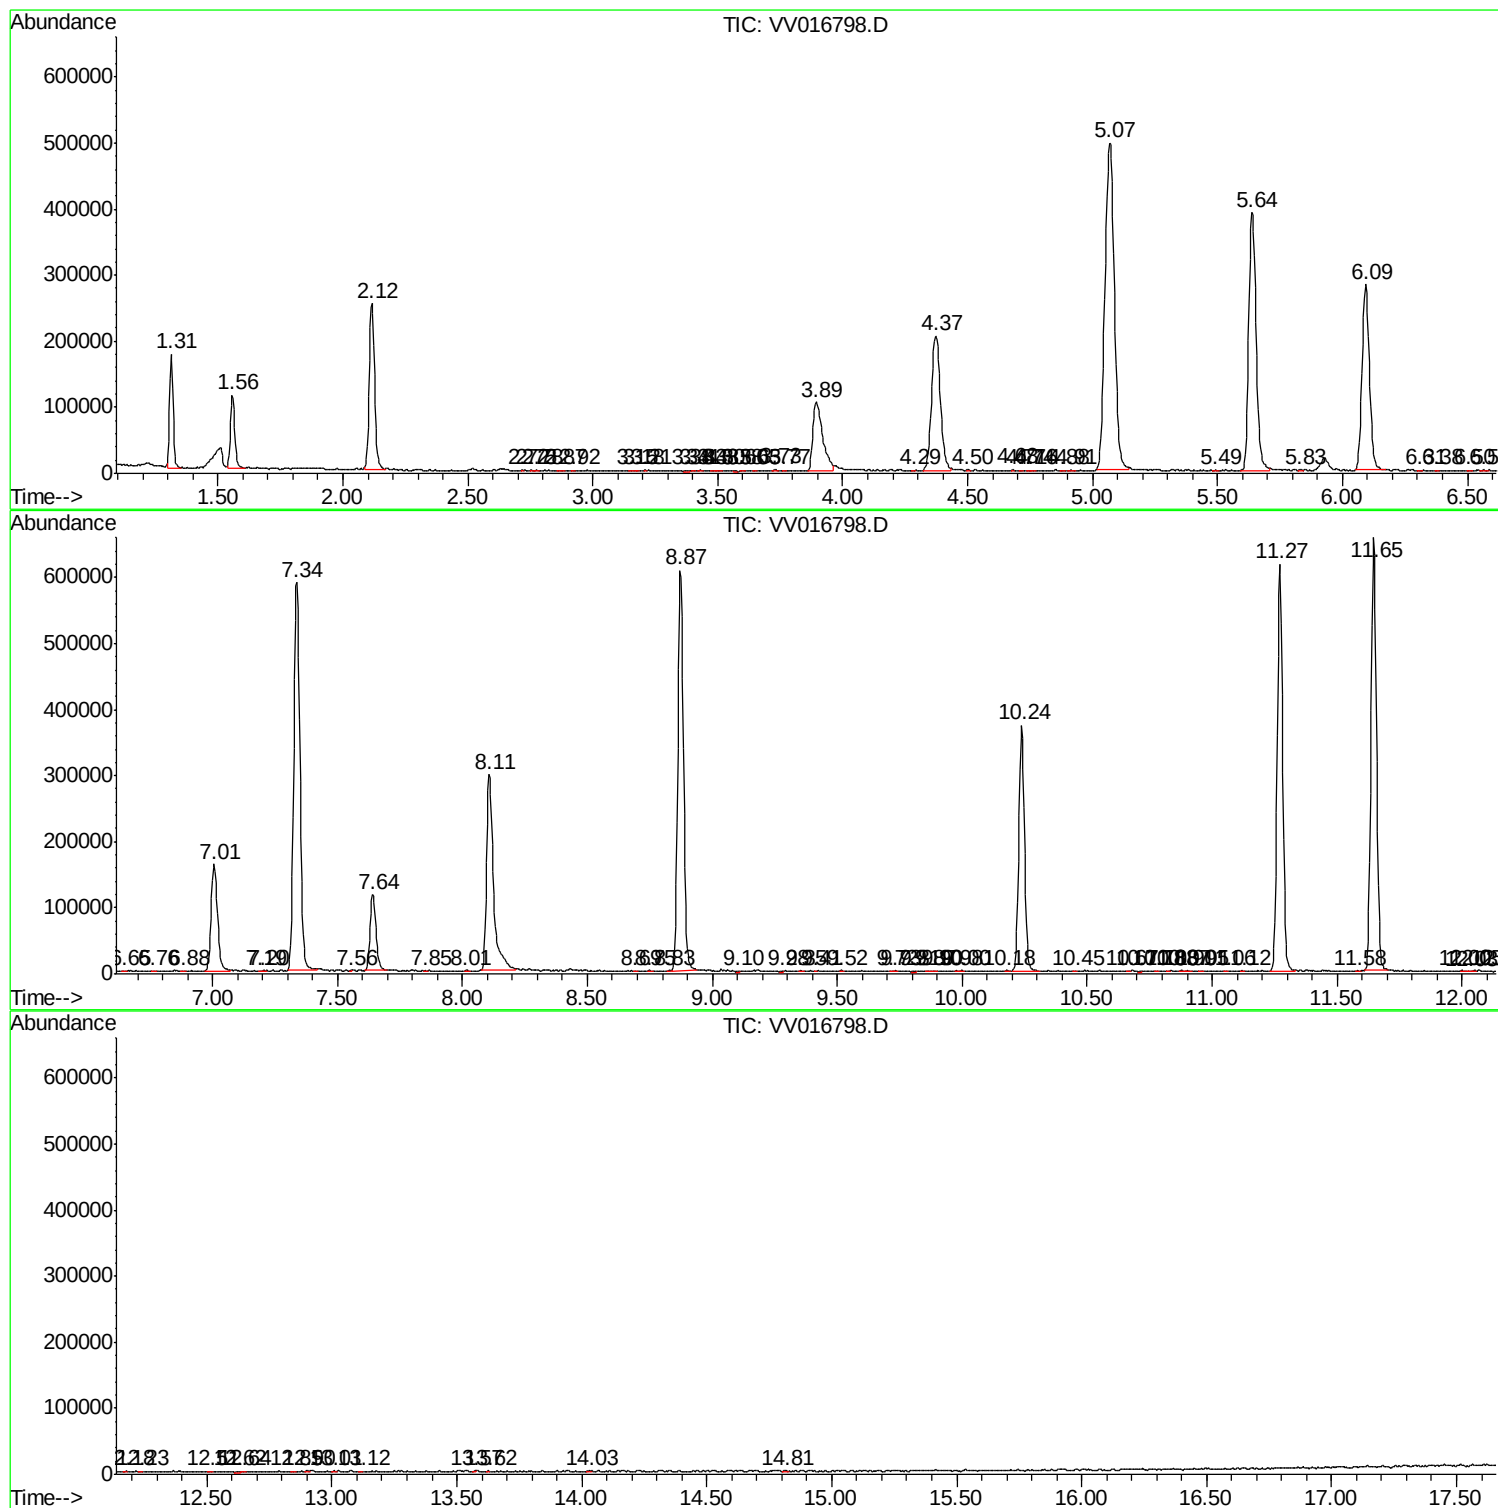

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV061020\
Data File : VV016798.D
Acq On : 11 Jun 2020 03:09
Operator : SY/MD
Sample : L2929-12 100X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTX8










Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown-01 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.01	18.00 ug/L	283366	1,4-Difluorobenzene	5.64

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	1,3-Cyclohexadiene	80	C6H8	000592-57-4	25
2		.alpha.,.alpha.-Dichloromethyl m...	114	C2H4Cl2O	004885-02-3	25
3		2-Propanol, 1,3-dichloro-	128	C3H6Cl2O	000096-23-1	17
4		2,3-Butanedione, dioxime	116	C4H8N2O2	000095-45-4	9
5		1,4-Cyclohexadiene	80	C6H8	000628-41-1	9

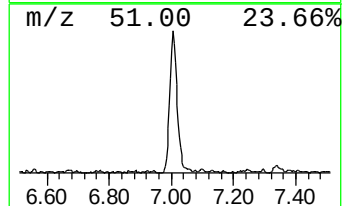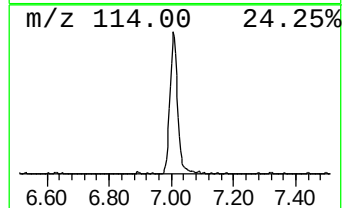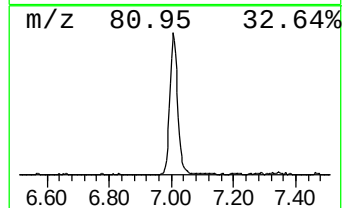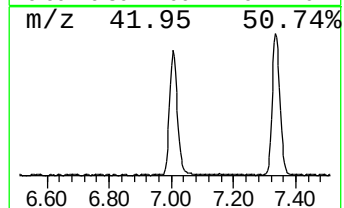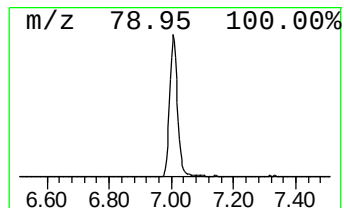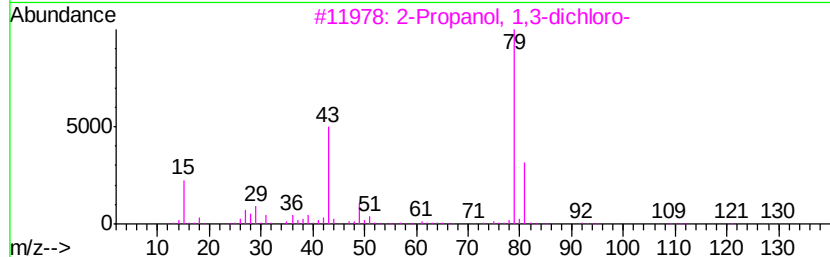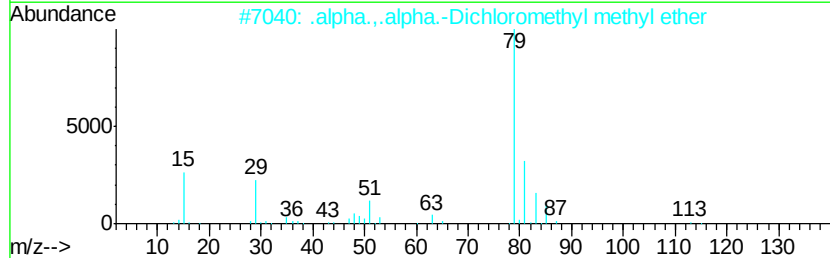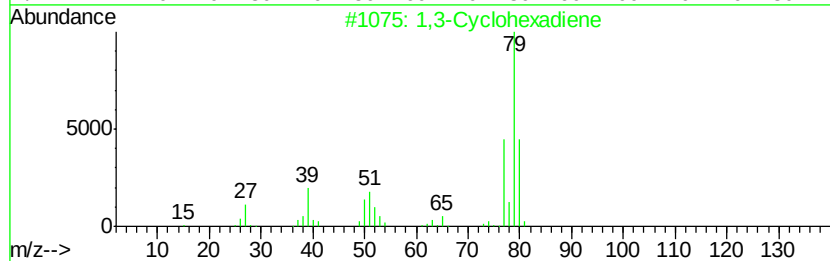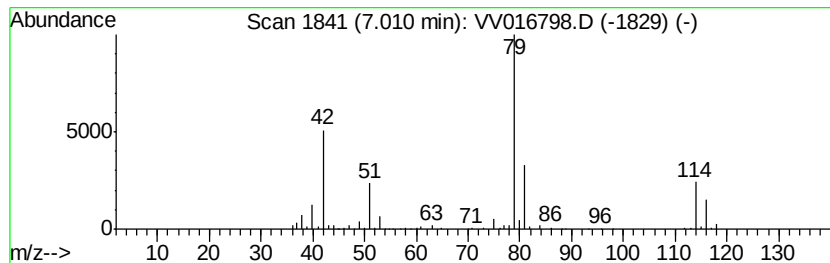

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV061020\
Data File : VV016798.D
Acq On : 11 Jun 2020 03:09
Operator : SY/MD
Sample : L2929-12 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTX8

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown-01	7.01	18.0	ug/L	283366	1	5.64	787014	50.0