

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061020\
 Data File : VV016805.D
 Acq On : 11 Jun 2020 05:56
 Operator : SY/MD
 Sample : L2901-10
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTT5

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.312	63	69	79	rVB	153023	152622	12.20%	1.586%
2	1.557	139	145	158	rVB	102339	126912	10.14%	1.319%
3	2.116	310	319	331	rBV	239280	347030	27.73%	3.605%
4	2.447	417	422	425	rBV6	2649	2562	0.20%	0.027%
5	2.669	489	491	495	rBV5	1786	1677	0.13%	0.017%
6	2.962	577	582	584	rBV6	1637	1353	0.11%	0.014%
7	3.052	607	610	614	rBV5	1107	892	0.07%	0.009%
8	3.264	673	676	678	rBV3	1527	980	0.08%	0.010%
9	3.315	690	692	696	rVB5	2464	1152	0.09%	0.012%
10	3.354	696	704	706	rBV8	2376	2850	0.23%	0.030%
11	3.495	746	748	752	rBV5	860	665	0.05%	0.007%
12	3.566	766	770	772	rBV3	875	792	0.06%	0.008%
13	3.676	802	804	806	rVB3	1500	722	0.06%	0.008%
14	3.698	806	811	814	rBV7	1553	1113	0.09%	0.012%
15	3.794	839	841	844	rBV4	1175	632	0.05%	0.007%
16	3.856	856	860	862	rBV4	1326	903	0.07%	0.009%
17	3.894	862	872	901	rVV	98833	263249	21.04%	2.735%
18	4.373	1006	1021	1043	rBV	201521	493140	39.41%	5.123%
19	4.653	1106	1108	1111	rBV4	1404	1154	0.09%	0.012%
20	4.785	1147	1149	1151	rBV3	1812	836	0.07%	0.009%
21	4.933	1193	1195	1198	rBV3	1276	607	0.05%	0.006%
22	4.987	1210	1212	1215	rVB3	1350	730	0.06%	0.008%
23	5.068	1218	1237	1261	rBV2	487410	1251369	100.00%	13.001%
24	5.640	1401	1415	1444	rBV	391430	783575	62.62%	8.141%
25	5.810	1466	1468	1470	rVB2	1660	588	0.05%	0.006%
26	5.891	1491	1493	1494	rBV2	1805	658	0.05%	0.007%
27	6.093	1543	1556	1578	rVB	282228	565594	45.20%	5.876%
28	6.219	1593	1595	1596	rBV2	1559	663	0.05%	0.007%
29	6.341	1629	1633	1635	rBV4	1471	1074	0.09%	0.011%
30	6.492	1678	1680	1682	rBV3	1459	730	0.06%	0.008%
31	6.505	1682	1684	1689	rVV5	1520	1204	0.10%	0.013%
32	6.527	1689	1691	1693	rBV3	1485	873	0.07%	0.009%
33	6.556	1698	1700	1701	rBV2	1350	685	0.05%	0.007%
34	6.598	1709	1713	1715	rBV5	1533	1258	0.10%	0.013%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061020\
 Data File : VV016805.D
 Acq On : 11 Jun 2020 05:56
 Operator : SY/MD
 Sample : L2901-10
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTT5

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

35	6.637	1721	1725	1727	rBV3	1501	1050	0.08%	0.011%
36	6.669	1732	1735	1743	rBV9	2145	2564	0.20%	0.027%
37	6.701	1743	1745	1750	rVB6	2015	1284	0.10%	0.013%
38	6.730	1752	1754	1756	rBV3	1111	692	0.06%	0.007%
39	6.852	1790	1792	1797	rBV6	854	597	0.05%	0.006%
40	7.007	1826	1840	1862	rBV	151754	277983	22.21%	2.888%
41	7.158	1884	1887	1889	rBV3	1648	1062	0.08%	0.011%
42	7.338	1930	1943	1960	rBV	572084	988528	79.00%	10.270%
43	7.556	2009	2011	2013	rBV3	1610	680	0.05%	0.007%
44	7.640	2025	2037	2052	rBV	109015	187410	14.98%	1.947%
45	8.109	2171	2183	2214	rBV	304876	593826	47.45%	6.169%
46	8.527	2311	2313	2316	rVB4	1525	605	0.05%	0.006%
47	8.669	2355	2357	2363	rVB7	1617	1451	0.12%	0.015%
48	8.698	2363	2366	2367	rBV3	1349	653	0.05%	0.007%
49	8.871	2408	2420	2441	rVV	596292	972898	77.75%	10.108%
50	9.450	2598	2600	2603	rBV4	1504	808	0.06%	0.008%
51	9.553	2628	2632	2634	rBV5	1659	1242	0.10%	0.013%
52	9.778	2698	2702	2704	rBV5	1256	941	0.08%	0.010%
53	9.817	2711	2714	2716	rBV3	2095	1394	0.11%	0.014%
54	9.920	2742	2746	2749	rBV4	1313	1111	0.09%	0.012%
55	10.026	2775	2779	2781	rVB4	1531	934	0.07%	0.010%
56	10.077	2793	2795	2797	rBV3	1154	677	0.05%	0.007%
57	10.100	2799	2802	2806	rBV5	1921	1250	0.10%	0.013%
58	10.196	2828	2832	2833	rBV3	2303	1439	0.11%	0.015%
59	10.238	2834	2845	2861	rVB	384108	597827	47.77%	6.211%
60	10.373	2883	2887	2889	rBV3	1319	911	0.07%	0.009%
61	10.460	2912	2914	2918	rVB5	1603	987	0.08%	0.010%
62	10.479	2918	2920	2923	rBV4	955	782	0.06%	0.008%
63	10.524	2932	2934	2936	rVB3	1509	631	0.05%	0.007%
64	10.579	2947	2951	2953	rVB5	1309	695	0.06%	0.007%
65	10.592	2953	2955	2957	rBV2	1479	615	0.05%	0.006%
66	10.611	2957	2961	2966	rVB6	1358	1171	0.09%	0.012%
67	10.669	2977	2979	2981	rBV3	1235	781	0.06%	0.008%
68	10.826	3026	3028	3030	rBV3	1813	746	0.06%	0.008%
69	10.842	3030	3033	3035	rBV3	1013	628	0.05%	0.007%
70	10.858	3035	3038	3041	rVV3	1201	860	0.07%	0.009%
71	10.929	3056	3060	3062	rBV5	1396	1046	0.08%	0.011%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061020\
 Data File : VV016805.D
 Acq On : 11 Jun 2020 05:56
 Operator : SY/MD
 Sample : L2901-10
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTT5

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

72	10.968	3069	3072	3077	rVB6	2137	1472	0.12%	0.015%
73	10.997	3077	3081	3082	rBV2	1034	608	0.05%	0.006%
74	11.109	3110	3116	3120	rBV8	2233	3112	0.25%	0.032%
75	11.270	3154	3166	3189	rBV	622664	940062	75.12%	9.767%
76	11.556	3247	3255	3263	rBV8	7397	13164	1.05%	0.137%
77	11.646	3272	3283	3304	rVB	624591	983627	78.60%	10.219%
78	12.074	3414	3416	3419	rBV3	1215	738	0.06%	0.008%
79	12.157	3440	3442	3445	rVB3	1149	598	0.05%	0.006%
80	12.177	3445	3448	3452	rBV4	1072	718	0.06%	0.007%
81	12.199	3452	3455	3459	rBV5	1006	1006	0.08%	0.010%
82	12.395	3514	3516	3517	rBV2	1293	688	0.05%	0.007%
83	12.440	3525	3530	3532	rBV4	1204	951	0.08%	0.010%
84	12.511	3550	3552	3555	rVB3	1554	694	0.06%	0.007%
85	12.598	3575	3579	3581	rBV3	2082	1484	0.12%	0.015%
86	12.701	3609	3611	3614	rBV2	1982	1114	0.09%	0.012%
87	12.775	3630	3634	3635	rBV2	1061	660	0.05%	0.007%
88	12.965	3690	3693	3697	rBV3	1414	1170	0.09%	0.012%
89	13.106	3733	3737	3738	rBV4	990	701	0.06%	0.007%
90	13.341	3807	3810	3813	rBV6	1890	1388	0.11%	0.014%
91	13.402	3824	3829	3832	rBV6	2319	2320	0.19%	0.024%
92	13.431	3836	3838	3840	rBV3	1087	657	0.05%	0.007%
93	13.608	3890	3893	3897	rBV7	1569	1271	0.10%	0.013%
94	13.984	4008	4010	4012	rBV3	1346	681	0.05%	0.007%
95	14.058	4029	4033	4034	rBV3	1200	1038	0.08%	0.011%
96	14.318	4112	4114	4116	rBV2	1331	659	0.05%	0.007%
97	14.444	4148	4153	4155	rBV5	1994	1661	0.13%	0.017%
98	14.543	4182	4184	4186	rVB3	1533	595	0.05%	0.006%
99	14.669	4220	4223	4224	rBV2	2167	1252	0.10%	0.013%
100	16.199	4697	4699	4703	rBV5	2031	1576	0.13%	0.016%


Sum of corrected areas: 9625268

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV061020\
Data File : VV016805.D
Acq On : 11 Jun 2020 05:56
Operator : SY/MD
Sample : L2901-10
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTT5

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

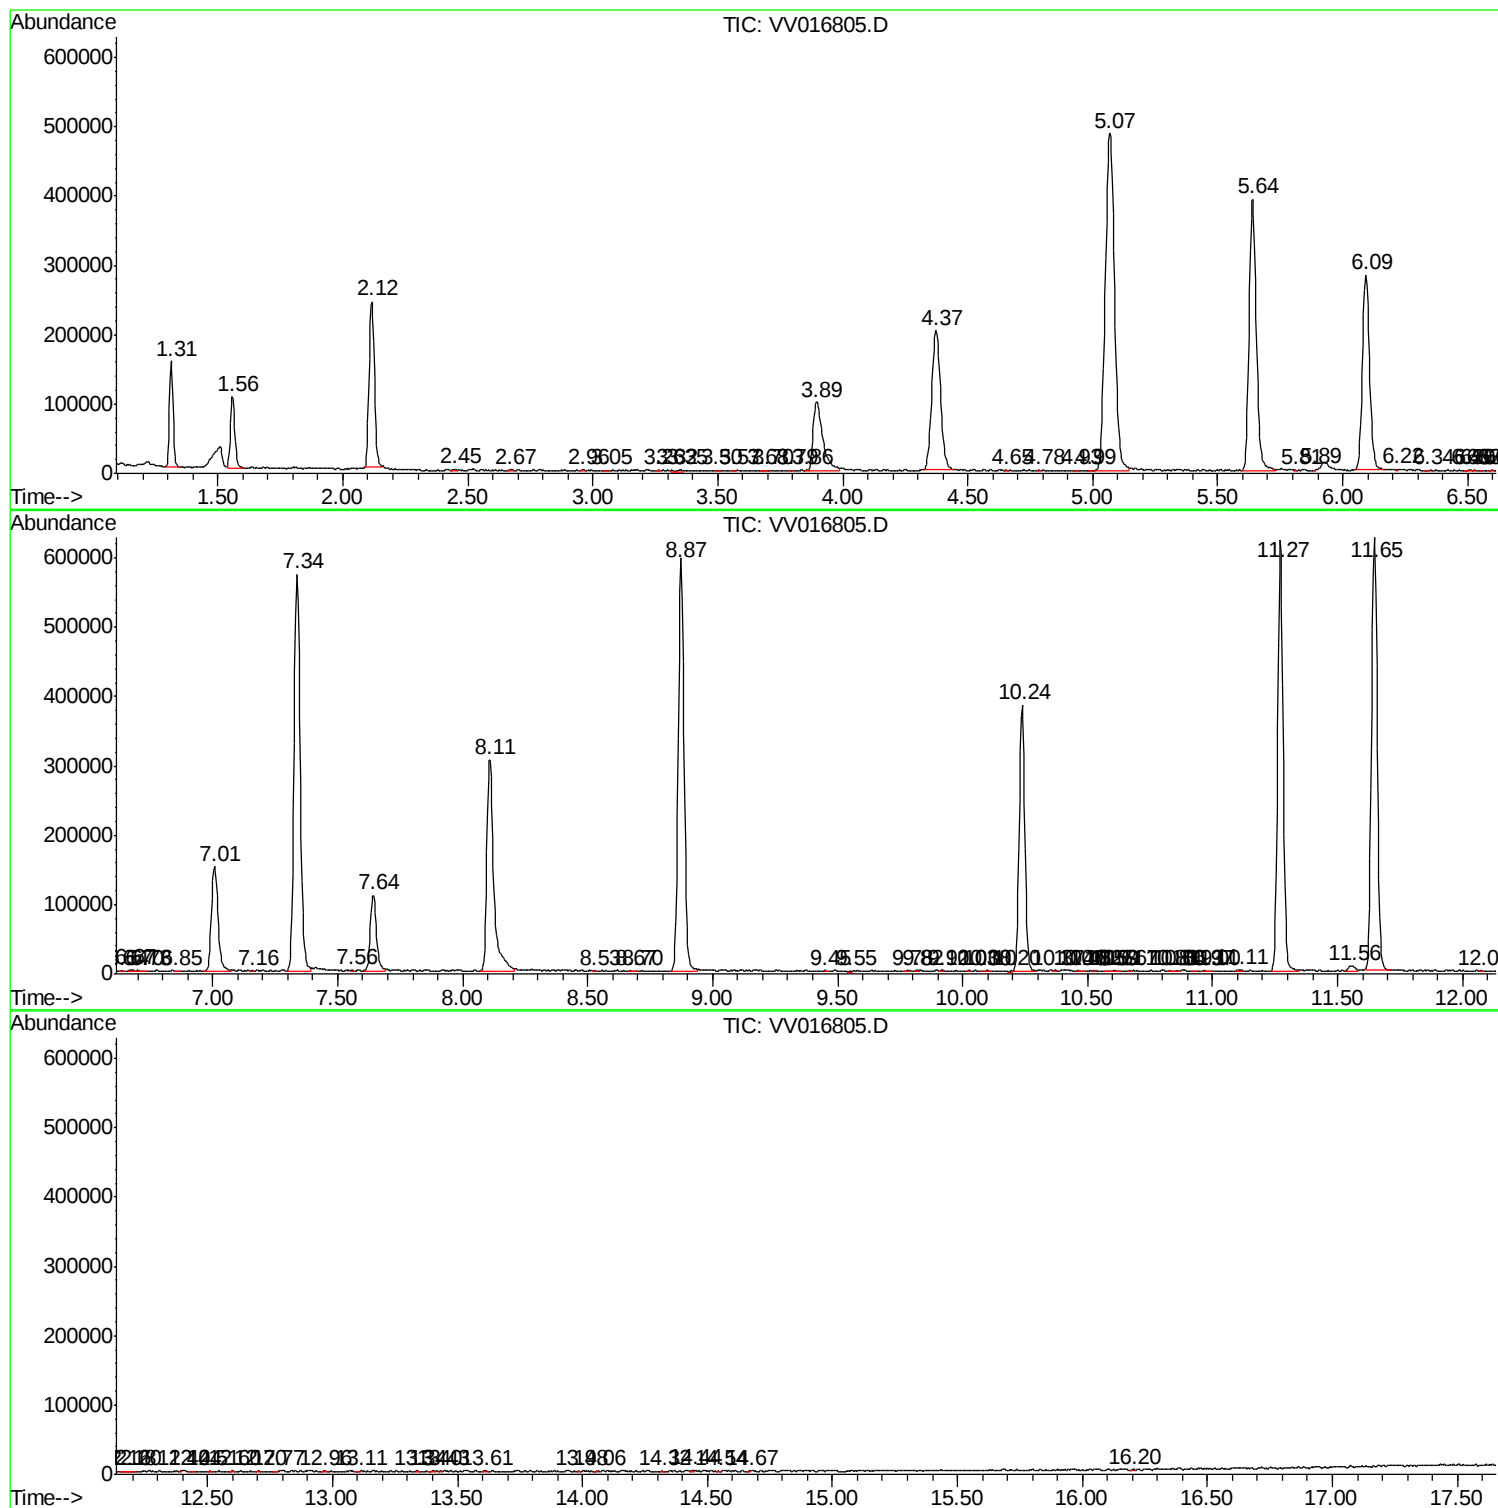

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV061020\
Data File : VV016805.D
Acq On : 11 Jun 2020 05:56
Operator : SY/MD
Sample : L2901-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTT5

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV061020\
Data File : VV016805.D
Acq On : 11 Jun 2020 05:56
Operator : SY/MD
Sample : L2901-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTT5

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc