

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061020\
 Data File : VV016806.D
 Acq On : 11 Jun 2020 06:20
 Operator : SY/MD
 Sample : L2945-01
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW0M6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.312	63	69	82	rVB	151694	157160	13.19%	1.690%
2	1.557	139	145	158	rVB	103909	126479	10.62%	1.360%
3	2.116	309	319	333	rBV	226368	334080	28.04%	3.592%
4	2.450	418	423	425	rBV5	1811	1742	0.15%	0.019%
5	2.614	472	474	476	rBV3	1220	666	0.06%	0.007%
6	2.717	503	506	509	rBV5	1871	1262	0.11%	0.014%
7	2.759	515	519	522	rBV6	2075	2278	0.19%	0.024%
8	2.814	534	536	539	rBV4	1028	771	0.06%	0.008%
9	2.981	587	588	592	rBV4	1125	667	0.06%	0.007%
10	3.068	613	615	619	rBV4	1044	809	0.07%	0.009%
11	3.229	662	665	669	rBV5	1307	1091	0.09%	0.012%
12	3.254	669	673	677	rVB7	1605	1373	0.12%	0.015%
13	3.274	677	679	682	rBV2	1418	790	0.07%	0.008%
14	3.315	690	692	694	rBV3	1420	746	0.06%	0.008%
15	3.405	715	720	721	rBV4	1196	876	0.07%	0.009%
16	3.467	737	739	741	rBV2	2148	1410	0.12%	0.015%
17	3.518	751	755	757	rBV5	2723	1629	0.14%	0.018%
18	3.611	782	784	789	rVB5	2120	1597	0.13%	0.017%
19	3.634	789	791	793	rBV3	1723	786	0.07%	0.008%
20	3.820	845	849	851	rBV5	1563	1311	0.11%	0.014%
21	3.894	863	872	907	rBV2	90362	273718	22.98%	2.943%
22	4.135	943	947	950	rBV6	1269	1136	0.10%	0.012%
23	4.190	962	964	967	rBV4	1518	785	0.07%	0.008%
24	4.235	973	978	981	rBV6	2529	2469	0.21%	0.027%
25	4.312	998	1002	1003	rBV4	1756	1138	0.10%	0.012%
26	4.373	1007	1021	1048	rVV	196590	478782	40.19%	5.148%
27	4.466	1048	1050	1053	rVB3	2289	1244	0.10%	0.013%
28	4.695	1119	1121	1123	rBV3	1442	891	0.07%	0.010%
29	4.820	1158	1160	1165	rVB5	1443	1050	0.09%	0.011%
30	4.843	1165	1167	1169	rBV3	1567	867	0.07%	0.009%
31	4.901	1183	1185	1188	rBV3	1181	676	0.06%	0.007%
32	4.923	1188	1192	1198	rVV8	1040	1130	0.09%	0.012%
33	5.068	1221	1237	1260	rBV2	466632	1191266	100.00%	12.809%
34	5.431	1347	1350	1352	rBV3	1248	691	0.06%	0.007%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061020\
 Data File : VV016806.D
 Acq On : 11 Jun 2020 06:20
 Operator : SY/MD
 Sample : L2945-01
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW0M6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

35	5.640	1399	1415	1440	rBV	387669	785084	65.90%	8.441%
36	6.093	1540	1556	1580	rBV2	264423	543671	45.64%	5.846%
37	6.540	1690	1695	1701	rVB9	2129	2119	0.18%	0.023%
38	6.720	1748	1751	1756	rBV6	1719	1749	0.15%	0.019%
39	6.846	1788	1790	1791	rBV	1431	716	0.06%	0.008%
40	6.878	1798	1800	1802	rBV3	1494	929	0.08%	0.010%
41	7.007	1829	1840	1855	rVV	144982	258451	21.70%	2.779%
42	7.084	1861	1864	1868	rBV6	1674	1367	0.11%	0.015%
43	7.267	1915	1921	1923	rBV5	2317	2121	0.18%	0.023%
44	7.338	1930	1943	1958	rBV	546502	931770	78.22%	10.019%
45	7.640	2026	2037	2055	rBV	106177	181318	15.22%	1.950%
46	8.029	2155	2158	2164	rBV6	1496	1361	0.11%	0.015%
47	8.109	2171	2183	2213	rBV	283245	550359	46.20%	5.918%
48	8.482	2297	2299	2303	rVB5	1514	788	0.07%	0.008%
49	8.566	2320	2325	2328	rBV6	1742	1698	0.14%	0.018%
50	8.871	2409	2420	2440	rBV	589441	940676	78.96%	10.114%
51	9.219	2525	2528	2530	rBV3	1739	964	0.08%	0.010%
52	9.309	2554	2556	2559	rBV4	1067	821	0.07%	0.009%
53	9.351	2567	2569	2572	rVB4	1722	817	0.07%	0.009%
54	9.367	2572	2574	2575	rBV2	1777	799	0.07%	0.009%
55	9.421	2587	2591	2592	rBV5	1376	983	0.08%	0.011%
56	9.457	2598	2602	2604	rVB6	1215	792	0.07%	0.009%
57	9.479	2604	2609	2612	rBV6	2458	2230	0.19%	0.024%
58	9.605	2647	2648	2653	rVB5	1389	674	0.06%	0.007%
59	9.714	2679	2682	2683	rBV2	1626	880	0.07%	0.009%
60	9.788	2703	2705	2708	rBV4	1037	732	0.06%	0.008%
61	9.830	2715	2718	2722	rBV5	1921	1612	0.14%	0.017%
62	9.974	2760	2763	2766	rBV5	1459	1247	0.10%	0.013%
63	10.084	2794	2797	2799	rBV3	1798	988	0.08%	0.011%
64	10.180	2823	2827	2830	rBV5	1666	1171	0.10%	0.013%
65	10.238	2834	2845	2859	rBV	367593	563595	47.31%	6.060%
66	10.334	2873	2875	2878	rBV4	2261	1304	0.11%	0.014%
67	10.428	2902	2904	2909	rVB4	1181	824	0.07%	0.009%
68	10.450	2909	2911	2915	rBV4	1419	1095	0.09%	0.012%
69	10.543	2938	2940	2945	rBV6	1535	1167	0.10%	0.013%
70	11.016	3085	3087	3088	rBV2	1565	702	0.06%	0.008%
71	11.074	3103	3105	3107	rVB2	2378	890	0.07%	0.010%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061020\
 Data File : VV016806.D
 Acq On : 11 Jun 2020 06:20
 Operator : SY/MD
 Sample : L2945-01
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW0M6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

72	11.132	3120	3123	3126	rVB5	1861	1032	0.09%	0.011%
73	11.151	3126	3129	3133	rBV6	1604	1305	0.11%	0.014%
74	11.219	3145	3150	3152	rBV5	1324	1180	0.10%	0.013%
75	11.270	3154	3166	3183	rVV	620671	939442	78.86%	10.101%
76	11.479	3229	3231	3236	rVB6	1874	1105	0.09%	0.012%
77	11.505	3236	3239	3244	rVB6	1973	1134	0.10%	0.012%
78	11.646	3272	3283	3301	rBV	608275	952454	79.95%	10.241%
79	11.823	3336	3338	3341	rBV3	1085	801	0.07%	0.009%
80	11.852	3345	3347	3351	rBV4	2296	1443	0.12%	0.016%
81	11.942	3372	3375	3379	rBV5	1624	974	0.08%	0.010%
82	12.064	3411	3413	3417	rBV3	1267	832	0.07%	0.009%
83	12.103	3422	3425	3427	rBV3	1392	895	0.08%	0.010%
84	12.145	3432	3438	3439	rBV5	837	799	0.07%	0.009%
85	12.617	3583	3585	3587	rBV2	1480	881	0.07%	0.009%
86	12.672	3599	3602	3605	rBV5	1967	1574	0.13%	0.017%
87	12.823	3646	3649	3653	rBV5	932	770	0.06%	0.008%
88	12.855	3656	3659	3661	rBV4	1456	1053	0.09%	0.011%
89	12.939	3683	3685	3688	rBV3	1202	679	0.06%	0.007%
90	13.141	3745	3748	3749	rBV3	1453	888	0.07%	0.010%
91	13.309	3798	3800	3802	rBV2	1461	756	0.06%	0.008%
92	13.392	3824	3826	3830	rBV5	1389	1118	0.09%	0.012%
93	13.431	3836	3838	3843	rVB5	1229	916	0.08%	0.010%
94	13.492	3854	3857	3859	rBV4	1852	1206	0.10%	0.013%
95	13.653	3902	3907	3909	rBV3	1160	1056	0.09%	0.011%
96	13.784	3945	3948	3951	rBV4	1556	1084	0.09%	0.012%
97	14.283	4101	4103	4105	rBV2	1191	728	0.06%	0.008%
98	14.302	4107	4109	4112	rVV2	1675	855	0.07%	0.009%
99	14.974	4316	4318	4320	rBV2	1574	869	0.07%	0.009%
100	15.058	4342	4344	4347	rBV4	1710	722	0.06%	0.008%


Sum of corrected areas: 9300381

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV061020\
Data File : VV016806.D
Acq On : 11 Jun 2020 06:20
Operator : SY/MD
Sample : L2945-01
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 48 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW0M6

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

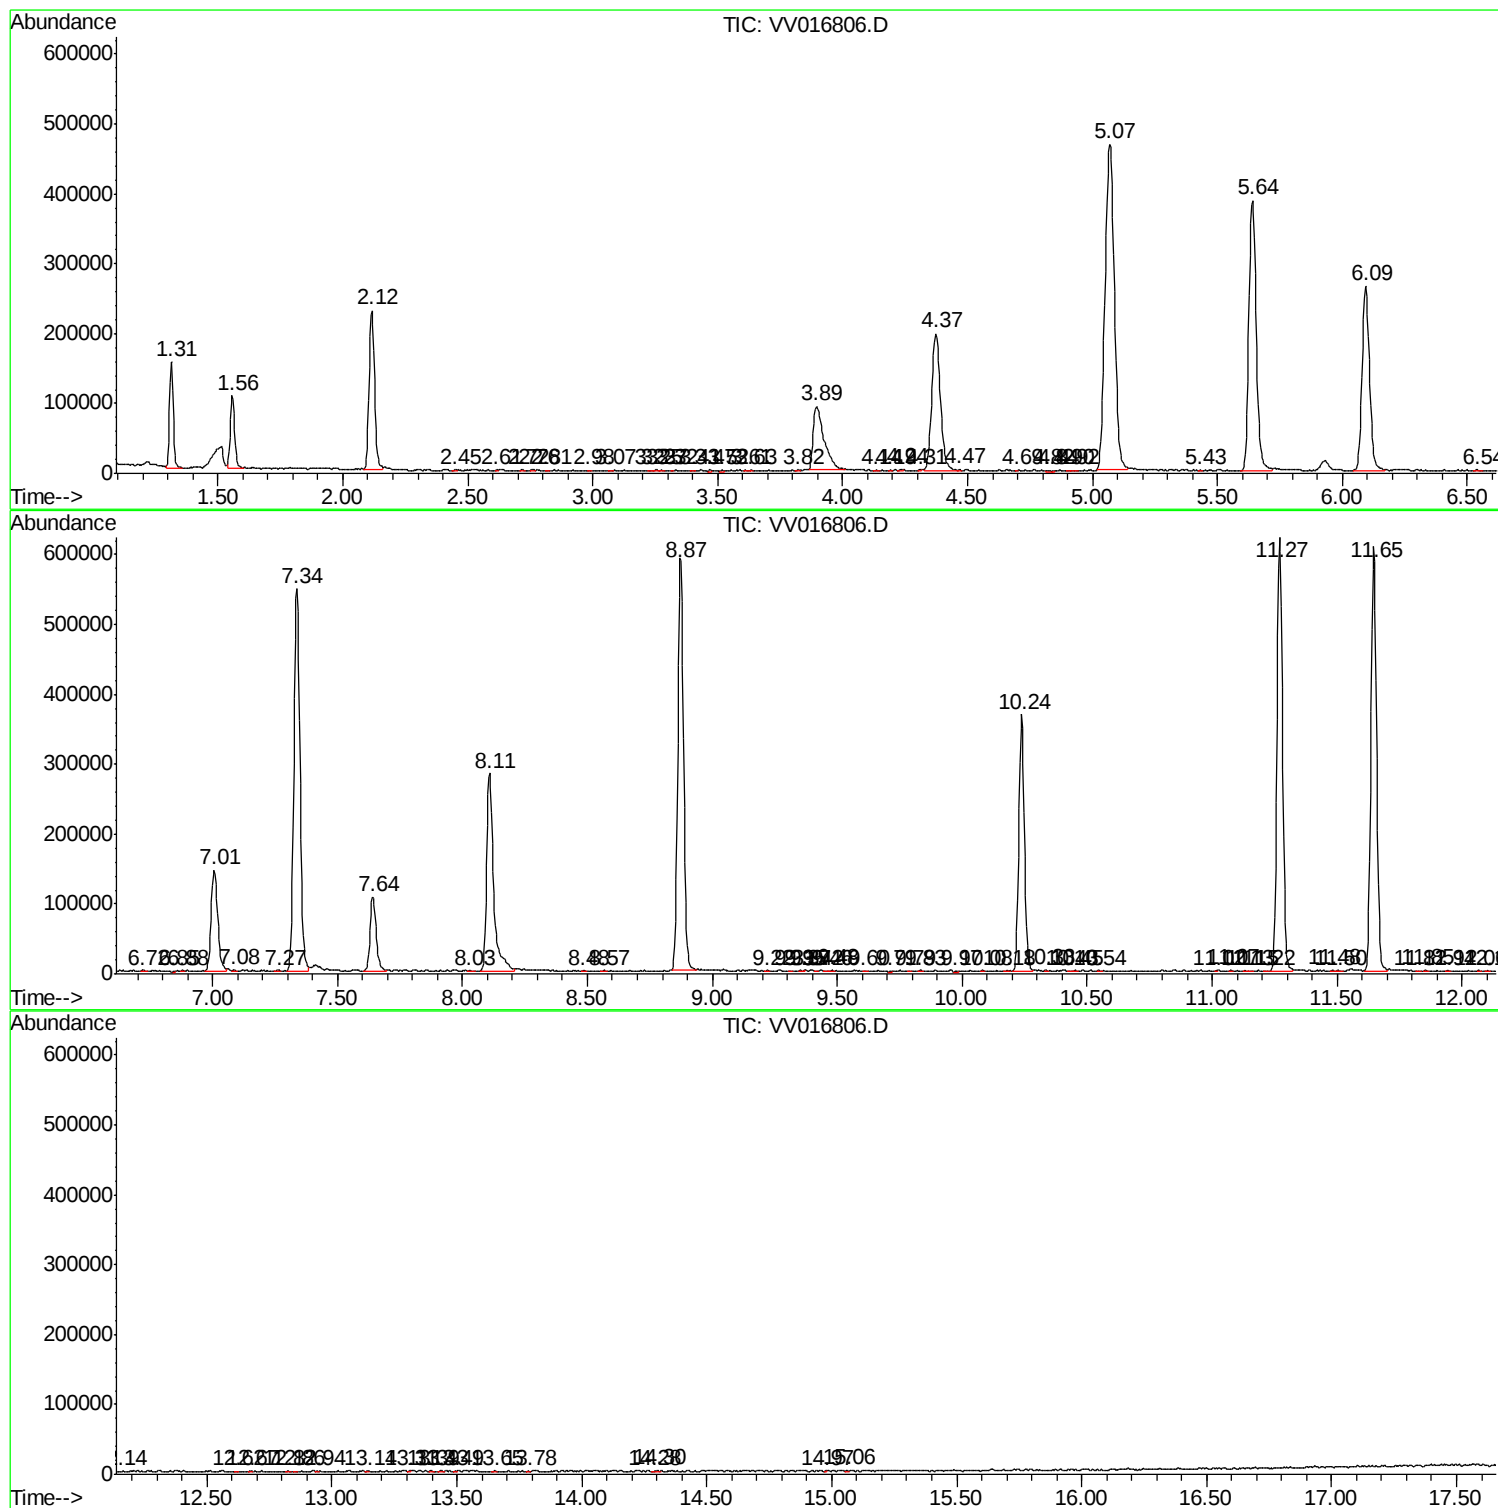

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV061020\
Data File : VV016806.D
Acq On : 11 Jun 2020 06:20
Operator : SY/MD
Sample : L2945-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 48 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW0M6

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV061020\
Data File : VV016806.D
Acq On : 11 Jun 2020 06:20
Operator : SY/MD
Sample : L2945-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 48 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW0M6

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc