


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV061020\
 Data File : VV016760.D
 Acq On : 10 Jun 2020 11:16
 Operator : SY/MD
 Sample : BFB85
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB85

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis
 Last Update : Thu Jun 11 08:28:49 2020

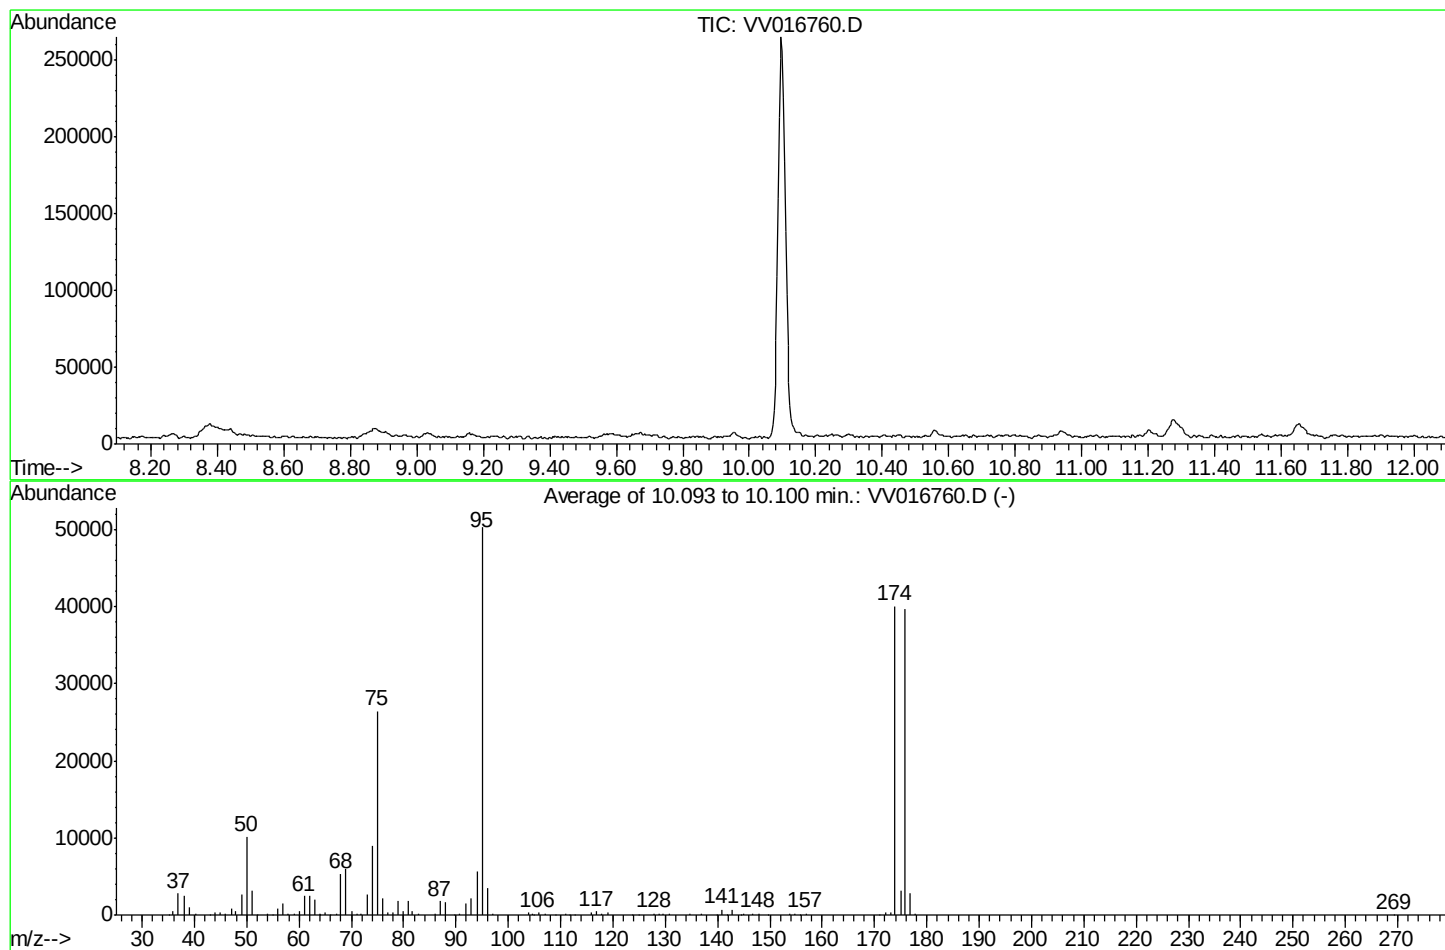

AutoFind: Scans 2800, 2801, 2802; Background Corrected with Scan 2788

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.2	10176	PASS
75	95	30	80	52.7	26469	PASS
95	95	100	100	100.0	50269	PASS
96	95	5	9	7.1	3545	PASS
173	174	0.00	2	0.7	279	PASS
174	95	50	120	79.6	40008	PASS
175	174	5	9	8.0	3214	PASS
176	174	95	101	99.1	39648	PASS
177	176	5	9	7.2	2858	PASS

m/z	Abundance
35.90	676.0
37.00	2881.0
38.00	2693.0
39.00	1106.0
39.90	388.0
40.20	287.0
41.20	155.0
42.00	105.0
43.00	187.0
44.00	874.0
44.90	648.0
45.80	130.0
47.10	668.0
47.90	396.0
49.00	2726.0
50.00	10089.0
51.00	3267.0
52.10	227.0
54.00	156.0
54.90	132.0
55.90	742.0
57.00	1331.0
57.90	161.0
59.00	146.0
60.00	652.0
61.00	2416.0
62.00	2384.0
63.00	2108.0
63.90	279.0
65.00	344.0
67.10	253.0
68.00	5353.0
69.00	5955.0
70.00	547.0
71.00	145.0
71.90	284.0
73.00	2578.0
74.00	9022.0
75.00	26728.0
76.00	2201.0
77.00	391.0
78.20	208.0
78.90	1746.0
79.90	474.0
80.80	1688.0
81.70	451.0
82.90	139.0
86.00	183.0
87.00	1874.0
87.90	1728.0
90.60	219.0
92.00	1526.0
93.00	2228.0
94.00	5419.0
95.00	48616.0
96.00	3493.0
97.00	162.0
103.90	284.0
104.70	152.0
105.80	273.0
107.00	165.0
108.90	107.0
110.90	112.0
111.70	113.0
112.80	107.0
115.90	322.0
116.80	409.0
117.90	290.0
119.00	346.0
128.00	201.0
128.80	181.0
129.60	118.0
134.80	162.0
136.80	144.0
139.80	124.0
140.90	705.0
141.80	103.0
142.80	647.0
145.00	197.0
146.70	105.0
147.80	165.0
153.70	126.0
154.90	171.0
155.70	112.0
156.90	168.0
172.00	394.0
173.10	838.0
173.90	38352.0
175.00	3339.0
175.90	37136.0
176.90	2748.0
177.80	160.0

Instrument :
MSVOA_V
ClientSampleId :
BFB85

m/z	Abundance
35.20	118.0
35.90	746.0
37.00	2935.0
38.00	2730.0
39.00	1111.0
39.90	386.0
41.20	140.0
42.00	119.0
43.10	200.0
44.00	843.0
44.90	599.0
45.90	132.0
47.10	789.0
48.00	414.0
49.00	2866.0
50.00	10348.0
51.00	3239.0
52.10	200.0
54.00	127.0
54.90	180.0
55.90	741.0
57.00	1540.0
57.90	168.0
59.00	138.0
60.00	654.0
61.00	2580.0
62.00	2574.0
63.00	2070.0
64.10	302.0
65.00	379.0
67.10	265.0
68.00	5656.0
69.00	6190.0
70.00	516.0
71.00	162.0
72.00	357.0
73.00	2867.0
74.00	9257.0
75.00	27448.0
76.00	2301.0
77.00	325.0
78.00	277.0
78.90	1928.0
79.80	531.0
80.90	1880.0
81.70	481.0
82.90	143.0
85.90	209.0
87.00	1918.0
87.90	1692.0
89.70	108.0
90.70	189.0
92.00	1570.0
93.00	2300.0
94.00	5689.0
95.00	52160.0
96.00	3640.0
97.00	172.0
103.90	258.0
104.60	145.0
105.80	324.0
107.00	211.0
109.00	113.0
110.90	118.0
115.90	357.0
116.80	471.0
117.90	248.0
119.00	341.0
127.90	193.0
128.90	191.0
129.70	171.0
130.80	126.0
134.80	215.0
136.90	154.0
139.80	119.0
140.90	731.0
142.80	660.0
144.50	100.0
145.00	195.0
146.70	136.0
147.80	204.0
153.80	123.0
154.80	143.0
156.90	195.0
171.00	111.0
172.00	403.0
173.90	41312.0
175.00	3329.0
175.90	40976.0
176.90	2960.0
177.90	140.0

Instrument :
MSVOA_V
ClientSampleId :
BFB85

m/z	Abundance
35.10	141.0
35.90	695.0
37.00	2835.0
38.00	2502.0
39.00	1063.0
40.00	386.0
41.20	113.0
42.10	142.0
43.10	242.0
44.00	668.0
44.90	532.0
46.00	130.0
47.10	888.0
47.90	372.0
48.10	368.0
49.00	2556.0
50.00	10091.0
51.00	3024.0
52.10	166.0
53.80	112.0
54.90	215.0
55.90	797.0
57.00	1599.0
57.90	193.0
59.00	109.0
60.00	643.0
61.00	2607.0
62.00	2578.0
63.00	1894.0
64.00	301.0
65.00	328.0
66.00	131.0
67.10	224.0
68.00	5189.0
69.00	5670.0
70.10	408.0
71.00	150.0
72.00	436.0
73.00	2709.0
74.00	8733.0
75.00	25232.0
76.00	2220.0
77.10	257.0
77.90	330.0
78.90	1912.0
79.80	581.0
80.90	1872.0
81.70	407.0
83.00	156.0
86.00	196.0
87.00	1846.0
87.90	1639.0
89.70	106.0
90.80	179.0
92.00	1525.0
92.90	2113.0
94.00	5808.0
95.00	50032.0
96.00	3504.0
96.90	155.0
104.00	267.0
104.90	101.0
105.80	316.0
107.00	212.0
110.90	108.0
115.90	328.0
116.90	466.0
117.90	179.0
119.00	324.0
123.80	117.0
125.00	125.0
127.80	212.0
129.00	175.0
129.70	215.0
130.70	161.0
134.70	222.0
136.80	144.0
140.90	693.0
142.90	681.0
144.90	155.0
146.80	125.0
147.80	236.0
149.60	110.0
153.80	120.0
154.80	110.0
156.90	167.0
172.10	378.0
173.90	40360.0
175.00	2974.0
175.90	40832.0
176.90	2866.0
269.30	111.0

Instrument :
MSVOA_V
ClientSampleId :
BFB85

m/z	Abundance
35.80	156.0
36.30	171.0
36.80	123.0
37.80	148.0
39.00	171.0
39.90	431.0
40.70	103.0
41.30	142.0
42.00	134.0
43.00	180.0
43.90	522.0
44.90	276.0
46.80	125.0
52.20	110.0
53.50	130.0
54.90	112.0
60.00	193.0
60.90	107.0
62.80	106.0
64.20	119.0
71.90	112.0
72.90	125.0
86.90	124.0
97.70	110.0

Instrument :
MSVOA_V
ClientSampleId :
BFB85