

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061021\
 Data File : VV021535.D
 Acq On : 10 Jun 2021 11:03
 Operator : SY/MD
 Sample : VV0610MBL01
 Misc : 5.0g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Jun 11 02:44:13 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Jun 11 02:43:15 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	479000	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	451976	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	266031	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	150419	47.696	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	95.400%
7) Chloroethane-d5	1.568	69	117785	50.208	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	100.420%
11) 1,1-Dichloroethene-d2	2.105	63	196658	36.494	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	72.980%
21) 2-Butanone-d5	3.886	46	204301	90.341	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	90.340%
24) Chloroform-d	4.346	84	286677	45.665	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	91.320%
26) 1,2-Dichloroethane-d4	5.031	65	168777	46.676	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	93.360%
32) Benzene-d6	5.047	84	591662	46.794	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	93.580%
36) 1,2-Dichloropropane-d6	6.069	67	178613	45.743	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	91.480%
41) Toluene-d8	7.317	98	565845	46.973	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	93.940%
43) trans-1,3-Dichloroprop...	7.622	79	94924	45.426	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	90.860%
47) 2-Hexanone-d5	8.088	63	152450	85.026	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	85.030%
56) 1,1,2,2-Tetrachloroeth...	10.217	84	243938	45.005	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	90.020%
66) 1,2-Dichlorobenzene-d4	11.625	152	251960	45.562	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	91.120%
Target Compounds						
44) trans-1,3-Dichloropropene	7.622	75	3710	0.707	ug/L	Qvalue 90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061021\
Data File : VV021535.D
Acq On : 10 Jun 2021 11:03
Operator : SY/MD
Sample : VV0610MBL01
Misc : 5.0g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :


Quant Time: Jun 11 02:44:13 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Jun 11 02:43:15 2021
Response via : Initial Calibration

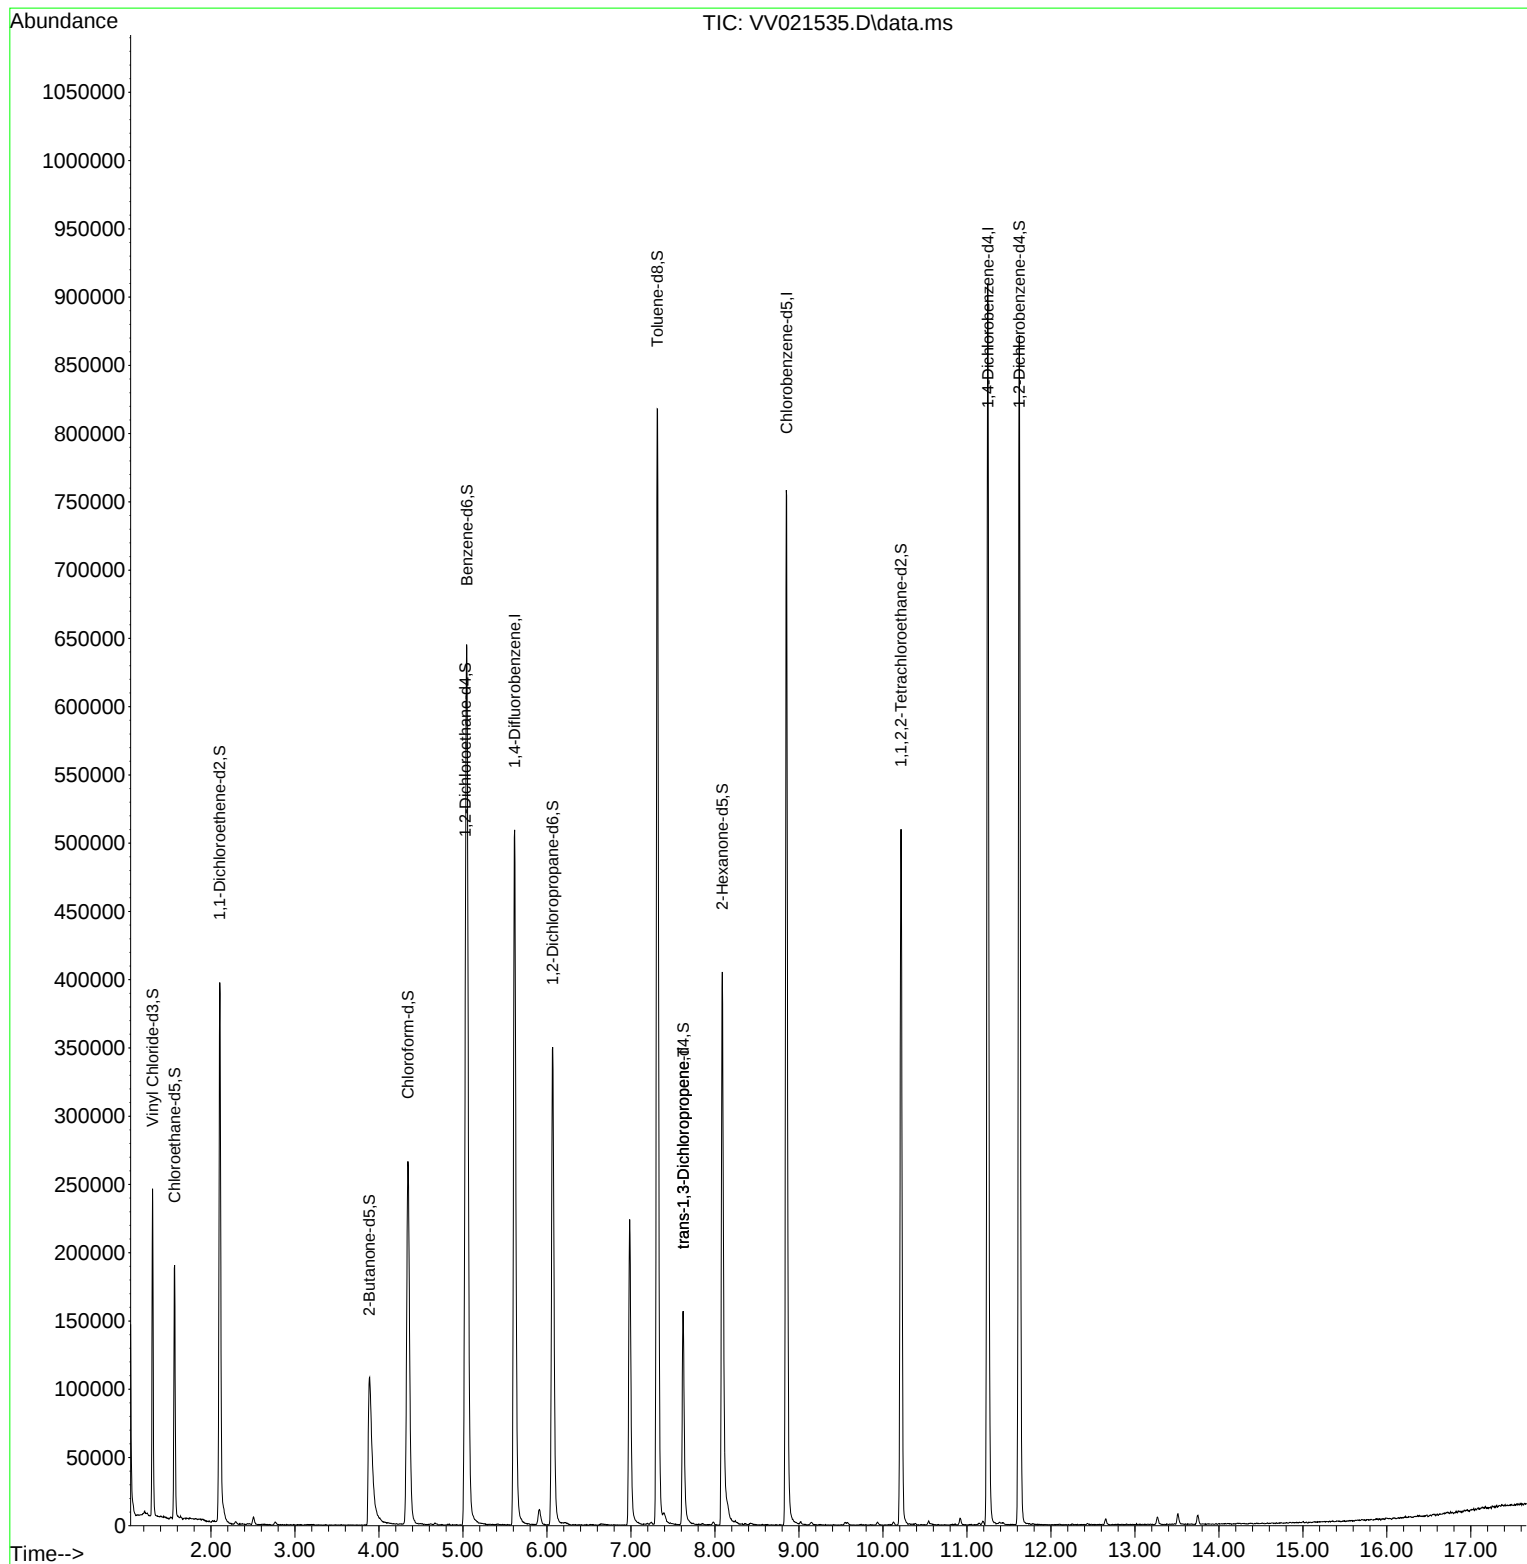

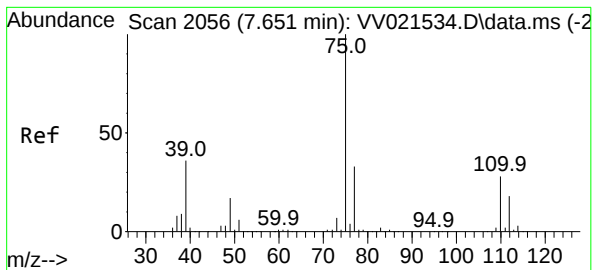

#44
 trans-1,3-Dichloropropene
 Concen: 0.707 ug/L
 RT: 7.622 min Scan# 2047
 Delta R.T. -0.029 min
 Lab File: VV021535.D
 Acq: 10 Jun 2021 11:03

Instrument :
 MSVOA_V
 ClientSampleId :

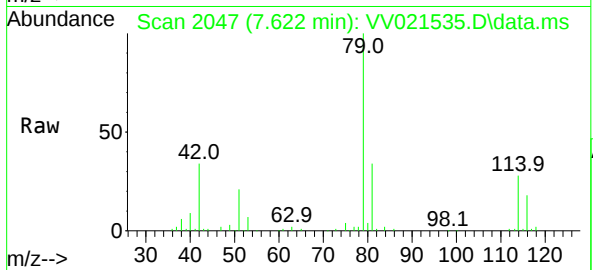

Tgt Ion: 75 Resp: 3710
 Ion Ratio Lower Upper
 75 100
 77 38.2 22.9 42.5

