

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061021\
 Data File : VV021536.D
 Acq On : 10 Jun 2021 11:26
 Operator : SY/MD
 Sample : VV0610WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Jun 11 02:44:24 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Jun 11 02:43:15 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	453981	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	430376	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	250833	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	150644	50.400	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	100.800%
7) Chloroethane-d5	1.568	69	113688	51.132	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	102.260%
11) 1,1-Dichloroethene-d2	2.108	63	192909	37.771	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	75.540%
21) 2-Butanone-d5	3.892	46	223461	104.260	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	104.260%
24) Chloroform-d	4.352	84	284597	47.832	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	95.660%
26) 1,2-Dichloroethane-d4	5.034	65	169391	49.427	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	98.860%
32) Benzene-d6	5.053	84	588671	48.894	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	97.780%
36) 1,2-Dichloropropane-d6	6.072	67	179572	48.297	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	96.600%
41) Toluene-d8	7.317	98	562041	48.998	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	98.000%
43) trans-1,3-Dichloroprop...	7.622	79	95395	47.943	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	95.880%
47) 2-Hexanone-d5	8.088	63	168068	98.442	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	98.440%
56) 1,1,2,2-Tetrachloroeth...	10.217	84	253138	49.047	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	98.100%
66) 1,2-Dichlorobenzene-d4	11.625	152	253876	48.690	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	97.380%
Target Compounds						Qvalue
44) trans-1,3-Dichloropropene	7.625	75	4047	0.810	ug/L	# 79


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061021\
Data File : VV021536.D
Acq On : 10 Jun 2021 11:26
Operator : SY/MD
Sample : VV0610WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :


Quant Time: Jun 11 02:44:24 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Jun 11 02:43:15 2021
Response via : Initial Calibration

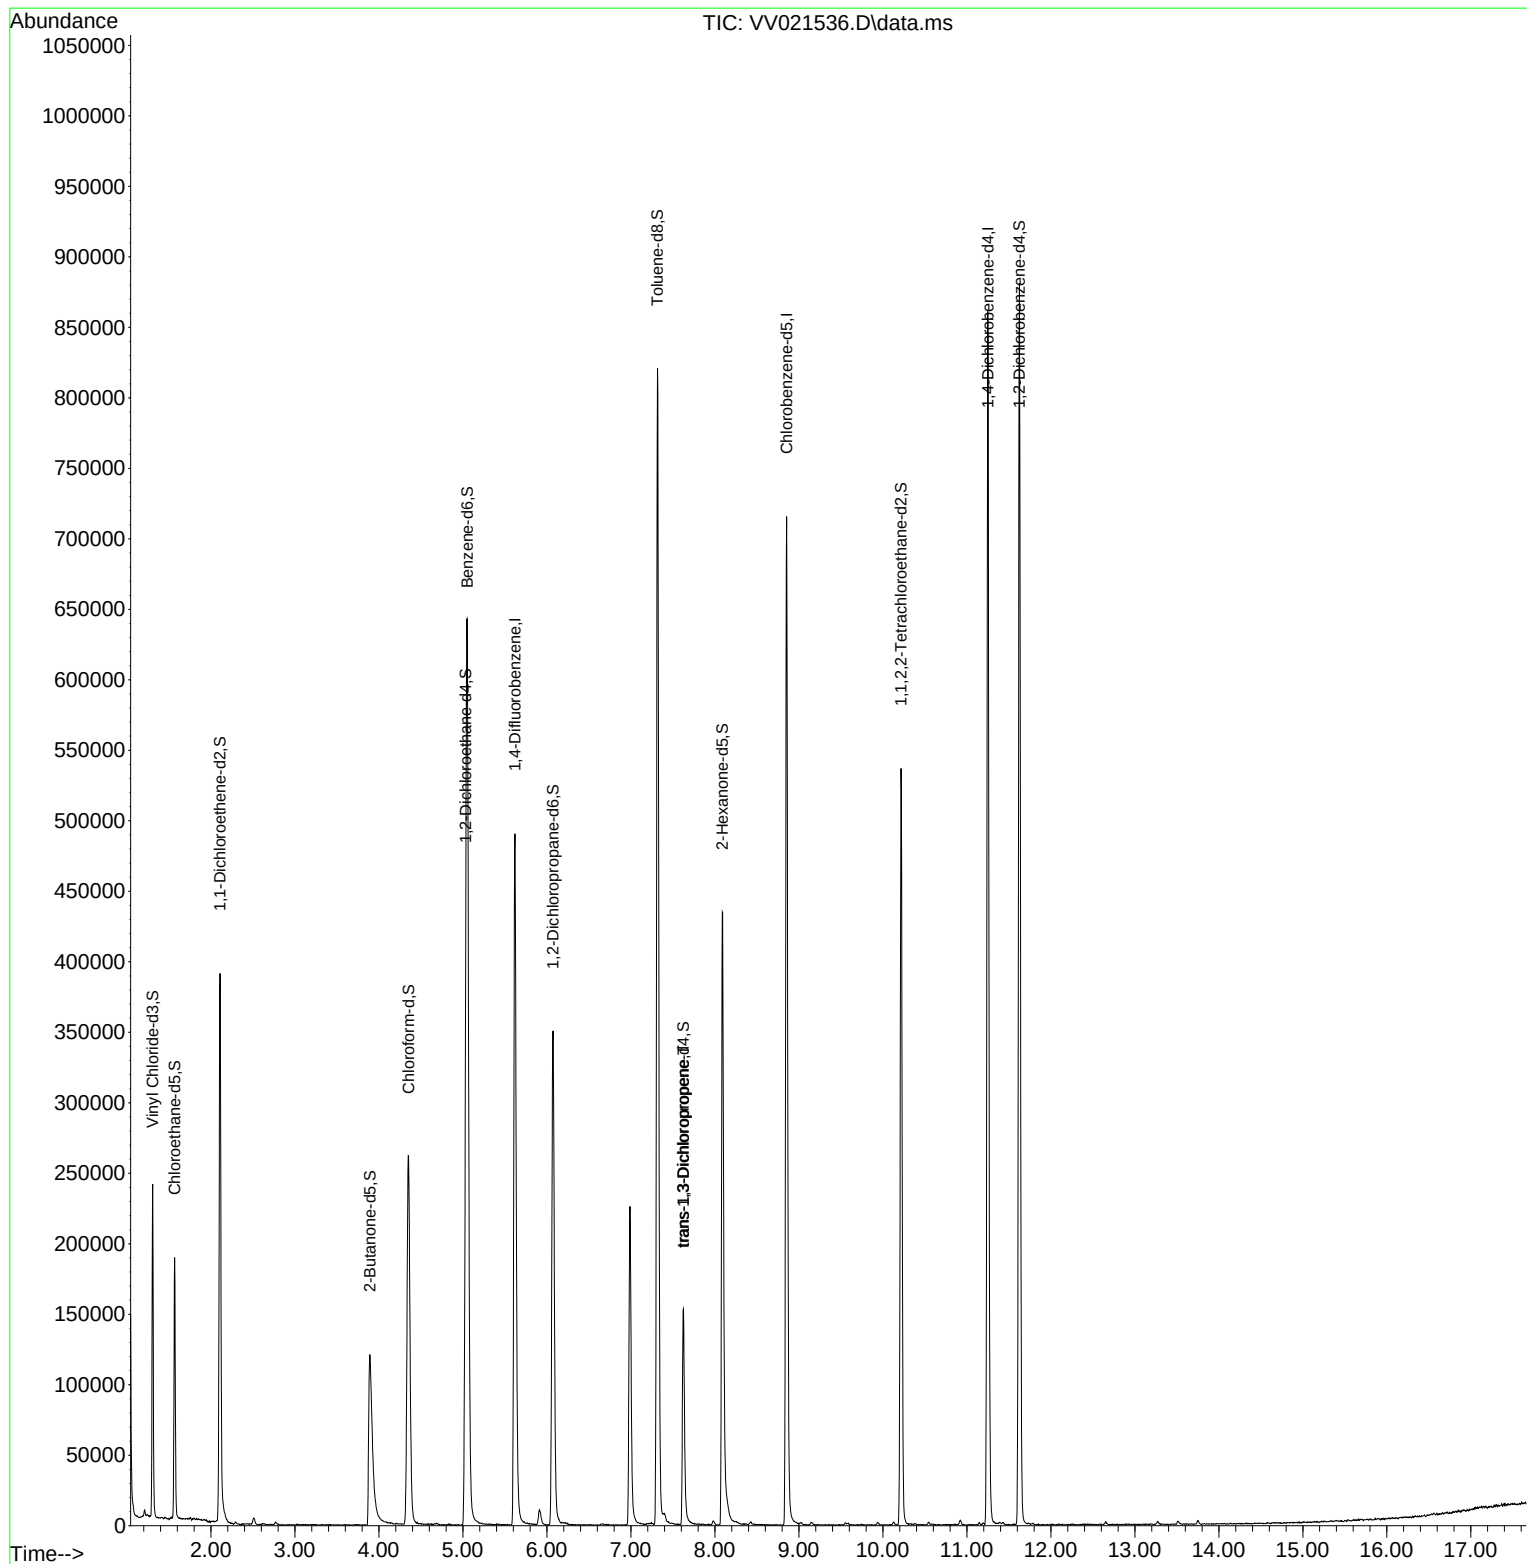

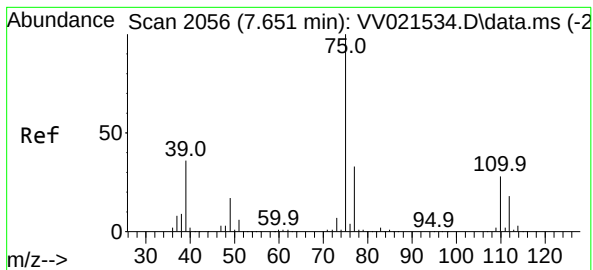

#44
 trans-1,3-Dichloropropene
 Concen: 0.810 ug/L
 RT: 7.625 min Scan# 2048
 Delta R.T. -0.026 min
 Lab File: VV021536.D
 Acq: 10 Jun 2021 11:26

Instrument :
 MSVOA_V
 ClientSampleId :

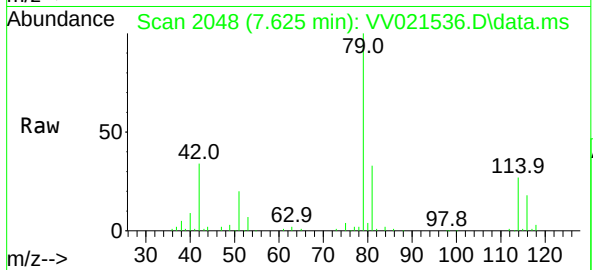

Tgt Ion: 75 Resp: 4047
 Ion Ratio Lower Upper
 75 100
 77 44.8 22.9 42.5#

