

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW061021\
 Data File : VW021538.D
 Acq On : 10 Jun 2021 12:16
 Operator : SY/MD
 Sample : M2649-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 B0AA7

Quant Time: Jun 11 02:44:44 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Jun 11 02:43:15 2021
 Response via : Initial Calibration

Compound		R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards							
1) 1,4-Difluorobenzene		5.619	114	445734	50.000	ug/L	0.00
28) Chlorobenzene-d5		8.854	117	423844	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4		11.249	152	246414	50.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3		1.304	65	147119	50.131	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	100.260%	
7) Chloroethane-d5		1.568	69	112991	51.759	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	103.520%	
11) 1,1-Dichloroethene-d2		2.108	63	191812	38.251	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	76.500%	
21) 2-Butanone-d5		3.889	46	226939	107.841	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	107.840%	
24) Chloroform-d		4.352	84	286119	48.977	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	97.960%	
26) 1,2-Dichloroethane-d4		5.034	65	173023	51.421	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	102.840%	
32) Benzene-d6		5.053	84	588926	49.669	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	99.340%	
36) 1,2-Dichloropropane-d6		6.072	67	179687	49.072	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	98.140%	
41) Toluene-d8		7.317	98	561359	49.693	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	99.380%	
43) trans-1,3-Dichloroprop...		7.622	79	94835	48.396	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	96.800%	
47) 2-Hexanone-d5		8.088	63	173592	103.244	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	103.240%	
56) 1,1,2,2-Tetrachloroeth...		10.217	84	256220	50.409	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	100.820%	
66) 1,2-Dichlorobenzene-d4		11.625	152	252488	49.292	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	98.580%	
Target Compounds							Qvalue
13) Acetone		2.185	43	6231	3.441	ug/L	# 91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061021\
Data File : VV021538.D
Acq On : 10 Jun 2021 12:16
Operator : SY/MD
Sample : M2649-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
B0AA7

Quant Time: Jun 11 02:44:44 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Jun 11 02:43:15 2021
Response via : Initial Calibration

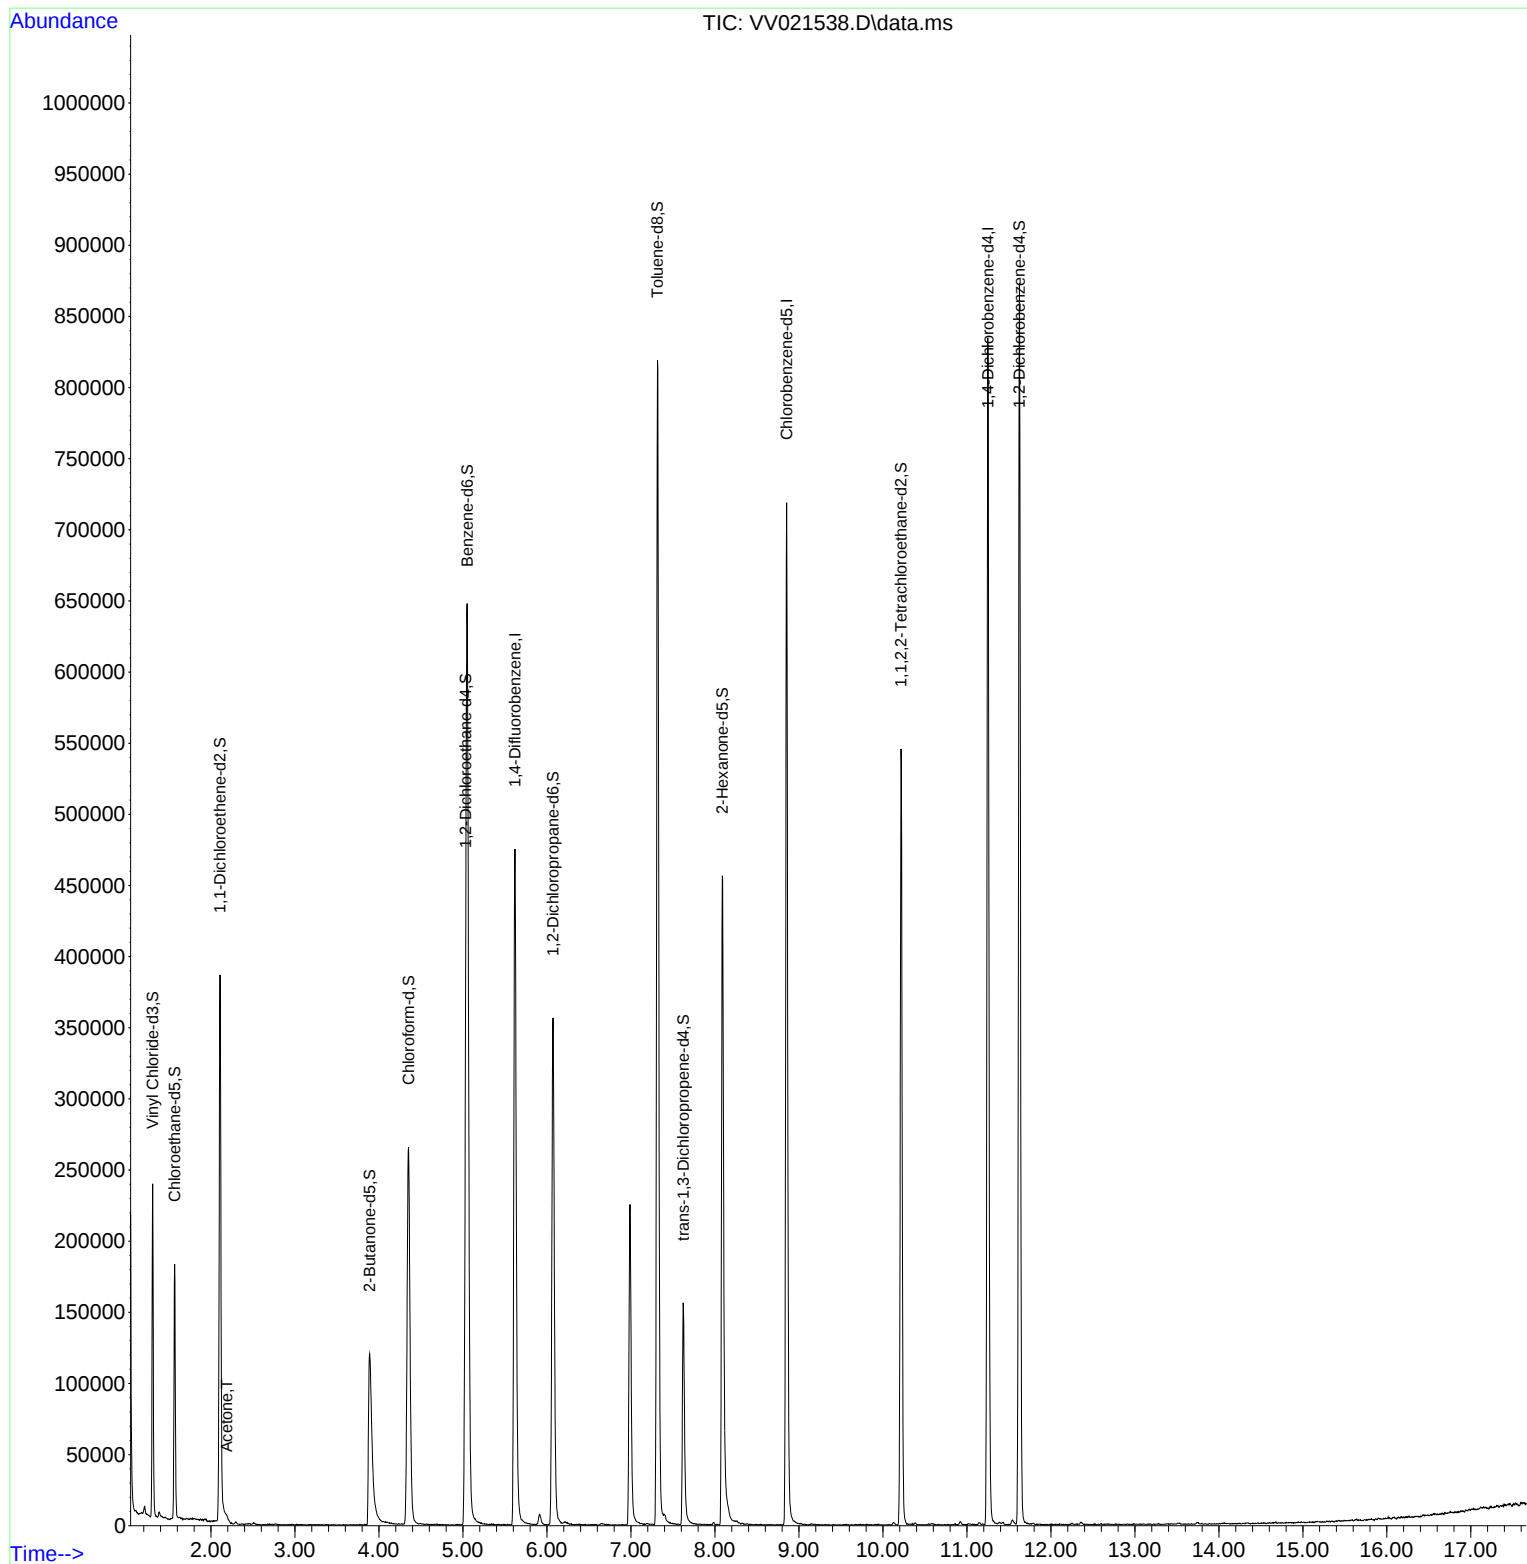

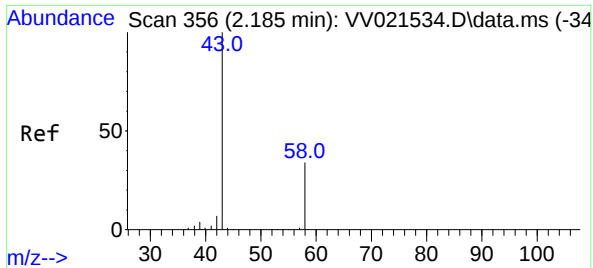

#13
 Acetone
 Concen: 3.441 ug/L
 RT: 2.185 min Scan# 356
 Delta R.T. 0.000 min
 Lab File: VV021538.D
 Acq: 10 Jun 2021 12:16

Instrument :
 MSVOA_V
 ClientSampleId :
 B0AA7

Tgt Ion: 43 Resp: 6231

Ion	Ratio	Lower	Upper
43	100		
58	22.3	0.0	0.2#

