

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061021\
 Data File : VV021535.D
 Acq On : 10 Jun 2021 11:03
 Operator : SY/MD
 Sample : VV0610MBL01
 Misc : 5.0g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK189

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
 Title : VOC Analysis

Signal : TIC: VV021535.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	94	rVB	239194	238068	14.36%	1.793%
2	1.568	157	164	176	rVB	183848	204846	12.35%	1.543%
3	2.105	322	331	369	rVB	396380	604359	36.45%	4.553%
4	2.507	448	456	465	rBV2	5593	8650	0.52%	0.065%
5	2.609	485	488	490	rBV2	545	373	0.02%	0.003%
6	2.677	507	509	512	rBV2	355	167	0.01%	0.001%
7	2.696	512	515	520	rVB3	370	339	0.02%	0.003%
8	2.725	523	524	526	rBV	192	75	0.00%	0.001%
9	2.764	529	536	546	rBV5	2085	3600	0.22%	0.027%
10	2.876	569	571	575	rVB	238	127	0.01%	0.001%
11	2.899	575	578	579	rBV	383	161	0.01%	0.001%
12	2.944	588	592	593	rBV2	340	243	0.01%	0.002%
13	2.989	603	606	609	rVB3	447	313	0.02%	0.002%
14	3.011	612	613	617	rBV	193	101	0.01%	0.001%
15	3.031	617	619	620	rBV	243	84	0.01%	0.001%
16	3.082	633	635	641	rBV2	196	136	0.01%	0.001%
17	3.143	651	654	657	rBV3	348	263	0.02%	0.002%
18	3.179	662	665	666	rBV	258	109	0.01%	0.001%
19	3.281	695	697	699	rBV	211	101	0.01%	0.001%
20	3.317	706	708	712	rVB3	277	177	0.01%	0.001%
21	3.349	715	718	721	rBV2	322	215	0.01%	0.002%
22	3.368	721	724	725	rBV2	338	162	0.01%	0.001%
23	3.407	734	736	739	rBV	141	92	0.01%	0.001%
24	3.510	766	768	772	rVB2	210	131	0.01%	0.001%
25	3.552	778	781	784	rBV	451	300	0.02%	0.002%
26	3.642	806	809	813	rBV	254	143	0.01%	0.001%
27	3.764	845	847	852	rVB	276	216	0.01%	0.002%
28	3.799	852	858	863	rBV2	366	459	0.03%	0.003%
29	3.835	867	869	872	rVB2	385	141	0.01%	0.001%
30	3.889	872	886	922	rBV	108244	357745	21.57%	2.695%
31	4.346	1013	1028	1062	rVB	265293	649657	39.18%	4.894%
32	4.719	1140	1144	1146	rBV2	339	225	0.01%	0.002%
33	4.738	1146	1150	1152	rVV3	383	236	0.01%	0.002%
34	4.751	1152	1154	1156	rBV2	429	190	0.01%	0.001%
35	4.783	1161	1164	1166	rBV	262	127	0.01%	0.001%
36	4.822	1172	1176	1178	rBV2	587	477	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061021\
 Data File : VV021535.D
 Acq On : 10 Jun 2021 11:03
 Operator : SY/MD
 Sample : VV0610MBL01
 Misc : 5.0g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK189

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
 Title : VOC Analysis

37	4.863	1186	1189	1191	rBV2	142	89	0.01%	0.001%
38	4.876	1191	1193	1197	rBV2	271	155	0.01%	0.001%
39	4.957	1215	1218	1221	rBV2	259	198	0.01%	0.001%
40	5.043	1225	1245	1284	rBV2	645022	1658183	100.00%	12.492%
41	5.301	1323	1325	1328	rBV	448	336	0.02%	0.003%
42	5.381	1348	1350	1353	rBV	374	241	0.01%	0.002%
43	5.494	1383	1385	1390	rVB4	361	185	0.01%	0.001%
44	5.532	1394	1397	1404	rBV3	559	629	0.04%	0.005%
45	5.571	1404	1409	1410	rBV	158	137	0.01%	0.001%
46	5.616	1410	1423	1454	rBV	509074	1026782	61.92%	7.735%
47	5.912	1503	1515	1531	rVB5	10956	24286	1.46%	0.183%
48	6.069	1550	1564	1595	rBV	349794	722763	43.59%	5.445%
49	6.310	1637	1639	1643	rVB2	359	209	0.01%	0.002%
50	6.449	1678	1682	1683	rBV2	275	175	0.01%	0.001%
51	6.474	1689	1690	1692	rVB2	270	79	0.00%	0.001%
52	6.510	1696	1701	1702	rBV2	435	299	0.02%	0.002%
53	6.555	1714	1715	1718	rVB	282	78	0.00%	0.001%
54	6.632	1735	1739	1741	rBV	613	545	0.03%	0.004%
55	6.770	1779	1782	1785	rVB	217	127	0.01%	0.001%
56	6.828	1796	1800	1802	rBV2	232	133	0.01%	0.001%
57	6.918	1826	1828	1830	rVB	239	77	0.00%	0.001%
58	6.986	1838	1849	1878	rBV	223843	413760	24.95%	3.117%
59	7.313	1940	1951	1971	rBV	816905	1421417	85.72%	10.708%
60	7.622	2034	2047	2075	rBV	156540	277796	16.75%	2.093%
61	7.928	2139	2142	2143	rBV	326	209	0.01%	0.002%
62	7.982	2152	2159	2166	rVB7	2258	3435	0.21%	0.026%
63	8.011	2166	2168	2171	rVV3	446	232	0.01%	0.002%
64	8.024	2171	2172	2176	rVB	241	116	0.01%	0.001%
65	8.088	2182	2192	2229	rBV	405107	744236	44.88%	5.607%
66	8.352	2271	2274	2275	rBV2	742	397	0.02%	0.003%
67	8.413	2290	2293	2294	rBV	866	493	0.03%	0.004%
68	8.535	2330	2331	2333	rBV	184	91	0.01%	0.001%
69	8.567	2338	2341	2346	rVB2	544	469	0.03%	0.004%
70	8.625	2356	2359	2361	rBV3	412	234	0.01%	0.002%
71	8.661	2367	2370	2372	rBV2	247	175	0.01%	0.001%
72	8.696	2379	2381	2384	rVB2	239	133	0.01%	0.001%
73	8.719	2384	2388	2389	rBV2	217	135	0.01%	0.001%
74	8.776	2402	2406	2408	rVB2	289	159	0.01%	0.001%
75	8.850	2417	2429	2452	rBV	758079	1231461	74.27%	9.277%
76	9.111	2506	2510	2512	rBV	333	208	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061021\
 Data File : VV021535.D
 Acq On : 10 Jun 2021 11:03
 Operator : SY/MD
 Sample : VV0610MBL01
 Misc : 5.0g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK189

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M

Title : VOC Analysis

77	9.149	2512	2522	2529	rBV8	1836	3369	0.20%	0.025%
78	9.255	2553	2555	2559	rBV2	354	266	0.02%	0.002%
79	9.320	2574	2575	2577	rVB	369	88	0.01%	0.001%
80	9.371	2588	2591	2594	rBV	160	97	0.01%	0.001%
81	9.468	2618	2621	2624	rBV	214	151	0.01%	0.001%
82	9.551	2638	2647	2651	rBV6	1968	2858	0.17%	0.022%
83	9.725	2697	2701	2702	rBV	389	276	0.02%	0.002%
84	9.934	2761	2766	2775	rVB4	1908	2535	0.15%	0.019%
85	10.027	2792	2795	2796	rBV	195	98	0.01%	0.001%
86	10.127	2822	2826	2835	rVB4	2278	2965	0.18%	0.022%
87	10.217	2840	2854	2873	rBV	509564	810434	48.87%	6.105%
88	10.423	2915	2918	2921	rVB2	348	176	0.01%	0.001%
89	10.545	2950	2956	2962	rBV3	2529	2902	0.18%	0.022%
90	10.918	3065	3072	3082	rBV4	4687	6778	0.41%	0.051%
91	11.188	3151	3156	3164	rVB5	2419	3296	0.20%	0.025%
92	11.249	3164	3175	3198	rBV	909104	1418238	85.53%	10.684%
93	11.519	3256	3259	3261	rBV2	559	334	0.02%	0.003%
94	11.625	3279	3292	3317	rBV	871161	1395421	84.15%	10.512%
95	11.783	3338	3341	3342	rBV	642	351	0.02%	0.003%
96	12.249	3484	3486	3487	rBV	629	308	0.02%	0.002%
97	12.461	3551	3552	3555	rBV2	527	249	0.02%	0.002%
98	12.654	3603	3612	3622	rBV4	4344	6872	0.41%	0.052%
99	12.799	3655	3657	3660	rVB2	535	225	0.01%	0.002%
100	13.513	3871	3879	3892	rBV2	7637	12364	0.75%	0.093%




Sum of corrected areas: 13274321

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061021\
Data File : VV021535.D
Acq On : 10 Jun 2021 11:03
Operator : SY/MD
Sample : VV0610MBL01
Misc : 5.0g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK189

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

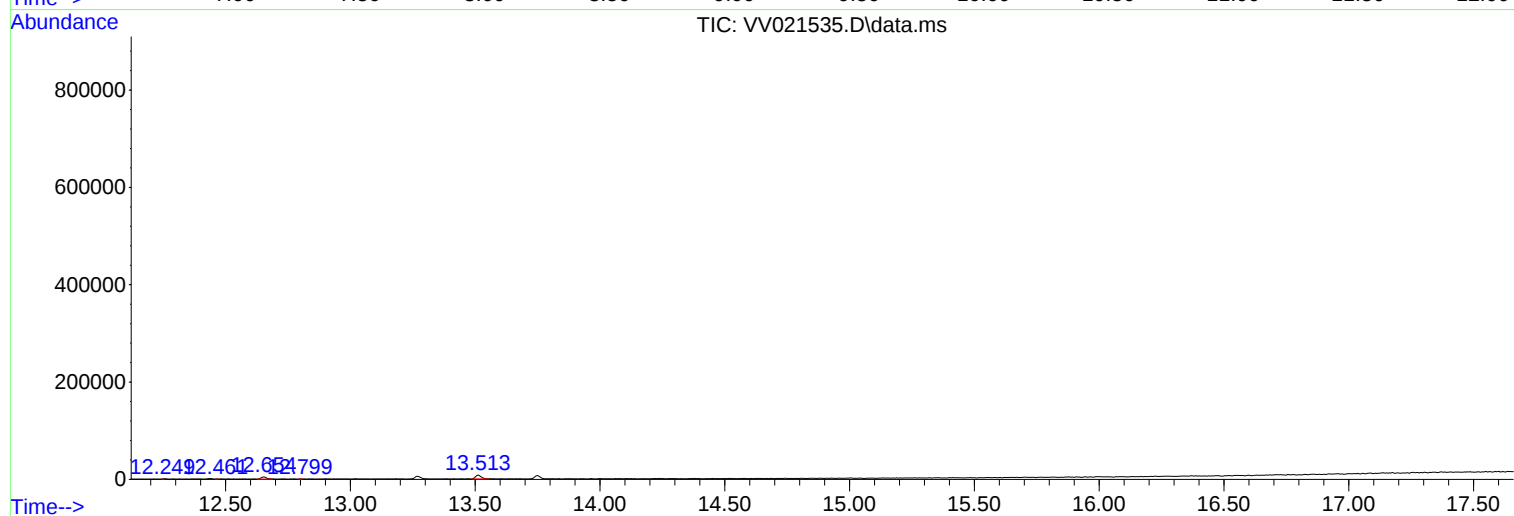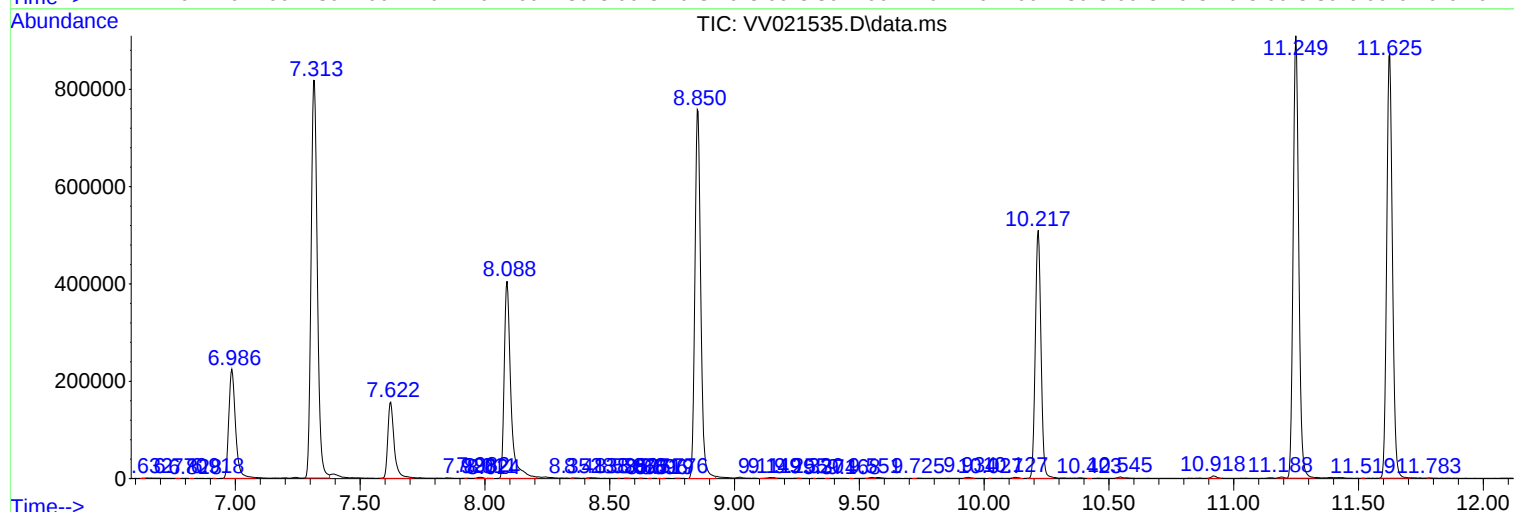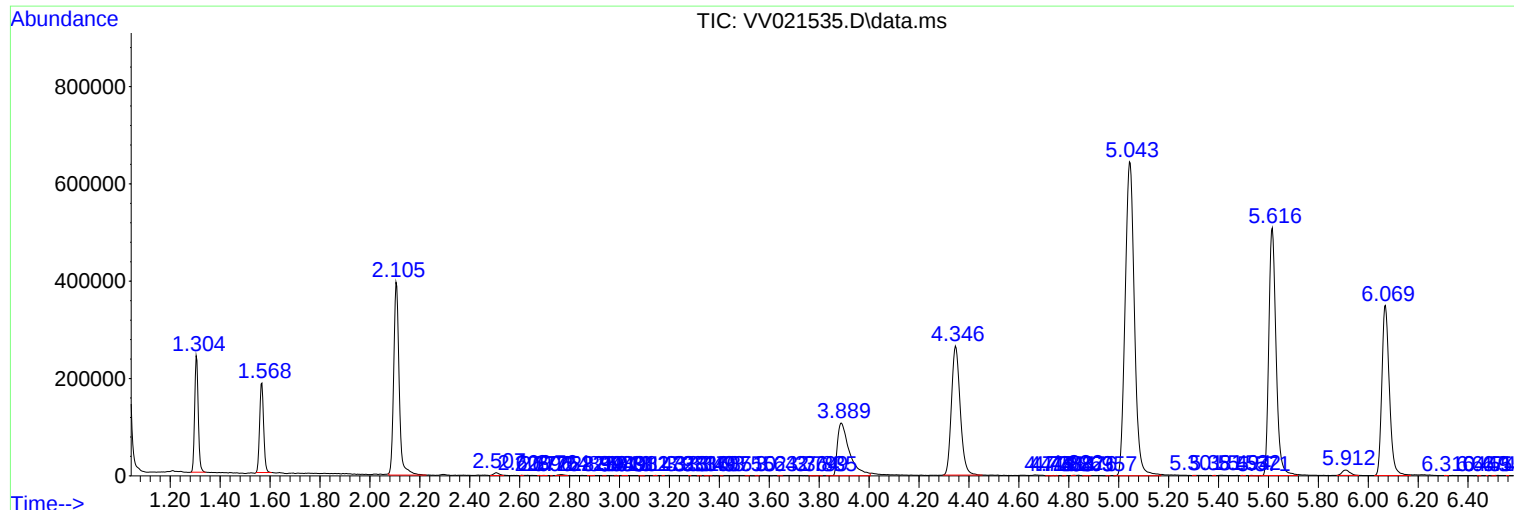

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061021\
Data File : VV021535.D
Acq On : 10 Jun 2021 11:03
Operator : SY/MD
Sample : VV0610MBL01
Misc : 5.0g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK189

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061021\
Data File : VV021535.D
Acq On : 10 Jun 2021 11:03
Operator : SY/MD
Sample : VV0610MBL01
Misc : 5.0g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK189

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
