

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061021\
 Data File : VV021537.D
 Acq On : 10 Jun 2021 11:52
 Operator : SY/MD
 Sample : M2649-15
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG5P7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M

Title : VOC Analysis

Signal : TIC: VV021537.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	96	rVB	232443	233803	14.33%	1.782%
2	1.568	157	164	177	rVB	176169	196757	12.06%	1.500%
3	2.108	322	332	349	rBV	380408	563067	34.51%	4.292%
4	2.564	470	474	475	rBV2	678	509	0.03%	0.004%
5	2.815	550	552	556	rVB3	572	360	0.02%	0.003%
6	2.838	556	559	560	rBV	197	133	0.01%	0.001%
7	2.966	595	599	602	rBV2	490	513	0.03%	0.004%
8	3.114	638	645	648	rBV3	305	309	0.02%	0.002%
9	3.179	664	665	669	rBV	236	168	0.01%	0.001%
10	3.233	678	682	684	rBV3	351	250	0.02%	0.002%
11	3.281	694	697	700	rBV2	312	201	0.01%	0.002%
12	3.314	705	707	711	rVB	173	138	0.01%	0.001%
13	3.384	727	729	735	rBV2	226	235	0.01%	0.002%
14	3.497	760	764	766	rBV2	217	132	0.01%	0.001%
15	3.552	779	781	786	rVB2	245	141	0.01%	0.001%
16	3.609	796	799	802	rVB3	383	196	0.01%	0.001%
17	3.683	816	822	825	rBV3	447	512	0.03%	0.004%
18	3.796	855	857	860	rVB2	522	240	0.01%	0.002%
19	3.889	875	886	922	rBV	106261	334676	20.51%	2.551%
20	4.349	1013	1029	1057	rBV	259647	640366	39.25%	4.881%
21	4.561	1090	1095	1096	rBV2	487	410	0.03%	0.003%
22	4.764	1154	1158	1159	rBV	320	168	0.01%	0.001%
23	4.799	1167	1169	1173	rBV	350	245	0.02%	0.002%
24	4.828	1173	1178	1184	rVB3	400	465	0.03%	0.004%
25	4.908	1198	1203	1206	rBV	426	482	0.03%	0.004%
26	4.957	1215	1218	1220	rBV	326	213	0.01%	0.002%
27	5.047	1229	1246	1275	rBV2	642796	1631379	100.00%	12.435%
28	5.314	1327	1329	1333	rBV3	320	205	0.01%	0.002%
29	5.365	1343	1345	1349	rVB2	579	269	0.02%	0.002%
30	5.455	1371	1373	1374	rBV	251	144	0.01%	0.001%
31	5.490	1383	1384	1388	rVB2	462	301	0.02%	0.002%
32	5.506	1388	1389	1391	rBV2	349	146	0.01%	0.001%
33	5.558	1401	1405	1406	rBV	648	348	0.02%	0.003%
34	5.616	1410	1423	1449	rBV	497249	1002415	61.45%	7.641%
35	5.908	1503	1514	1532	rBV3	15720	33666	2.06%	0.257%
36	6.069	1541	1564	1596	rBV	348464	730466	44.78%	5.568%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW061021\
 Data File : VW021537.D
 Acq On : 10 Jun 2021 11:52
 Operator : SY/MD
 Sample : M2649-15
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG5P7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
 Title : VOC Analysis

37	6.426	1673	1675	1680	rVB4	385	220	0.01%	0.002%
38	6.494	1691	1696	1698	rBV2	437	403	0.02%	0.003%
39	6.587	1721	1725	1727	rBV2	442	394	0.02%	0.003%
40	6.625	1732	1737	1738	rBV4	389	312	0.02%	0.002%
41	6.725	1766	1768	1772	rBV3	334	234	0.01%	0.002%
42	6.773	1779	1783	1784	rBV3	170	132	0.01%	0.001%
43	6.821	1795	1798	1800	rVV2	179	131	0.01%	0.001%
44	6.873	1811	1814	1818	rVV2	183	166	0.01%	0.001%
45	6.989	1834	1850	1878	rBV	226928	412452	25.28%	3.144%
46	7.317	1938	1952	1972	rBV	816495	1407896	86.30%	10.731%
47	7.622	2037	2047	2075	rBV	154402	271225	16.63%	2.067%
48	7.786	2096	2098	2100	rVB	522	167	0.01%	0.001%
49	7.940	2136	2146	2157	rBV2	9374	16921	1.04%	0.129%
50	8.050	2176	2180	2182	rBV2	547	408	0.03%	0.003%
51	8.088	2182	2192	2232	rBV	405309	748805	45.90%	5.708%
52	8.461	2306	2308	2311	rBV3	496	265	0.02%	0.002%
53	8.567	2339	2341	2345	rVB2	552	384	0.02%	0.003%
54	8.596	2345	2350	2355	rVB3	425	440	0.03%	0.003%
55	8.628	2358	2360	2363	rBV2	215	156	0.01%	0.001%
56	8.680	2372	2376	2378	rBV2	426	259	0.02%	0.002%
57	8.706	2381	2384	2387	rVB3	367	230	0.01%	0.002%
58	8.722	2387	2389	2393	rBV2	486	234	0.01%	0.002%
59	8.751	2395	2398	2400	rBV2	240	152	0.01%	0.001%
60	8.854	2415	2430	2456	rBV	750019	1219927	74.78%	9.299%
61	9.066	2493	2496	2497	rBV	333	178	0.01%	0.001%
62	9.153	2517	2523	2534	rVB3	1360	2052	0.13%	0.016%
63	9.233	2546	2548	2549	rBV3	299	152	0.01%	0.001%
64	9.262	2553	2557	2558	rVV2	171	137	0.01%	0.001%
65	9.304	2567	2570	2571	rBV	333	181	0.01%	0.001%
66	9.339	2579	2581	2587	rVB2	313	213	0.01%	0.002%
67	9.455	2614	2617	2621	rVB2	309	158	0.01%	0.001%
68	9.477	2621	2624	2626	rBV2	265	153	0.01%	0.001%
69	9.490	2626	2628	2633	rVB2	201	167	0.01%	0.001%
70	9.526	2637	2639	2642	rBV2	247	153	0.01%	0.001%
71	9.561	2642	2650	2654	rBV3	625	874	0.05%	0.007%
72	9.667	2679	2683	2686	rBV2	228	193	0.01%	0.001%
73	9.722	2695	2700	2702	rBV4	529	526	0.03%	0.004%
74	9.825	2723	2732	2740	rBV6	1827	3385	0.21%	0.026%
75	9.892	2750	2753	2755	rBV	310	132	0.01%	0.001%
76	9.908	2755	2758	2760	rVV2	384	205	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW061021\
 Data File : VW021537.D
 Acq On : 10 Jun 2021 11:52
 Operator : SY/MD
 Sample : M2649-15
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG5P7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
 Title : VOC Analysis

77	9.927	2762	2764	2772	rVB3	559	589	0.04%	0.004%
78	9.982	2779	2781	2784	rVB2	409	185	0.01%	0.001%
79	10.120	2819	2824	2835	rVB6	1859	3392	0.21%	0.026%
80	10.217	2841	2854	2875	rBV	522746	797890	48.91%	6.082%
81	10.384	2896	2906	2920	rVB2	18269	31679	1.94%	0.241%
82	10.458	2925	2929	2931	rBV3	364	301	0.02%	0.002%
83	10.522	2945	2949	2950	rBV2	418	288	0.02%	0.002%
84	10.661	2985	2992	2996	rVB3	560	778	0.05%	0.006%
85	10.699	3002	3004	3010	rVB2	309	239	0.01%	0.002%
86	10.818	3038	3041	3043	rBV2	338	179	0.01%	0.001%
87	10.853	3051	3052	3055	rVB3	783	361	0.02%	0.003%
88	11.159	3135	3147	3153	rBV8	3093	5694	0.35%	0.043%
89	11.249	3164	3175	3195	rBV	909201	1393838	85.44%	10.624%
90	11.538	3257	3265	3280	rBV3	11263	21308	1.31%	0.162%
91	11.625	3281	3292	3312	rVV	891646	1384278	84.85%	10.551%
92	12.072	3429	3431	3435	rBV3	762	469	0.03%	0.004%
93	12.162	3455	3459	3463	rBV2	488	452	0.03%	0.003%
94	12.320	3506	3508	3510	rBV3	298	163	0.01%	0.001%
95	12.349	3510	3517	3529	rVV6	6945	11285	0.69%	0.086%
96	12.455	3548	3550	3551	rBV	384	152	0.01%	0.001%
97	12.561	3581	3583	3587	rVB2	418	215	0.01%	0.002%
98	12.606	3594	3597	3600	rBV3	788	619	0.04%	0.005%
99	12.635	3604	3606	3607	rBV	439	135	0.01%	0.001%
100	12.805	3657	3659	3664	rVB2	395	236	0.01%	0.002%




Sum of corrected areas: 13119525

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061021\
Data File : VV021537.D
Acq On : 10 Jun 2021 11:52
Operator : SY/MD
Sample : M2649-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG5P7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

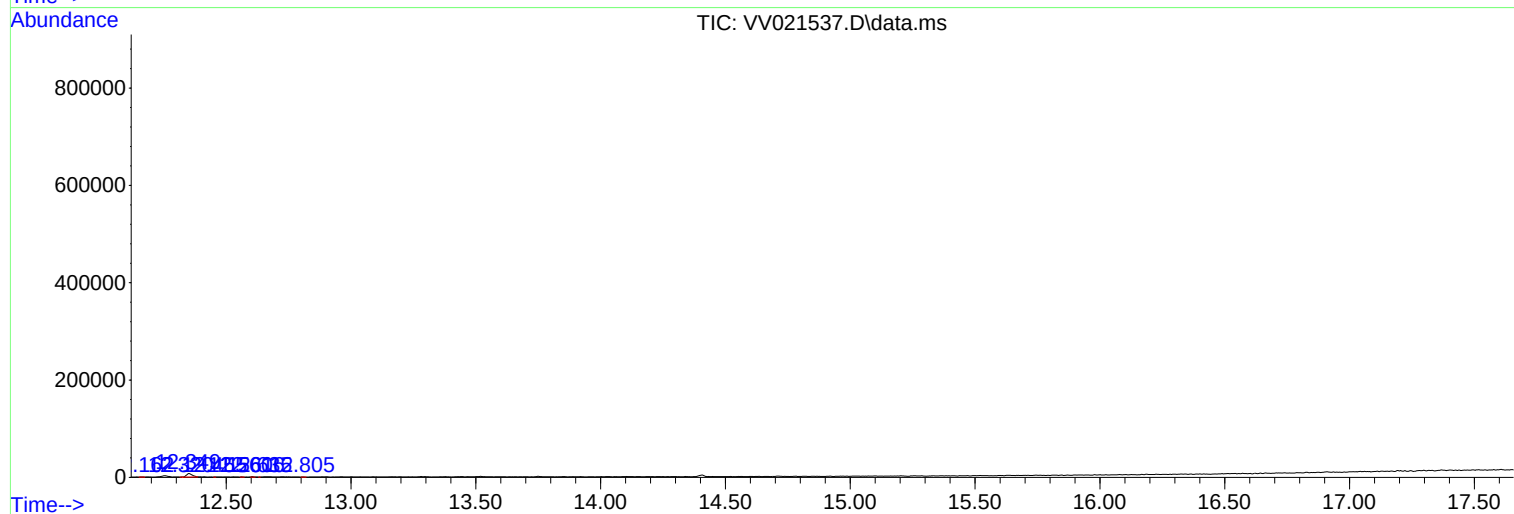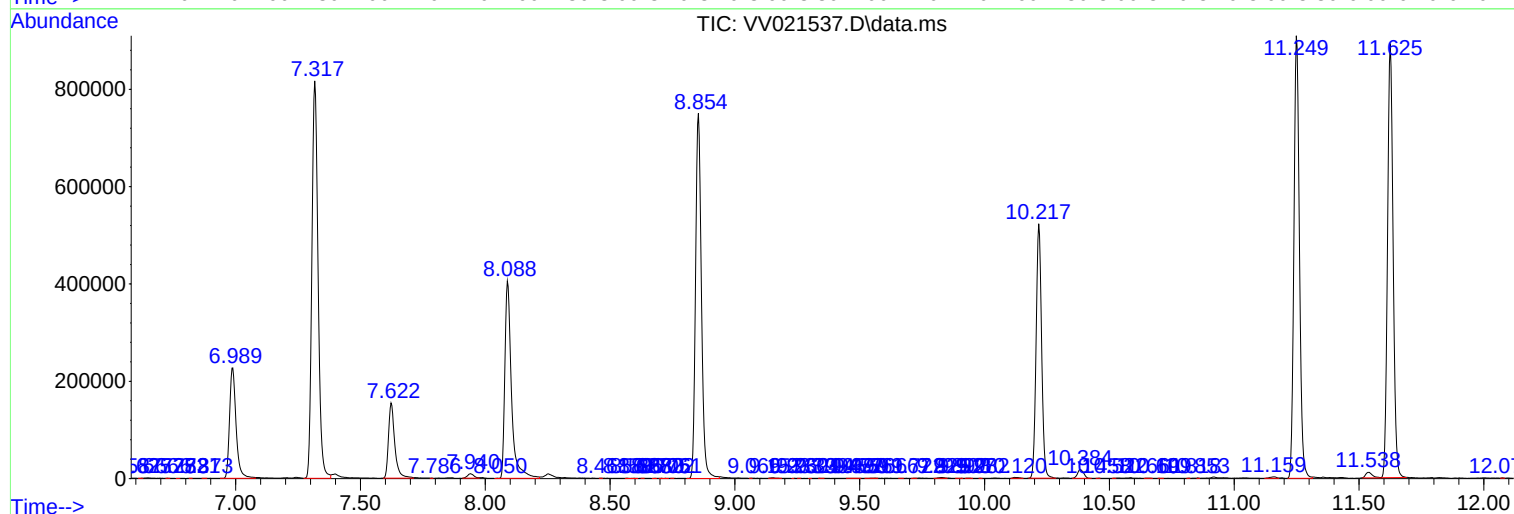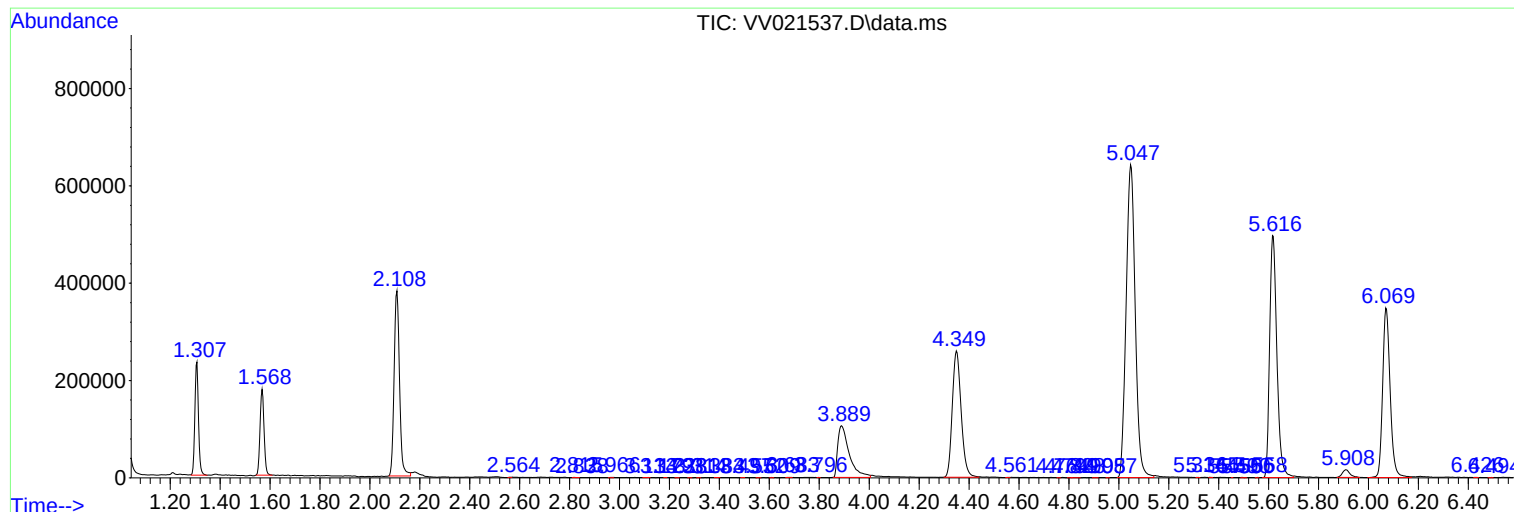

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061021\
Data File : VV021537.D
Acq On : 10 Jun 2021 11:52
Operator : SY/MD
Sample : M2649-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG5P7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061021\
Data File : VV021537.D
Acq On : 10 Jun 2021 11:52
Operator : SY/MD
Sample : M2649-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG5P7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
