

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061021\
 Data File : VV021539.D
 Acq On : 10 Jun 2021 12:40
 Operator : SY/MD
 Sample : M2649-14
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 B0AA9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M

Title : VOC Analysis

Signal : TIC: VV021539.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	96	rVB	229751	235627	14.35%	1.802%
2	1.565	157	163	177	rVB	157237	173075	10.54%	1.324%
3	2.108	322	332	348	rBV	384870	567947	34.59%	4.344%
4	2.555	469	471	475	rBV2	460	315	0.02%	0.002%
5	2.590	479	482	484	rBV2	411	304	0.02%	0.002%
6	2.626	491	493	496	rVB2	231	125	0.01%	0.001%
7	2.732	522	526	531	rVB4	598	500	0.03%	0.004%
8	2.764	531	536	537	rBV3	670	585	0.04%	0.004%
9	2.883	571	573	576	rBV	306	177	0.01%	0.001%
10	3.150	652	656	658	rVB2	377	264	0.02%	0.002%
11	3.230	678	681	682	rBV	253	130	0.01%	0.001%
12	3.298	700	702	705	rBV2	266	155	0.01%	0.001%
13	3.368	721	724	726	rBV	279	185	0.01%	0.001%
14	3.474	755	757	759	rVB	366	183	0.01%	0.001%
15	3.519	768	771	772	rVV	240	144	0.01%	0.001%
16	3.558	781	783	787	rVB3	407	230	0.01%	0.002%
17	3.632	804	806	809	rBV2	365	215	0.01%	0.002%
18	3.677	814	820	825	rVB2	228	317	0.02%	0.002%
19	3.716	829	832	839	rVB2	143	143	0.01%	0.001%
20	3.751	839	843	850	rBV3	522	687	0.04%	0.005%
21	3.786	850	854	860	rVB4	477	467	0.03%	0.004%
22	3.812	860	862	866	rVB2	434	280	0.02%	0.002%
23	3.883	874	884	921	rBV	127972	353571	21.53%	2.704%
24	4.349	1013	1029	1062	rBV	261887	646577	39.38%	4.945%
25	4.661	1121	1126	1130	rBV4	419	442	0.03%	0.003%
26	4.773	1157	1161	1163	rBV2	165	146	0.01%	0.001%
27	4.854	1184	1186	1188	rVB2	287	129	0.01%	0.001%
28	4.870	1188	1191	1193	rBV2	384	193	0.01%	0.001%
29	4.953	1213	1217	1220	rVB3	324	235	0.01%	0.002%
30	5.047	1229	1246	1279	rBV2	640212	1642038	100.00%	12.559%
31	5.375	1345	1348	1351	rBV3	486	249	0.02%	0.002%
32	5.481	1377	1381	1382	rBV	578	333	0.02%	0.003%
33	5.535	1396	1398	1402	rVB4	489	249	0.02%	0.002%
34	5.564	1402	1407	1408	rBV3	348	286	0.02%	0.002%
35	5.619	1411	1424	1456	rBV	490027	994452	60.56%	7.606%
36	5.912	1505	1515	1534	rVB3	7326	16359	1.00%	0.125%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061021\
 Data File : VV021539.D
 Acq On : 10 Jun 2021 12:40
 Operator : SY/MD
 Sample : M2649-14
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 B0AA9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
 Title : VOC Analysis

37	6.072	1550	1565	1594	rBV	350613	723600	44.07%	5.534%
38	6.307	1635	1638	1641	rVB3	637	388	0.02%	0.003%
39	6.326	1641	1644	1646	rBV2	405	244	0.01%	0.002%
40	6.407	1667	1669	1671	rBV	216	127	0.01%	0.001%
41	6.449	1680	1682	1685	rVB3	333	184	0.01%	0.001%
42	6.490	1691	1695	1697	rBV2	277	205	0.01%	0.002%
43	6.510	1700	1701	1705	rVB	339	134	0.01%	0.001%
44	6.529	1705	1707	1710	rBV	452	291	0.02%	0.002%
45	6.577	1720	1722	1726	rBV	383	254	0.02%	0.002%
46	6.606	1728	1731	1735	rVB3	370	322	0.02%	0.002%
47	6.632	1735	1739	1741	rBV2	904	595	0.04%	0.005%
48	6.767	1776	1781	1783	rBV3	540	358	0.02%	0.003%
49	6.783	1785	1786	1790	rVV	299	126	0.01%	0.001%
50	6.892	1816	1820	1821	rBV	260	151	0.01%	0.001%
51	6.921	1826	1829	1834	rVB2	273	223	0.01%	0.002%
52	6.989	1838	1850	1876	rBV	221653	407034	24.79%	3.113%
53	7.227	1922	1924	1927	rBV2	526	309	0.02%	0.002%
54	7.317	1940	1952	1974	rBV	806938	1404728	85.55%	10.744%
55	7.622	2037	2047	2070	rBV	154106	271743	16.55%	2.078%
56	7.867	2118	2123	2126	rBV2	822	701	0.04%	0.005%
57	7.982	2155	2159	2169	rVB4	1614	2239	0.14%	0.017%
58	8.034	2172	2175	2177	rVB2	401	208	0.01%	0.002%
59	8.088	2182	2192	2232	rBV	457458	816241	49.71%	6.243%
60	8.638	2361	2363	2367	rBV3	409	291	0.02%	0.002%
61	8.854	2413	2430	2451	rBV	722849	1186234	72.24%	9.073%
62	9.137	2513	2518	2519	rBV2	781	454	0.03%	0.003%
63	9.233	2547	2548	2551	rVB	300	125	0.01%	0.001%
64	9.304	2564	2570	2571	rBV	157	172	0.01%	0.001%
65	9.330	2576	2578	2582	rVB2	490	273	0.02%	0.002%
66	9.375	2588	2592	2595	rBV4	378	273	0.02%	0.002%
67	9.506	2630	2633	2635	rBV2	396	251	0.02%	0.002%
68	9.632	2669	2672	2675	rVB	273	173	0.01%	0.001%
69	9.722	2697	2700	2704	rBV2	354	236	0.01%	0.002%
70	9.754	2704	2710	2713	rVV3	310	283	0.02%	0.002%
71	9.773	2713	2716	2717	rVB	281	141	0.01%	0.001%
72	9.802	2721	2725	2727	rBV2	234	188	0.01%	0.001%
73	9.828	2731	2733	2738	rVV2	298	249	0.02%	0.002%
74	9.850	2738	2740	2743	rVB2	332	159	0.01%	0.001%
75	10.127	2818	2826	2834	rVB5	1897	2974	0.18%	0.023%
76	10.165	2834	2838	2842	rBV	143	164	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061021\
 Data File : VV021539.D
 Acq On : 10 Jun 2021 12:40
 Operator : SY/MD
 Sample : M2649-14
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 B0AA9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
 Title : VOC Analysis

77	10.217	2842	2854	2876	rBV	545718	845072	51.46%	6.463%
78	10.362	2895	2899	2900	rBV	622	373	0.02%	0.003%
79	10.436	2919	2922	2924	rBV2	256	190	0.01%	0.001%
80	10.542	2951	2955	2960	rBV3	624	713	0.04%	0.005%
81	10.657	2989	2991	2998	rVB4	436	403	0.02%	0.003%
82	10.837	3044	3047	3050	rBV3	329	284	0.02%	0.002%
83	10.915	3065	3071	3073	rBV4	2225	2157	0.13%	0.016%
84	11.149	3136	3144	3151	rVB4	1497	2549	0.16%	0.019%
85	11.188	3151	3156	3160	rBV2	602	571	0.03%	0.004%
86	11.249	3163	3175	3194	rBV	854637	1334228	81.25%	10.205%
87	11.545	3258	3267	3275	rBV8	2115	4539	0.28%	0.035%
88	11.625	3280	3292	3319	rVV	847032	1363288	83.02%	10.427%
89	11.937	3387	3389	3393	rVB3	437	225	0.01%	0.002%
90	11.956	3393	3395	3402	rVB3	341	216	0.01%	0.002%
91	11.992	3403	3406	3407	rBV2	301	193	0.01%	0.001%
92	12.040	3419	3421	3425	rVB3	453	296	0.02%	0.002%
93	12.066	3425	3429	3431	rBV3	613	449	0.03%	0.003%
94	12.181	3463	3465	3469	rBV4	440	330	0.02%	0.003%
95	12.313	3504	3506	3510	rBV	266	204	0.01%	0.002%
96	12.551	3578	3580	3582	rBV2	295	150	0.01%	0.001%
97	12.921	3688	3695	3705	rVB3	18995	27925	1.70%	0.214%
98	12.989	3708	3716	3726	rVB6	11630	17926	1.09%	0.137%
99	13.075	3736	3743	3751	rVB9	7931	11728	0.71%	0.090%
100	13.722	3942	3944	3945	rBV	882	376	0.02%	0.003%




Sum of corrected areas: 13074744

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061021\
Data File : VV021539.D
Acq On : 10 Jun 2021 12:40
Operator : SY/MD
Sample : M2649-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
B0AA9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

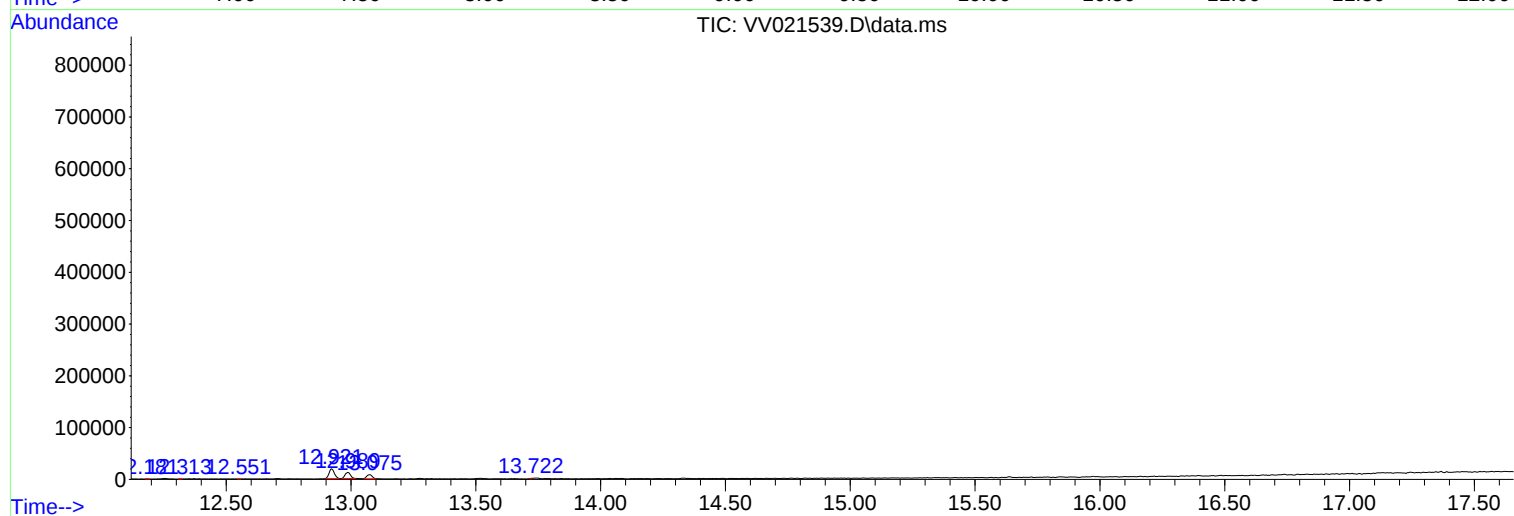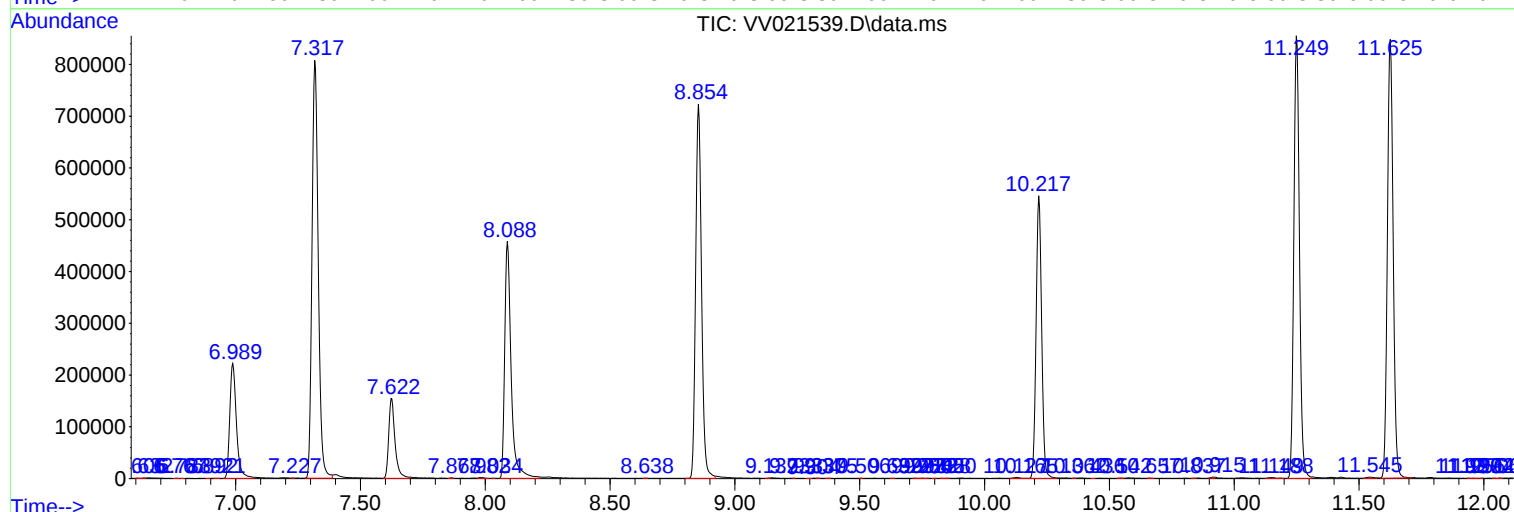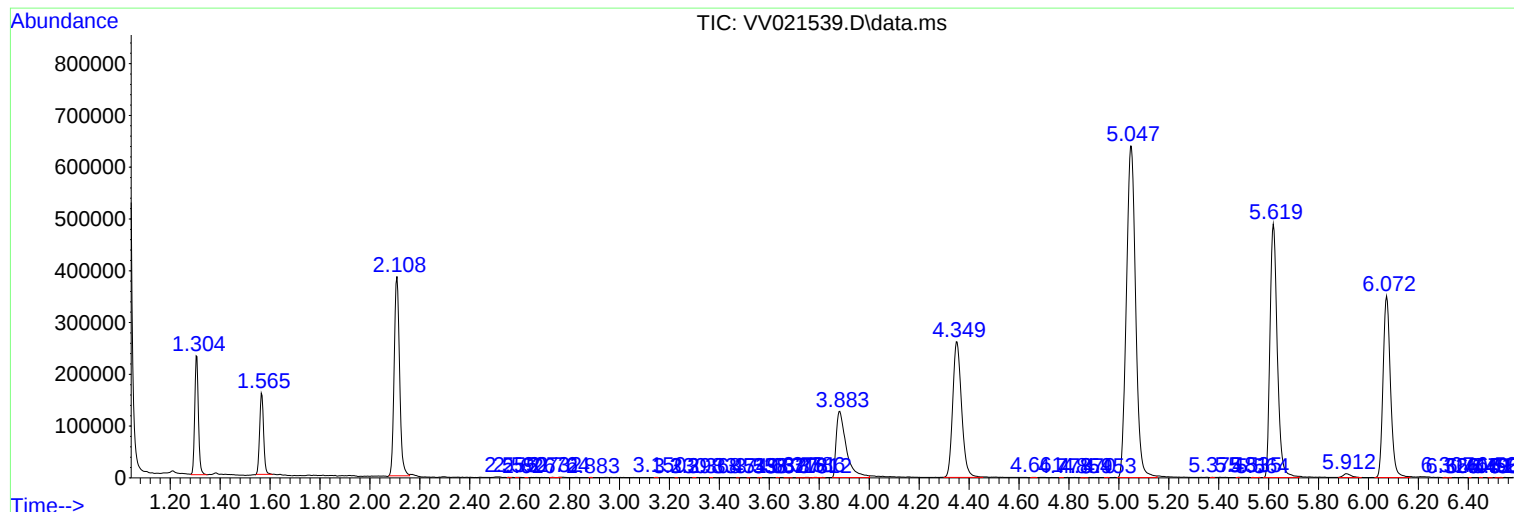

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061021\
Data File : VV021539.D
Acq On : 10 Jun 2021 12:40
Operator : SY/MD
Sample : M2649-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
B0AA9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061021\
Data File : VV021539.D
Acq On : 10 Jun 2021 12:40
Operator : SY/MD
Sample : M2649-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
B0AA9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------