

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061021\
 Data File : VV021540.D
 Acq On : 10 Jun 2021 13:03
 Operator : SY/MD
 Sample : M2662-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGDM1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M

Title : VOC Analysis

Signal : TIC: VV021540.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	95	rVB	261356	263735	14.35%	1.843%
2	1.568	156	164	180	rBV	201564	222990	12.13%	1.558%
3	2.108	322	332	349	rBV	431324	635670	34.58%	4.442%
4	2.728	523	525	527	rBV2	352	188	0.01%	0.001%
5	2.757	529	534	535	rBV2	307	187	0.01%	0.001%
6	2.802	545	548	550	rBV2	373	243	0.01%	0.002%
7	2.915	581	583	586	rBV2	276	150	0.01%	0.001%
8	3.027	616	618	621	rVV3	403	241	0.01%	0.002%
9	3.044	621	623	628	rVB3	383	249	0.01%	0.002%
10	3.156	654	658	660	rBV2	176	149	0.01%	0.001%
11	3.256	686	689	694	rVB3	325	228	0.01%	0.002%
12	3.281	694	697	701	rBV2	180	160	0.01%	0.001%
13	3.391	728	731	733	rBV	183	120	0.01%	0.001%
14	3.442	743	747	750	rBV2	179	167	0.01%	0.001%
15	3.490	755	762	766	rBV2	382	535	0.03%	0.004%
16	3.545	775	779	782	rBV2	234	200	0.01%	0.001%
17	3.597	791	795	797	rVB2	301	141	0.01%	0.001%
18	3.609	797	799	804	rBV3	382	263	0.01%	0.002%
19	3.667	813	817	819	rBV2	214	133	0.01%	0.001%
20	3.716	829	832	834	rBV2	177	139	0.01%	0.001%
21	3.773	846	850	855	rVB3	314	288	0.02%	0.002%
22	3.796	855	857	860	rBV	236	174	0.01%	0.001%
23	3.847	869	873	875	rBV2	239	144	0.01%	0.001%
24	3.889	875	886	931	rBV	127180	390234	21.23%	2.727%
25	4.352	1014	1030	1063	rBV	290418	718257	39.07%	5.019%
26	4.670	1126	1129	1134	rBV3	341	326	0.02%	0.002%
27	4.715	1141	1143	1145	rBV	359	161	0.01%	0.001%
28	4.818	1172	1175	1177	rBV	375	212	0.01%	0.001%
29	4.886	1190	1196	1202	rBV3	428	524	0.03%	0.004%
30	4.915	1202	1205	1208	rBV2	228	170	0.01%	0.001%
31	5.050	1229	1247	1280	rBV2	721472	1838194	100.00%	12.846%
32	5.481	1379	1381	1382	rBV	271	127	0.01%	0.001%
33	5.558	1400	1405	1406	rBV2	249	170	0.01%	0.001%
34	5.619	1411	1424	1454	rBV	506796	1015379	55.24%	7.096%
35	5.912	1503	1515	1532	rBV3	18081	38040	2.07%	0.266%
36	5.998	1540	1542	1549	rBV3	369	321	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061021\
 Data File : VV021540.D
 Acq On : 10 Jun 2021 13:03
 Operator : SY/MD
 Sample : M2662-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGDM1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
 Title : VOC Analysis

37	6.072	1551	1565	1597	rBV	394221	805503	43.82%	5.629%
38	6.317	1639	1641	1644	rVB2	338	157	0.01%	0.001%
39	6.336	1644	1647	1651	rBV3	539	436	0.02%	0.003%
40	6.362	1651	1655	1657	rBV2	514	356	0.02%	0.002%
41	6.445	1678	1681	1685	rBV2	262	193	0.01%	0.001%
42	6.487	1691	1694	1696	rBV2	184	124	0.01%	0.001%
43	6.526	1701	1706	1709	rBV2	477	395	0.02%	0.003%
44	6.641	1736	1742	1752	rBV4	1310	2253	0.12%	0.016%
45	6.703	1758	1761	1767	rVB2	613	582	0.03%	0.004%
46	6.744	1767	1774	1777	rBV2	409	517	0.03%	0.004%
47	6.776	1782	1784	1786	rVB	349	118	0.01%	0.001%
48	6.789	1786	1788	1790	rBV2	279	163	0.01%	0.001%
49	6.812	1792	1795	1798	rVB3	575	320	0.02%	0.002%
50	6.989	1837	1850	1872	rBV	250616	455517	24.78%	3.183%
51	7.317	1939	1952	1972	rBV	909480	1583848	86.16%	11.068%
52	7.622	2037	2047	2069	rBV	173559	301205	16.39%	2.105%
53	7.812	2103	2106	2111	rVB3	716	591	0.03%	0.004%
54	7.838	2111	2114	2116	rBV	418	296	0.02%	0.002%
55	7.873	2124	2125	2127	rVB	558	157	0.01%	0.001%
56	7.940	2134	2146	2156	rBV3	10758	19513	1.06%	0.136%
57	8.088	2182	2192	2234	rBV	472698	864426	47.03%	6.041%
58	8.458	2304	2307	2311	rBV4	323	302	0.02%	0.002%
59	8.625	2354	2359	2362	rBV2	518	451	0.02%	0.003%
60	8.802	2409	2414	2417	rBV2	230	254	0.01%	0.002%
61	8.854	2418	2430	2463	rBV	750804	1222639	66.51%	8.544%
62	9.088	2498	2503	2504	rBV3	554	453	0.02%	0.003%
63	9.136	2516	2518	2519	rBV3	646	249	0.01%	0.002%
64	9.191	2533	2535	2539	rVB2	399	278	0.02%	0.002%
65	9.223	2541	2545	2548	rVB2	296	236	0.01%	0.002%
66	9.246	2548	2552	2556	rBV3	251	238	0.01%	0.002%
67	9.346	2579	2583	2584	rBV	254	130	0.01%	0.001%
68	9.394	2595	2598	2602	rBV	214	146	0.01%	0.001%
69	9.413	2602	2604	2606	rBV	299	140	0.01%	0.001%
70	9.548	2642	2646	2649	rBV	470	449	0.02%	0.003%
71	9.587	2655	2658	2662	rVB4	425	321	0.02%	0.002%
72	9.664	2678	2682	2684	rVB2	264	153	0.01%	0.001%
73	9.744	2704	2707	2708	rBV	327	185	0.01%	0.001%
74	9.802	2721	2725	2727	rBV	258	164	0.01%	0.001%
75	9.828	2727	2733	2737	rBV5	1019	1176	0.06%	0.008%
76	9.976	2778	2779	2784	rVB2	321	217	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061021\
 Data File : VV021540.D
 Acq On : 10 Jun 2021 13:03
 Operator : SY/MD
 Sample : M2662-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGDM1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M

Title : VOC Analysis

77	10.127	2818	2826	2836	rBV5	2139	3358	0.18%	0.023%
78	10.217	2840	2854	2874	rBV	586917	903760	49.17%	6.316%
79	10.384	2896	2906	2919	rVB	20356	33783	1.84%	0.236%
80	10.435	2919	2922	2925	rBV2	216	182	0.01%	0.001%
81	10.448	2925	2926	2930	rVB	338	165	0.01%	0.001%
82	10.526	2946	2950	2953	rBV3	595	491	0.03%	0.003%
83	10.857	3050	3053	3057	rBV4	502	458	0.02%	0.003%
84	10.889	3057	3063	3064	rBV3	251	214	0.01%	0.001%
85	11.040	3107	3110	3113	rVB2	564	301	0.02%	0.002%
86	11.088	3123	3125	3127	rVB	372	163	0.01%	0.001%
87	11.153	3137	3145	3147	rBV4	2385	2819	0.15%	0.020%
88	11.249	3164	3175	3196	rBV	905257	1389199	75.57%	9.708%
89	11.542	3255	3266	3280	rBV3	8573	17478	0.95%	0.122%
90	11.625	3280	3292	3315	rVV	985427	1550980	84.38%	10.839%
91	11.853	3358	3363	3369	rVB4	632	841	0.05%	0.006%
92	11.905	3377	3379	3381	rVB	349	132	0.01%	0.001%
93	11.992	3404	3406	3407	rBV	381	137	0.01%	0.001%
94	12.037	3415	3420	3425	rBV3	574	631	0.03%	0.004%
95	12.091	3435	3437	3441	rBV2	557	393	0.02%	0.003%
96	12.320	3506	3508	3510	rBV2	406	220	0.01%	0.002%
97	12.352	3511	3518	3529	rVB6	6156	9953	0.54%	0.070%
98	12.651	3609	3611	3612	rBV	339	130	0.01%	0.001%
99	12.712	3627	3630	3633	rVB3	282	173	0.01%	0.001%
100	12.876	3679	3681	3683	rBV2	295	141	0.01%	0.001%




Sum of corrected areas: 14309562

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061021\
Data File : VV021540.D
Acq On : 10 Jun 2021 13:03
Operator : SY/MD
Sample : M2662-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGDM1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

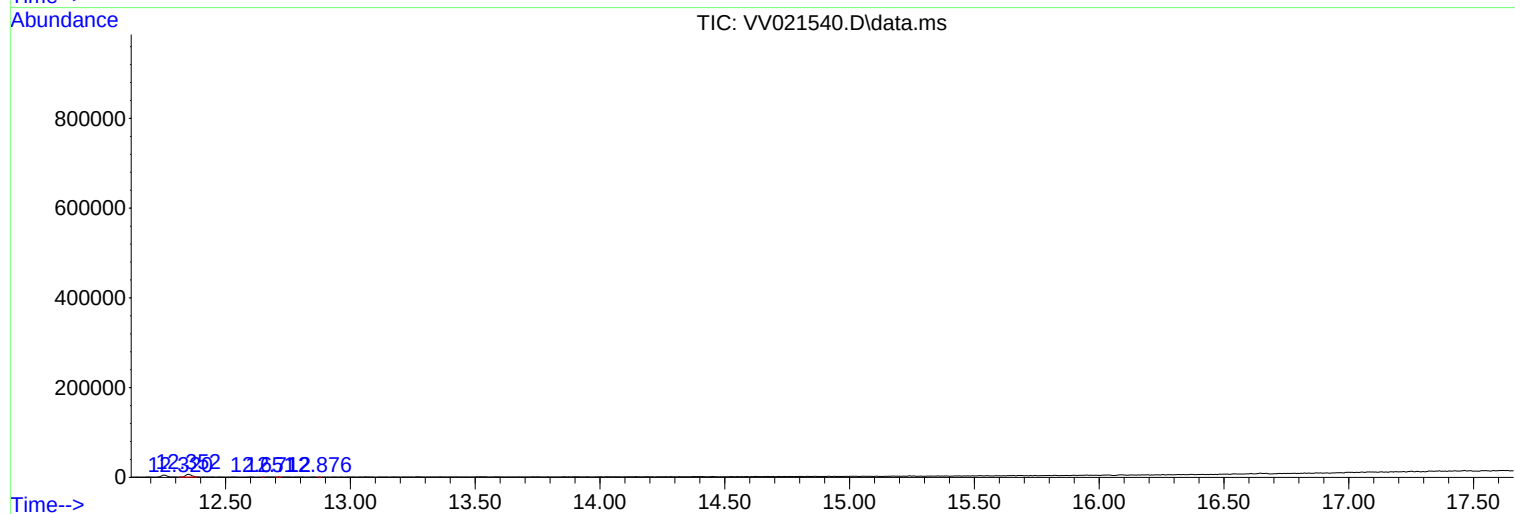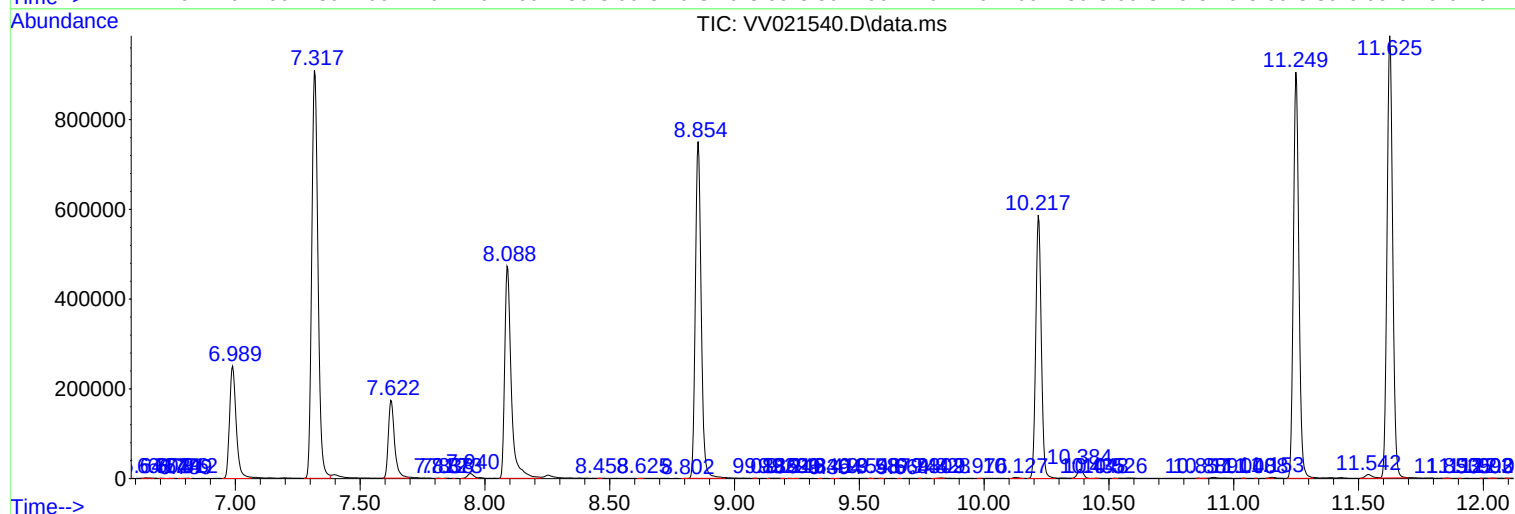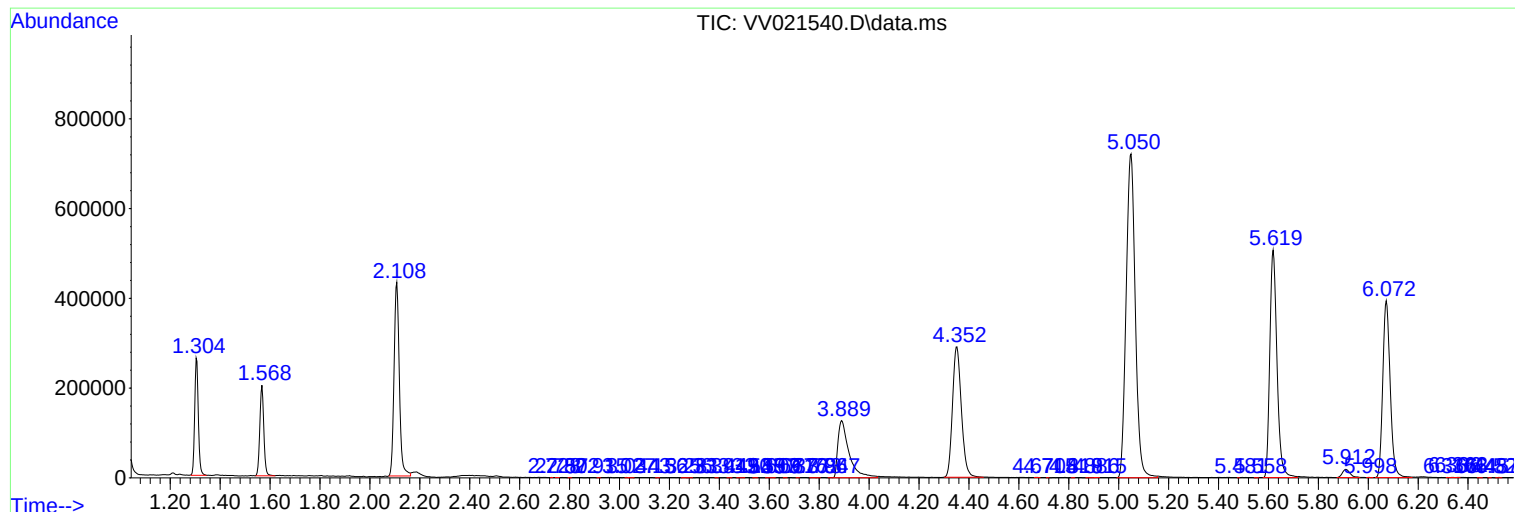

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061021\
Data File : VV021540.D
Acq On : 10 Jun 2021 13:03
Operator : SY/MD
Sample : M2662-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGDM1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061021\
Data File : VV021540.D
Acq On : 10 Jun 2021 13:03
Operator : SY/MD
Sample : M2662-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGDM1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
