

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061021\
 Data File : VV021541.D
 Acq On : 10 Jun 2021 13:34
 Operator : SY/MD
 Sample : M2662-15
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M

Title : VOC Analysis

Signal : TIC: VV021541.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	96	rVB	238099	243443	14.61%	1.842%
2	1.568	157	164	178	rVB	181194	205412	12.33%	1.554%
3	2.108	322	332	359	rVB	392125	593048	35.59%	4.486%
4	2.507	448	456	469	rVB6	4048	7314	0.44%	0.055%
5	2.709	516	519	523	rBV	301	226	0.01%	0.002%
6	2.838	556	559	561	rBV	272	155	0.01%	0.001%
7	2.886	571	574	575	rBV	207	82	0.00%	0.001%
8	2.979	601	603	611	rVB2	440	360	0.02%	0.003%
9	3.053	623	626	627	rBV	152	86	0.01%	0.001%
10	3.150	653	656	657	rBV	193	131	0.01%	0.001%
11	3.301	701	703	704	rBV	167	56	0.00%	0.000%
12	3.465	748	754	758	rBV2	322	401	0.02%	0.003%
13	3.481	758	759	762	rVV2	354	213	0.01%	0.002%
14	3.510	766	768	771	rVB2	227	121	0.01%	0.001%
15	3.597	793	795	800	rVV	359	167	0.01%	0.001%
16	3.616	800	801	804	rVB	162	53	0.00%	0.000%
17	3.699	825	827	828	rBV	155	69	0.00%	0.001%
18	3.831	865	868	869	rBV	215	142	0.01%	0.001%
19	3.886	874	885	924	rBV	109754	343115	20.59%	2.596%
20	4.346	1013	1028	1057	rBV	264935	651349	39.09%	4.927%
21	4.719	1143	1144	1148	rBV	325	105	0.01%	0.001%
22	4.760	1154	1157	1162	rVB2	377	309	0.02%	0.002%
23	4.786	1162	1165	1168	rBV2	343	280	0.02%	0.002%
24	4.818	1172	1175	1179	rVV2	359	224	0.01%	0.002%
25	4.841	1179	1182	1185	rVB3	336	257	0.02%	0.002%
26	4.857	1185	1187	1193	rVB2	257	202	0.01%	0.002%
27	4.883	1193	1195	1198	rBV	191	136	0.01%	0.001%
28	5.047	1229	1246	1282	rBV2	649593	1666267	100.00%	12.605%
29	5.558	1404	1405	1407	rBV2	201	70	0.00%	0.001%
30	5.616	1410	1423	1450	rBV	505984	1009680	60.60%	7.638%
31	5.905	1504	1513	1532	rVB5	10578	22724	1.36%	0.172%
32	6.069	1550	1564	1587	rBV	358453	724325	43.47%	5.479%
33	6.275	1626	1628	1630	rBV2	349	168	0.01%	0.001%
34	6.307	1636	1638	1640	rBV	192	114	0.01%	0.001%
35	6.391	1661	1664	1667	rBV	222	168	0.01%	0.001%
36	6.429	1674	1676	1680	rBV3	413	261	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061021\
 Data File : VV021541.D
 Acq On : 10 Jun 2021 13:34
 Operator : SY/MD
 Sample : M2662-15
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
 Title : VOC Analysis

37	6.535	1705	1709	1711	rBV2	346	282	0.02%	0.002%
38	6.574	1718	1721	1727	rVB	449	366	0.02%	0.003%
39	6.613	1729	1733	1734	rBV	365	172	0.01%	0.001%
40	6.641	1734	1742	1745	rBV3	912	1098	0.07%	0.008%
41	6.760	1777	1779	1781	rBV	200	71	0.00%	0.001%
42	6.834	1800	1802	1804	rBV	260	113	0.01%	0.001%
43	6.847	1804	1806	1809	rVV2	153	74	0.00%	0.001%
44	6.863	1809	1811	1812	rVB2	188	53	0.00%	0.000%
45	6.985	1838	1849	1882	rBV	227300	414285	24.86%	3.134%
46	7.268	1935	1937	1940	rBV2	429	324	0.02%	0.002%
47	7.317	1940	1952	1973	rBV	816189	1441038	86.48%	10.901%
48	7.622	2036	2047	2076	rBV	158144	275651	16.54%	2.085%
49	8.011	2166	2168	2171	rVB2	516	219	0.01%	0.002%
50	8.027	2171	2173	2175	rBV	203	86	0.01%	0.001%
51	8.040	2175	2177	2181	rVB3	382	180	0.01%	0.001%
52	8.088	2182	2192	2225	rBV	413291	765742	45.96%	5.793%
53	8.587	2344	2347	2350	rBV	219	159	0.01%	0.001%
54	8.641	2361	2364	2365	rBV2	236	96	0.01%	0.001%
55	8.651	2365	2367	2369	rVB	232	94	0.01%	0.001%
56	8.664	2369	2371	2375	rBV3	191	140	0.01%	0.001%
57	8.693	2378	2380	2381	rBV	137	31	0.00%	0.000%
58	8.792	2409	2411	2412	rBV	321	127	0.01%	0.001%
59	8.854	2417	2430	2453	rBV	734042	1210342	72.64%	9.156%
60	9.066	2494	2496	2504	rVB3	706	665	0.04%	0.005%
61	9.294	2563	2567	2568	rBV2	265	163	0.01%	0.001%
62	9.323	2574	2576	2577	rBV2	259	125	0.01%	0.001%
63	9.352	2583	2585	2588	rVB2	324	132	0.01%	0.001%
64	9.368	2588	2590	2594	rVB2	164	67	0.00%	0.001%
65	9.391	2594	2597	2600	rBV	264	153	0.01%	0.001%
66	9.609	2662	2665	2669	rVB2	280	147	0.01%	0.001%
67	9.821	2729	2731	2735	rBV	217	111	0.01%	0.001%
68	9.895	2752	2754	2756	rBV	225	134	0.01%	0.001%
69	10.043	2798	2800	2802	rVB	321	98	0.01%	0.001%
70	10.056	2802	2804	2808	rBV	226	144	0.01%	0.001%
71	10.127	2818	2826	2833	rVB2	1857	2763	0.17%	0.021%
72	10.217	2842	2854	2875	rBV	522596	827835	49.68%	6.262%
73	10.725	3010	3012	3014	rBV	208	78	0.00%	0.001%
74	10.873	3056	3058	3059	rBV	196	65	0.00%	0.000%
75	10.918	3065	3072	3082	rBV5	2088	3374	0.20%	0.026%
76	11.143	3136	3142	3152	rBV5	1185	1788	0.11%	0.014%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061021\
Data File : VV021541.D
Acq On : 10 Jun 2021 13:34
Operator : SY/MD
Sample : M2662-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK002

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
Title : VOC Analysis

77	11.249	3163	3175	3195	rBV	898806	1396498	83.81%	10.564%
78	11.513	3254	3257	3260	rBV2	389	222	0.01%	0.002%
79	11.625	3280	3292	3314	rBV	877271	1402340	84.16%	10.608%
80	11.927	3385	3386	3392	rBV3	368	224	0.01%	0.002%
81	11.995	3405	3407	3408	rBV3	379	151	0.01%	0.001%
82	12.056	3423	3426	3428	rBV	325	191	0.01%	0.001%




Sum of corrected areas: 13219444

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061021\
Data File : VV021541.D
Acq On : 10 Jun 2021 13:34
Operator : SY/MD
Sample : M2662-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

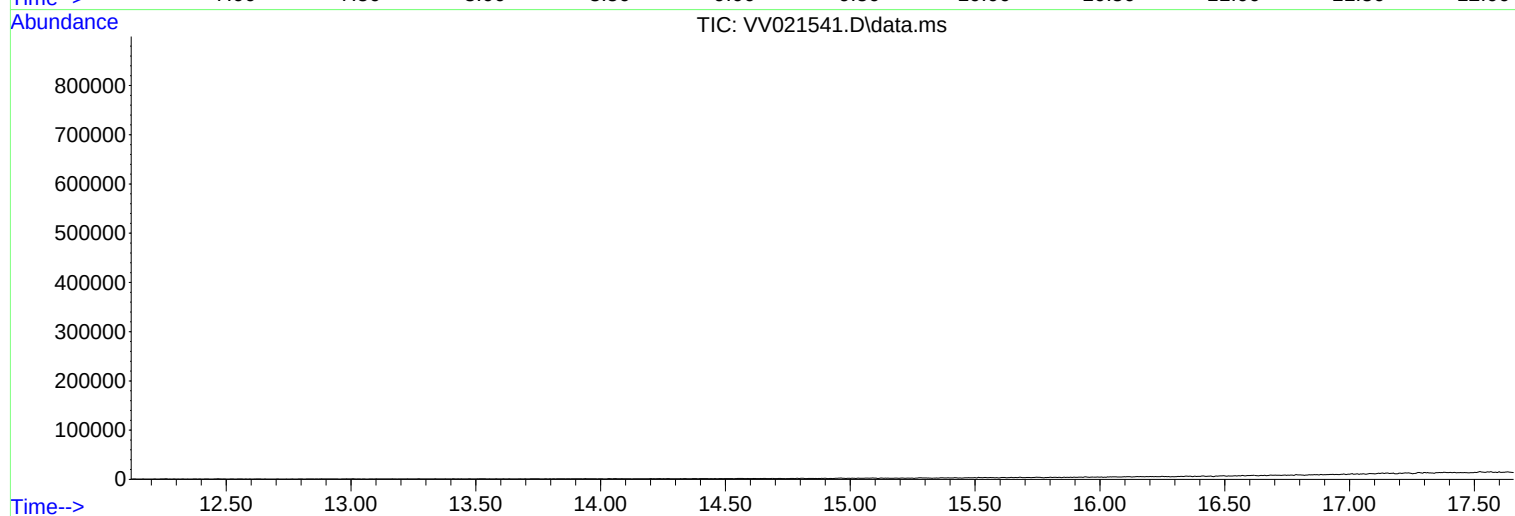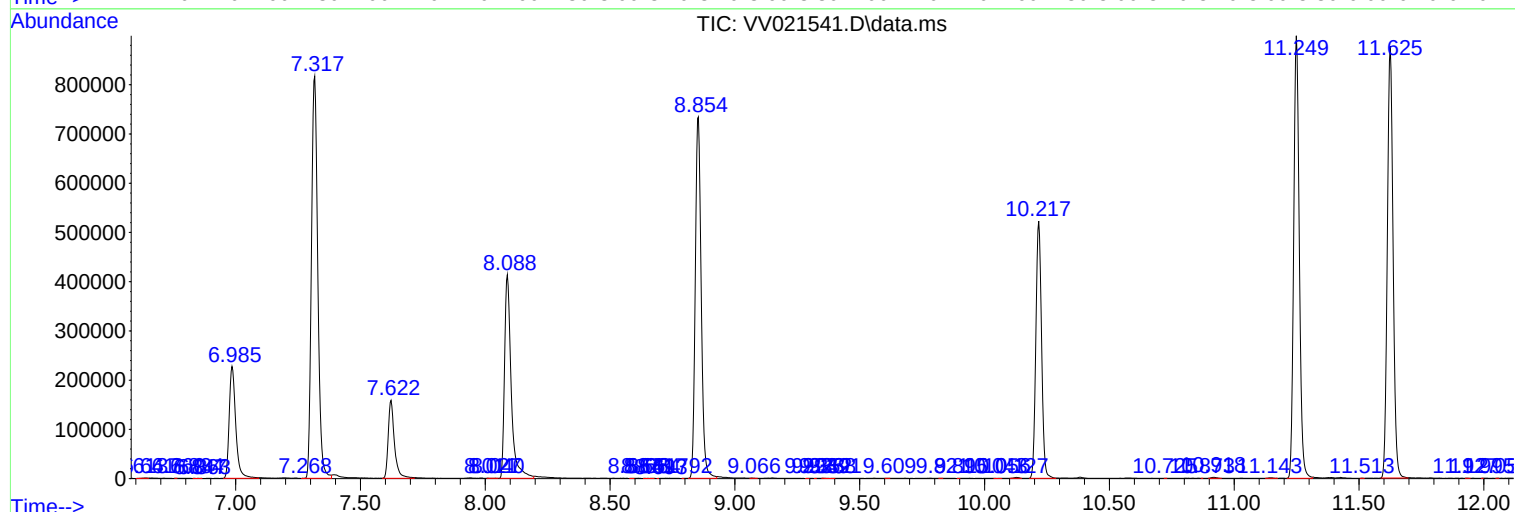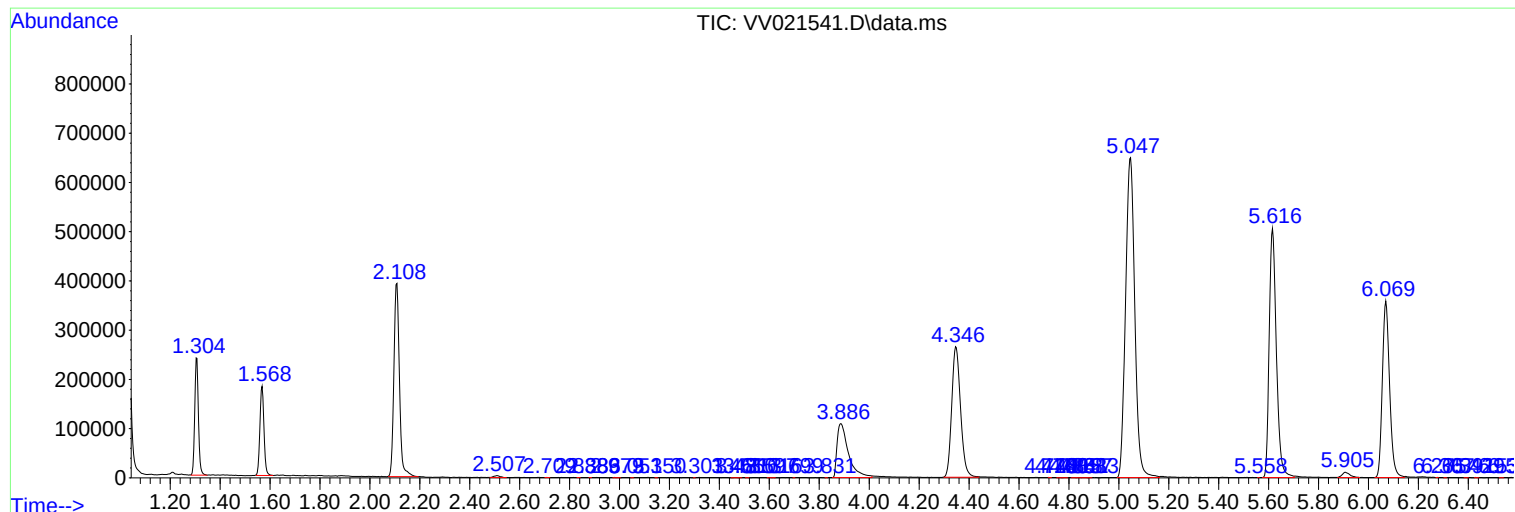

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061021\
Data File : VV021541.D
Acq On : 10 Jun 2021 13:34
Operator : SY/MD
Sample : M2662-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061021\
Data File : VV021541.D
Acq On : 10 Jun 2021 13:34
Operator : SY/MD
Sample : M2662-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
