

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061021\
 Data File : VV021542.D
 Acq On : 10 Jun 2021 13:58
 Operator : SY/MD
 Sample : M2649-16
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M

Title : VOC Analysis

Signal : TIC: VV021542.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	95	rVB	225896	229093	14.28%	1.778%
2	1.568	157	164	177	rVB	173680	197016	12.28%	1.529%
3	2.108	322	332	366	rVB	377766	571636	35.63%	4.437%
4	2.384	414	418	421	rBV4	484	368	0.02%	0.003%
5	2.590	477	482	485	rVB2	468	403	0.03%	0.003%
6	2.609	485	488	492	rBV2	604	485	0.03%	0.004%
7	2.651	495	501	502	rBV2	266	299	0.02%	0.002%
8	2.722	518	523	526	rBV3	618	541	0.03%	0.004%
9	2.815	549	552	556	rBV2	284	266	0.02%	0.002%
10	2.847	559	562	565	rVV	238	181	0.01%	0.001%
11	2.924	584	586	590	rVB3	354	182	0.01%	0.001%
12	2.947	590	593	596	rBV2	313	247	0.02%	0.002%
13	3.047	622	624	632	rVB2	440	447	0.03%	0.003%
14	3.079	632	634	637	rVB	321	161	0.01%	0.001%
15	3.108	637	643	648	rBV2	273	354	0.02%	0.003%
16	3.127	648	649	652	rBV	209	137	0.01%	0.001%
17	3.413	732	738	740	rBV2	539	394	0.02%	0.003%
18	3.445	745	748	752	rBV	315	302	0.02%	0.002%
19	3.522	769	772	777	rVB3	309	275	0.02%	0.002%
20	3.625	801	804	806	rBV2	242	114	0.01%	0.001%
21	3.670	814	818	820	rBV2	273	134	0.01%	0.001%
22	3.686	820	823	826	rVB2	212	151	0.01%	0.001%
23	3.709	826	830	832	rBV2	247	154	0.01%	0.001%
24	3.725	832	835	836	rBV2	282	125	0.01%	0.001%
25	3.892	876	887	929	rBV	113730	364468	22.71%	2.829%
26	4.352	1015	1030	1056	rBV	256116	624632	38.93%	4.849%
27	4.657	1121	1125	1126	rBV2	360	264	0.02%	0.002%
28	4.699	1135	1138	1140	rBV	304	203	0.01%	0.002%
29	4.715	1141	1143	1145	rVB2	433	175	0.01%	0.001%
30	4.735	1145	1149	1152	rVB	435	258	0.02%	0.002%
31	4.751	1152	1154	1158	rVB3	244	175	0.01%	0.001%
32	4.831	1176	1179	1182	rBV2	236	155	0.01%	0.001%
33	4.963	1217	1220	1223	rBV2	180	147	0.01%	0.001%
34	4.982	1223	1226	1230	rBV	267	217	0.01%	0.002%
35	5.050	1230	1247	1276	rBV2	631599	1604530	100.00%	12.455%
36	5.394	1349	1354	1357	rBV2	283	342	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW061021\
 Data File : VW021542.D
 Acq On : 10 Jun 2021 13:58
 Operator : SY/MD
 Sample : M2649-16
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
 Title : VOC Analysis

37	5.481	1379	1381	1385	rBV4	245	217	0.01%	0.002%
38	5.619	1412	1424	1450	rBV	483926	966468	60.23%	7.502%
39	5.915	1504	1516	1537	rVB3	9919	22756	1.42%	0.177%
40	6.014	1545	1547	1551	rVB3	425	270	0.02%	0.002%
41	6.072	1551	1565	1595	rBV	343564	702172	43.76%	5.451%
42	6.294	1631	1634	1637	rVB2	515	318	0.02%	0.002%
43	6.336	1645	1647	1649	rVB3	369	141	0.01%	0.001%
44	6.439	1675	1679	1683	rBV3	416	303	0.02%	0.002%
45	6.542	1707	1711	1713	rBV2	279	214	0.01%	0.002%
46	6.609	1730	1732	1734	rBV2	275	126	0.01%	0.001%
47	6.635	1736	1740	1741	rBV2	443	310	0.02%	0.002%
48	6.773	1781	1783	1785	rVB2	289	124	0.01%	0.001%
49	6.786	1785	1787	1789	rBV	265	110	0.01%	0.001%
50	6.805	1789	1793	1796	rVV3	325	246	0.02%	0.002%
51	6.918	1826	1828	1830	rBV	263	167	0.01%	0.001%
52	6.989	1839	1850	1873	rBV	221133	400007	24.93%	3.105%
53	7.316	1940	1952	1972	rBV	793291	1384580	86.29%	10.748%
54	7.587	2034	2036	2037	rBV	546	202	0.01%	0.002%
55	7.625	2037	2048	2071	rVV	147036	263530	16.42%	2.046%
56	7.834	2110	2113	2117	rVB3	530	367	0.02%	0.003%
57	7.879	2124	2127	2129	rVB3	338	132	0.01%	0.001%
58	7.892	2130	2131	2133	rBV2	209	113	0.01%	0.001%
59	7.918	2137	2139	2142	rVB2	513	223	0.01%	0.002%
60	7.947	2142	2148	2153	rBV2	682	1037	0.06%	0.008%
61	7.982	2157	2159	2161	rBV2	665	236	0.01%	0.002%
62	8.021	2170	2171	2174	rVB	396	138	0.01%	0.001%
63	8.088	2182	2192	2229	rBV	440675	809953	50.48%	6.287%
64	8.461	2306	2308	2312	rVB2	376	259	0.02%	0.002%
65	8.519	2324	2326	2328	rBV	237	128	0.01%	0.001%
66	8.615	2354	2356	2360	rVB3	394	228	0.01%	0.002%
67	8.699	2379	2382	2386	rVB	583	330	0.02%	0.003%
68	8.731	2387	2392	2398	rBV2	185	230	0.01%	0.002%
69	8.757	2398	2400	2403	rBV	176	124	0.01%	0.001%
70	8.853	2418	2430	2463	rBV	719858	1177189	73.37%	9.138%
71	9.181	2530	2532	2534	rBV	368	167	0.01%	0.001%
72	9.233	2545	2548	2550	rBV	255	140	0.01%	0.001%
73	9.275	2559	2561	2564	rVB2	245	115	0.01%	0.001%
74	9.439	2609	2612	2615	rBV2	338	235	0.01%	0.002%
75	9.538	2640	2643	2646	rBV2	187	148	0.01%	0.001%
76	9.712	2694	2697	2698	rBV	283	151	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061021\
 Data File : VV021542.D
 Acq On : 10 Jun 2021 13:58
 Operator : SY/MD
 Sample : M2649-16
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
 Title : VOC Analysis

77	9.831	2729	2734	2736	rBV	126	142	0.01%	0.001%
78	9.857	2740	2742	2747	rVB2	278	168	0.01%	0.001%
79	10.075	2806	2810	2812	rBV2	253	171	0.01%	0.001%
80	10.130	2819	2827	2834	rVB3	1993	2747	0.17%	0.021%
81	10.217	2839	2854	2877	rBV	528059	830793	51.78%	6.449%
82	10.660	2990	2992	2994	rBV	476	171	0.01%	0.001%
83	10.767	3024	3025	3027	rBV	278	121	0.01%	0.001%
84	10.873	3055	3058	3059	rBV	201	113	0.01%	0.001%
85	10.995	3093	3096	3100	rBV2	258	178	0.01%	0.001%
86	11.021	3101	3104	3106	rBV	300	212	0.01%	0.002%
87	11.146	3138	3143	3150	rBV6	1131	1516	0.09%	0.012%
88	11.249	3163	3175	3203	rBV	857007	1335914	83.26%	10.370%
89	11.625	3280	3292	3314	rBV	870577	1369231	85.34%	10.629%
90	11.889	3373	3374	3378	rVB2	418	192	0.01%	0.001%
91	12.030	3416	3418	3422	rBV2	340	213	0.01%	0.002%
92	12.056	3422	3426	3427	rBV	344	238	0.01%	0.002%
93	12.310	3502	3505	3507	rBV2	230	131	0.01%	0.001%
94	12.339	3511	3514	3517	rBV	388	318	0.02%	0.002%
95	12.483	3557	3559	3571	rVB3	451	730	0.05%	0.006%
96	12.596	3592	3594	3595	rBV3	307	112	0.01%	0.001%
97	12.651	3609	3611	3614	rBV2	350	227	0.01%	0.002%
98	12.828	3662	3666	3672	rBV	8224	4850	0.30%	0.038%
99	12.895	3682	3687	3692	rBV3	559	823	0.05%	0.006%
100	13.114	3752	3755	3756	rBV2	412	198	0.01%	0.002%




Sum of corrected areas: 12882444

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061021\
Data File : VV021542.D
Acq On : 10 Jun 2021 13:58
Operator : SY/MD
Sample : M2649-16
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

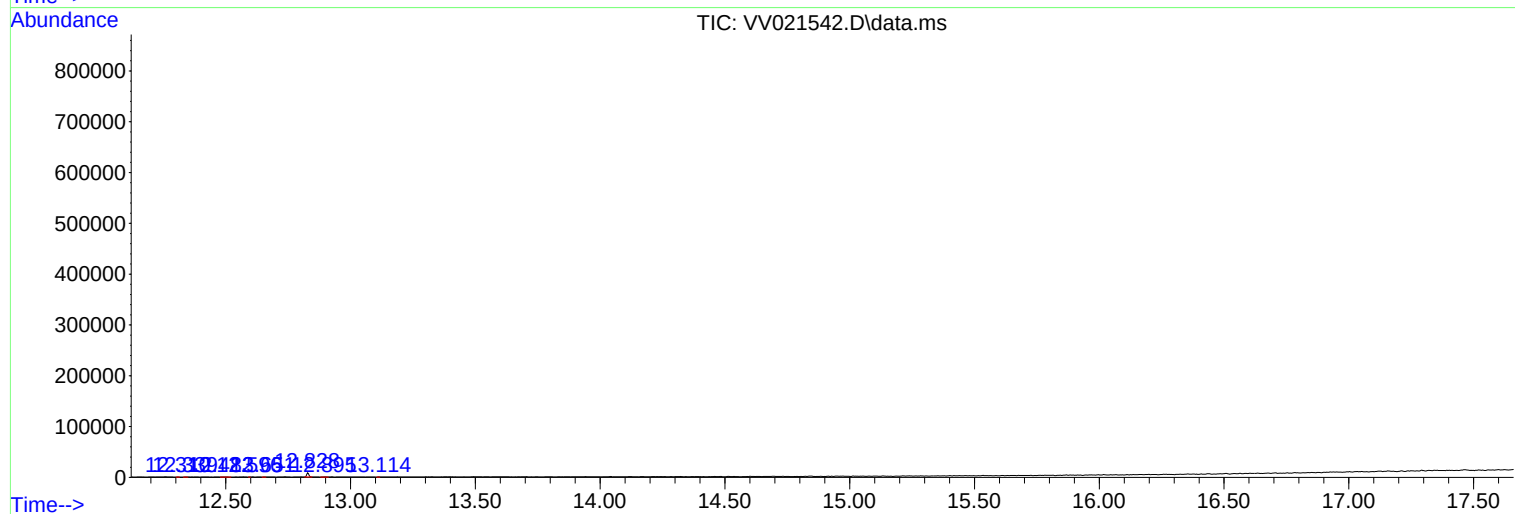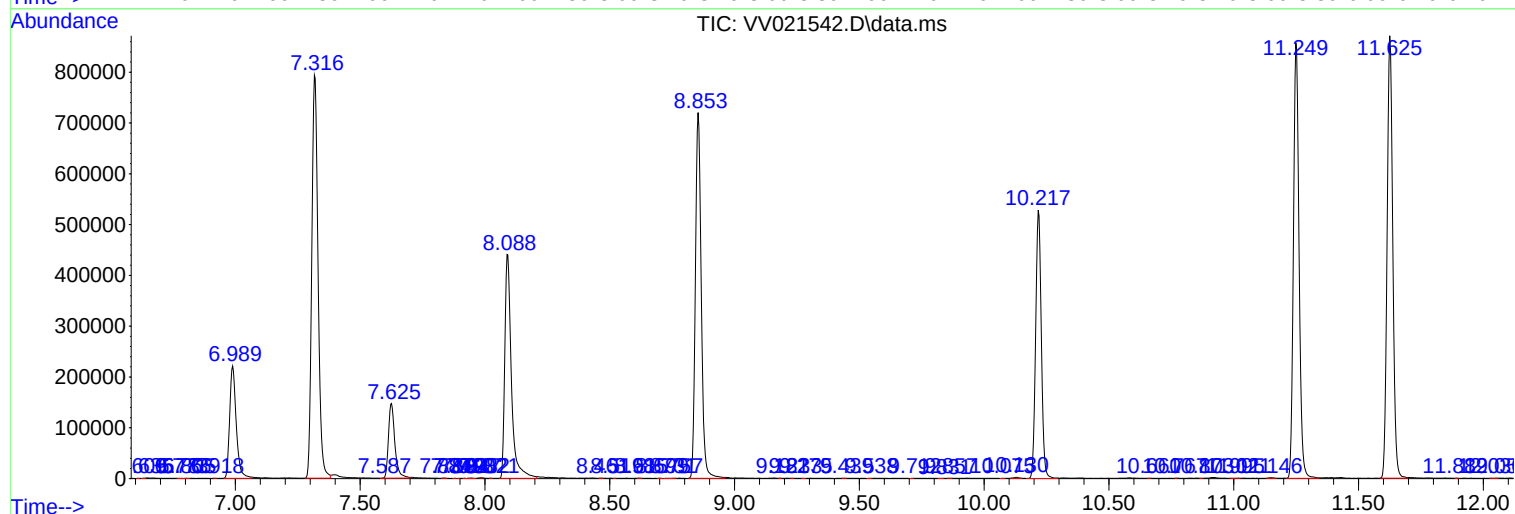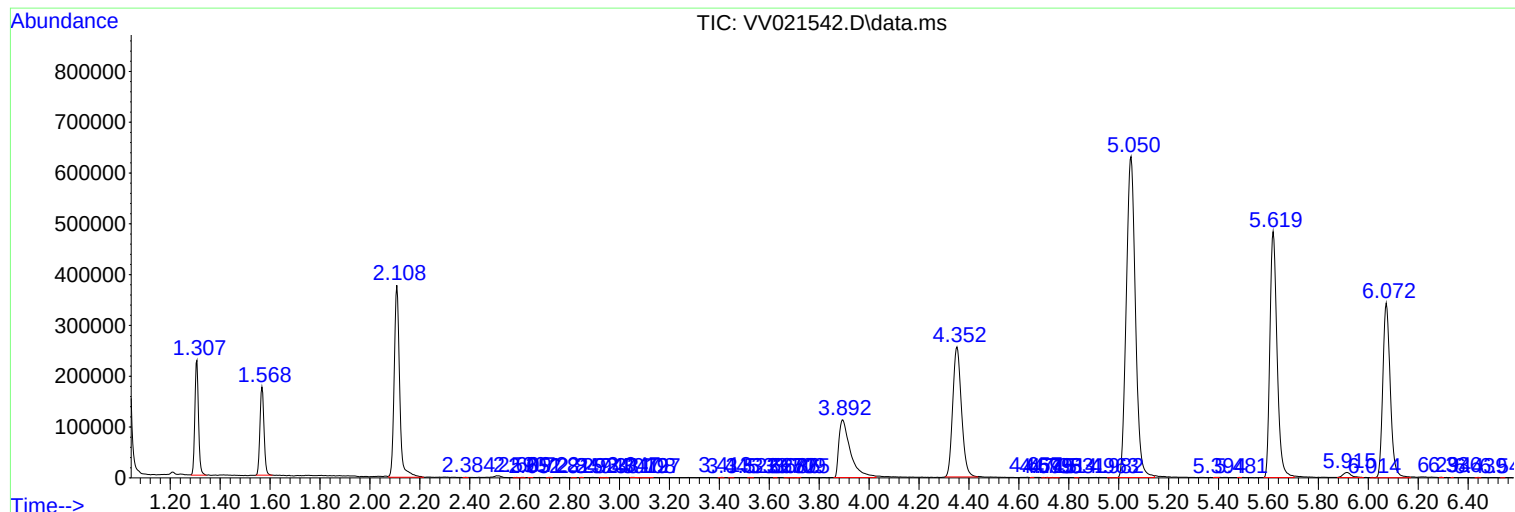

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061021\
Data File : VV021542.D
Acq On : 10 Jun 2021 13:58
Operator : SY/MD
Sample : M2649-16
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061021\
Data File : VV021542.D
Acq On : 10 Jun 2021 13:58
Operator : SY/MD
Sample : M2649-16
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
