
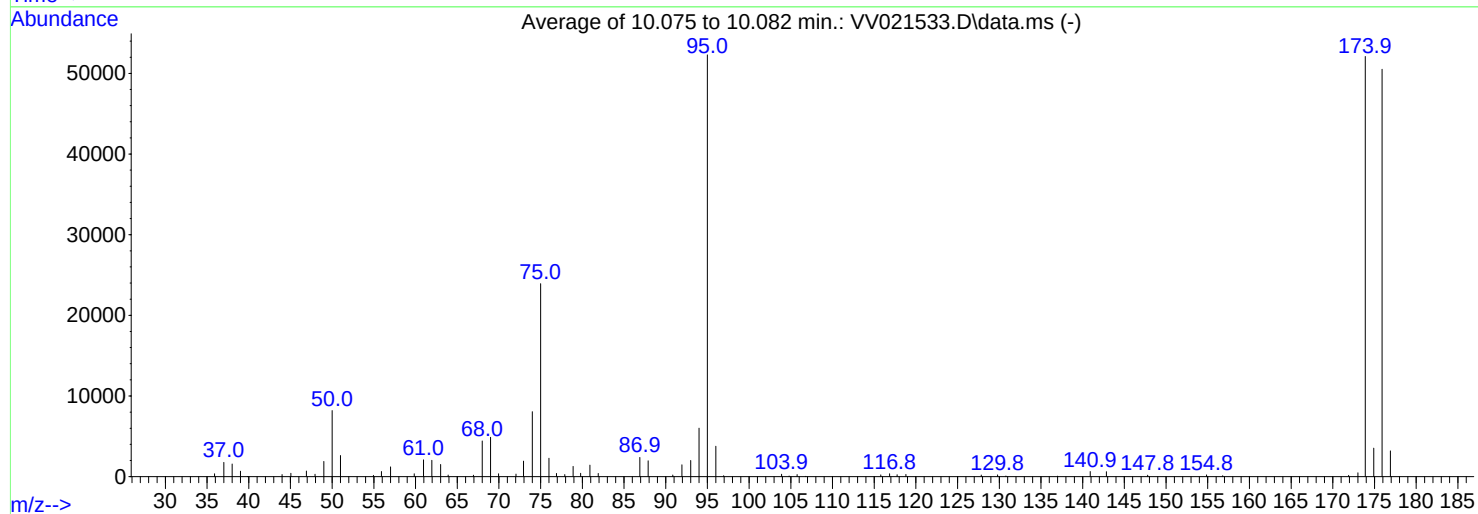


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061021\
 Data File : VV021533.D
 Acq On : 10 Jun 2021 10:03
 Operator : SY/MD
 Sample : BFB69
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB169

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
 Title : VOC Analysis
 Last Update : Fri Jun 11 02:43:15 2021

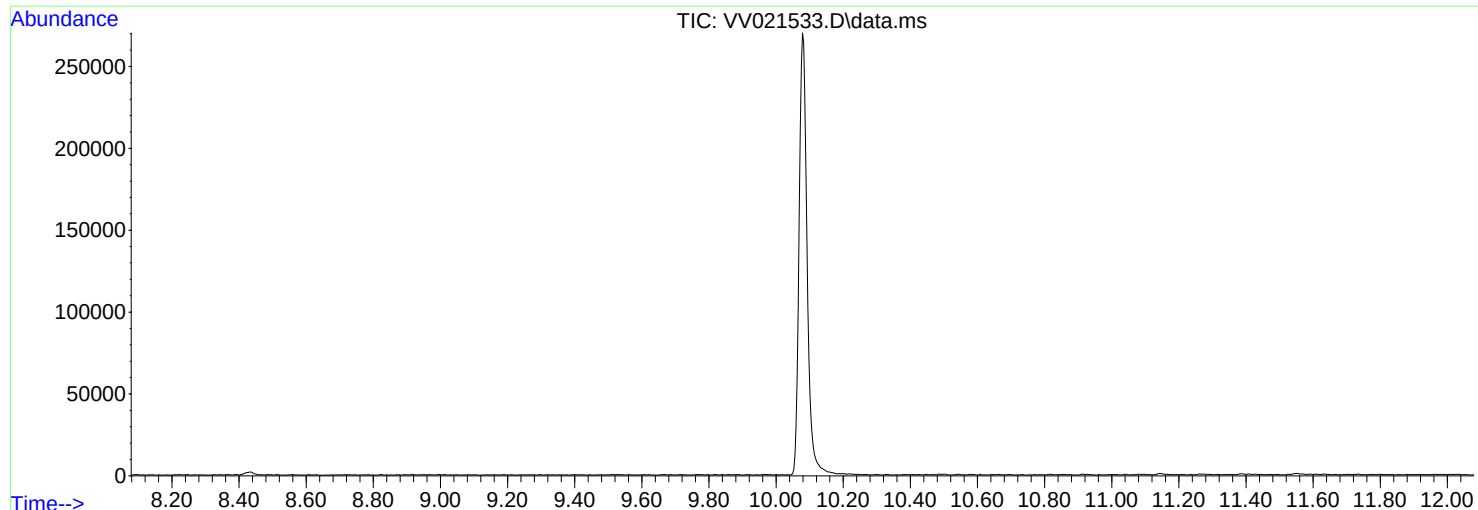

AutoFind: Scans 2810, 2811, 2812; Background Corrected with Scan 2799

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.7	8198	PASS
75	95	30	80	45.8	23928	PASS
95	95	100	100	100.0	52296	PASS
96	95	5	9	7.2	3772	PASS
173	174	0.00	2	0.9	480	PASS
174	95	50	120	99.6	52091	PASS
175	174	5	9	6.8	3528	PASS
176	174	95	105	96.9	50499	PASS
177	176	5	10	6.3	3205	PASS

m/z	Abundance
35.90	312.0
37.00	1750.0
38.00	1466.0
39.00	684.0
39.90	169.0
44.00	697.0
45.00	411.0
46.90	754.0
47.90	338.0
49.00	1820.0
50.00	8185.0
51.00	2531.0
55.00	162.0
55.90	633.0
57.00	1267.0
59.80	377.0
61.00	2020.0
61.90	1932.0
63.00	1508.0
63.90	144.0
67.00	158.0
68.00	4467.0
69.00	4672.0
69.90	373.0
72.00	320.0
72.90	1838.0
74.00	7665.0
75.00	23480.0
76.00	2195.0
76.80	398.0
77.90	291.0
78.90	1215.0
79.80	414.0
80.90	1403.0
81.90	408.0
86.90	2201.0
87.90	1878.0
90.90	189.0
91.90	1380.0
93.00	1858.0
94.00	6202.0
95.00	50008.0
96.00	3800.0
97.00	131.0
103.90	278.0
105.70	275.0
115.80	174.0
116.80	379.0
117.80	215.0
118.80	272.0
127.90	179.0
129.80	199.0
130.80	110.0
137.00	101.0
140.90	601.0
142.80	594.0
147.80	175.0
154.90	234.0
156.90	136.0
171.90	120.0
173.00	427.0
173.90	49040.0
174.90	3461.0
175.90	48112.0
176.90	3124.0

Instrument :
MSVOA_V
ClientSampleId :
BFB169

m/z	Abundance
35.90	380.0
37.00	1740.0
38.00	1615.0
39.00	618.0
39.90	179.0
44.00	656.0
45.10	433.0
46.90	617.0
48.00	250.0
49.00	1849.0
50.00	7945.0
51.00	2597.0
54.90	171.0
55.90	601.0
57.00	1145.0
59.90	358.0
60.90	2096.0
62.00	2074.0
63.00	1467.0
63.90	246.0
66.90	183.0
68.00	4275.0
69.00	4967.0
70.00	347.0
72.10	315.0
73.00	1963.0
74.00	8171.0
75.00	23624.0
76.00	2256.0
77.00	394.0
77.90	242.0
78.90	1284.0
79.80	397.0
80.90	1408.0
81.90	370.0
86.90	2476.0
87.90	1974.0
90.90	206.0
92.00	1510.0
93.00	2110.0
94.00	5667.0
95.00	53048.0
96.00	3526.0
96.90	100.0
103.90	295.0
104.80	108.0
105.80	246.0
115.80	242.0
116.90	334.0
117.80	247.0
118.80	282.0
127.80	223.0
129.80	253.0
140.90	630.0
142.90	625.0
147.80	204.0
154.80	199.0
156.70	111.0
171.90	181.0
173.00	531.0
173.90	53504.0
174.90	3537.0
175.90	51424.0
176.90	3200.0

Instrument :
MSVOA_V
ClientSampleId :
BFB169

m/z	Abundance
39.80	159.0
44.00	428.0

Instrument :
MSVOA_V
ClientSampleId :
BFB169

m/z	Abundance
35.90	356.0
37.00	1829.0
38.00	1597.0
39.00	697.0
39.90	182.0
44.00	738.0
45.10	434.0
46.90	711.0
47.90	314.0
49.00	1963.0
50.00	8465.0
51.00	2739.0
54.90	169.0
55.90	674.0
57.00	1232.0
59.80	359.0
61.00	2138.0
62.00	2091.0
63.00	1555.0
63.90	200.0
66.90	184.0
68.00	4528.0
69.00	5005.0
69.90	368.0
72.00	323.0
73.00	1962.0
74.00	8301.0
75.00	24680.0
76.00	2400.0
76.90	397.0
77.90	271.0
78.90	1319.0
79.80	417.0
80.90	1457.0
81.90	398.0
86.90	2477.0
87.90	2037.0
90.80	217.0
91.90	1515.0
93.00	2054.0
94.00	6167.0
95.00	53832.0
96.00	3989.0
96.90	122.0
103.90	311.0
104.80	111.0
105.70	284.0
106.80	106.0
115.80	231.0
116.80	371.0
117.70	244.0
118.80	290.0
127.80	195.0
129.80	211.0
130.80	105.0
137.00	107.0
140.90	651.0
142.90	619.0
147.80	172.0
154.80	238.0
156.80	129.0
171.90	165.0
173.00	481.0
173.90	53728.0
174.90	3585.0
175.90	51960.0
176.90	3291.0

Instrument :
MSVOA_V
ClientSampleId :
BFB169