

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW061022\
 Data File : VW026095.D
 Acq On : 10 Jun 2022 16:06
 Operator : SY/MD
 Sample : N3247-01RE
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXYS3RE

Quant Time: Jun 11 01:25:57 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Jun 11 01:25:15 2022
 Response via : Initial Calibration

Compound	R.T. QIon		Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	175470	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	170407	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.246	152	71054	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.317	65	105996	10.290	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	= 205.800%#		
7) Chloroethane-d5	1.577	69	113414	10.532	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	= 210.600%#		
11) 1,1-Dichloroethene-d2	2.117	63	173843	7.307	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	= 146.200%#		
20) 2-Butanone-d5	3.905	46	121933	80.037	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	= 160.080%#		
24) Chloroform-d	4.355	84	207087	9.486	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	= 189.800%#		
26) 1,2-Dichloroethane-d4	5.037	65	87905	9.872	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	= 197.400%#		
32) Benzene-d6	5.053	84	420987	10.224	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	= 204.400%#		
36) 1,2-Dichloropropane-d6	6.069	67	126471	9.928	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	= 198.600%#		
41) Toluene-d8	7.317	98	345585	9.497	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	= 190.000%#		
43) trans-1,3-Dichloroprop...	7.622	79	31312	8.348	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	= 167.000%#		
46) 2-Hexanone-d5	8.088	63	138656	84.008	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	= 168.020%#		
56) 1,1,2,2-Tetrachloroeth...	10.214	84	69080	8.042	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	= 160.800%#		
66) 1,2-Dichlorobenzene-d4	11.622	152	105233	9.680	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	= 193.600%#		
Target Compounds						
13) Acetone	2.201	43	11202	9.220	ug/L	83
16) Methylene chloride	2.519	84	3139	0.223	ug/L	96
25) Chloroform	4.387	83	8628	0.347	ug/L	97
34) Trichloroethene	5.921	95	5117	0.366	ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061022\
Data File : VV026095.D
Acq On : 10 Jun 2022 16:06
Operator : SY/MD
Sample : N3247-01RE
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXYS3RE

Quant Time: Jun 11 01:25:57 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Jun 11 01:25:15 2022
Response via : Initial Calibration




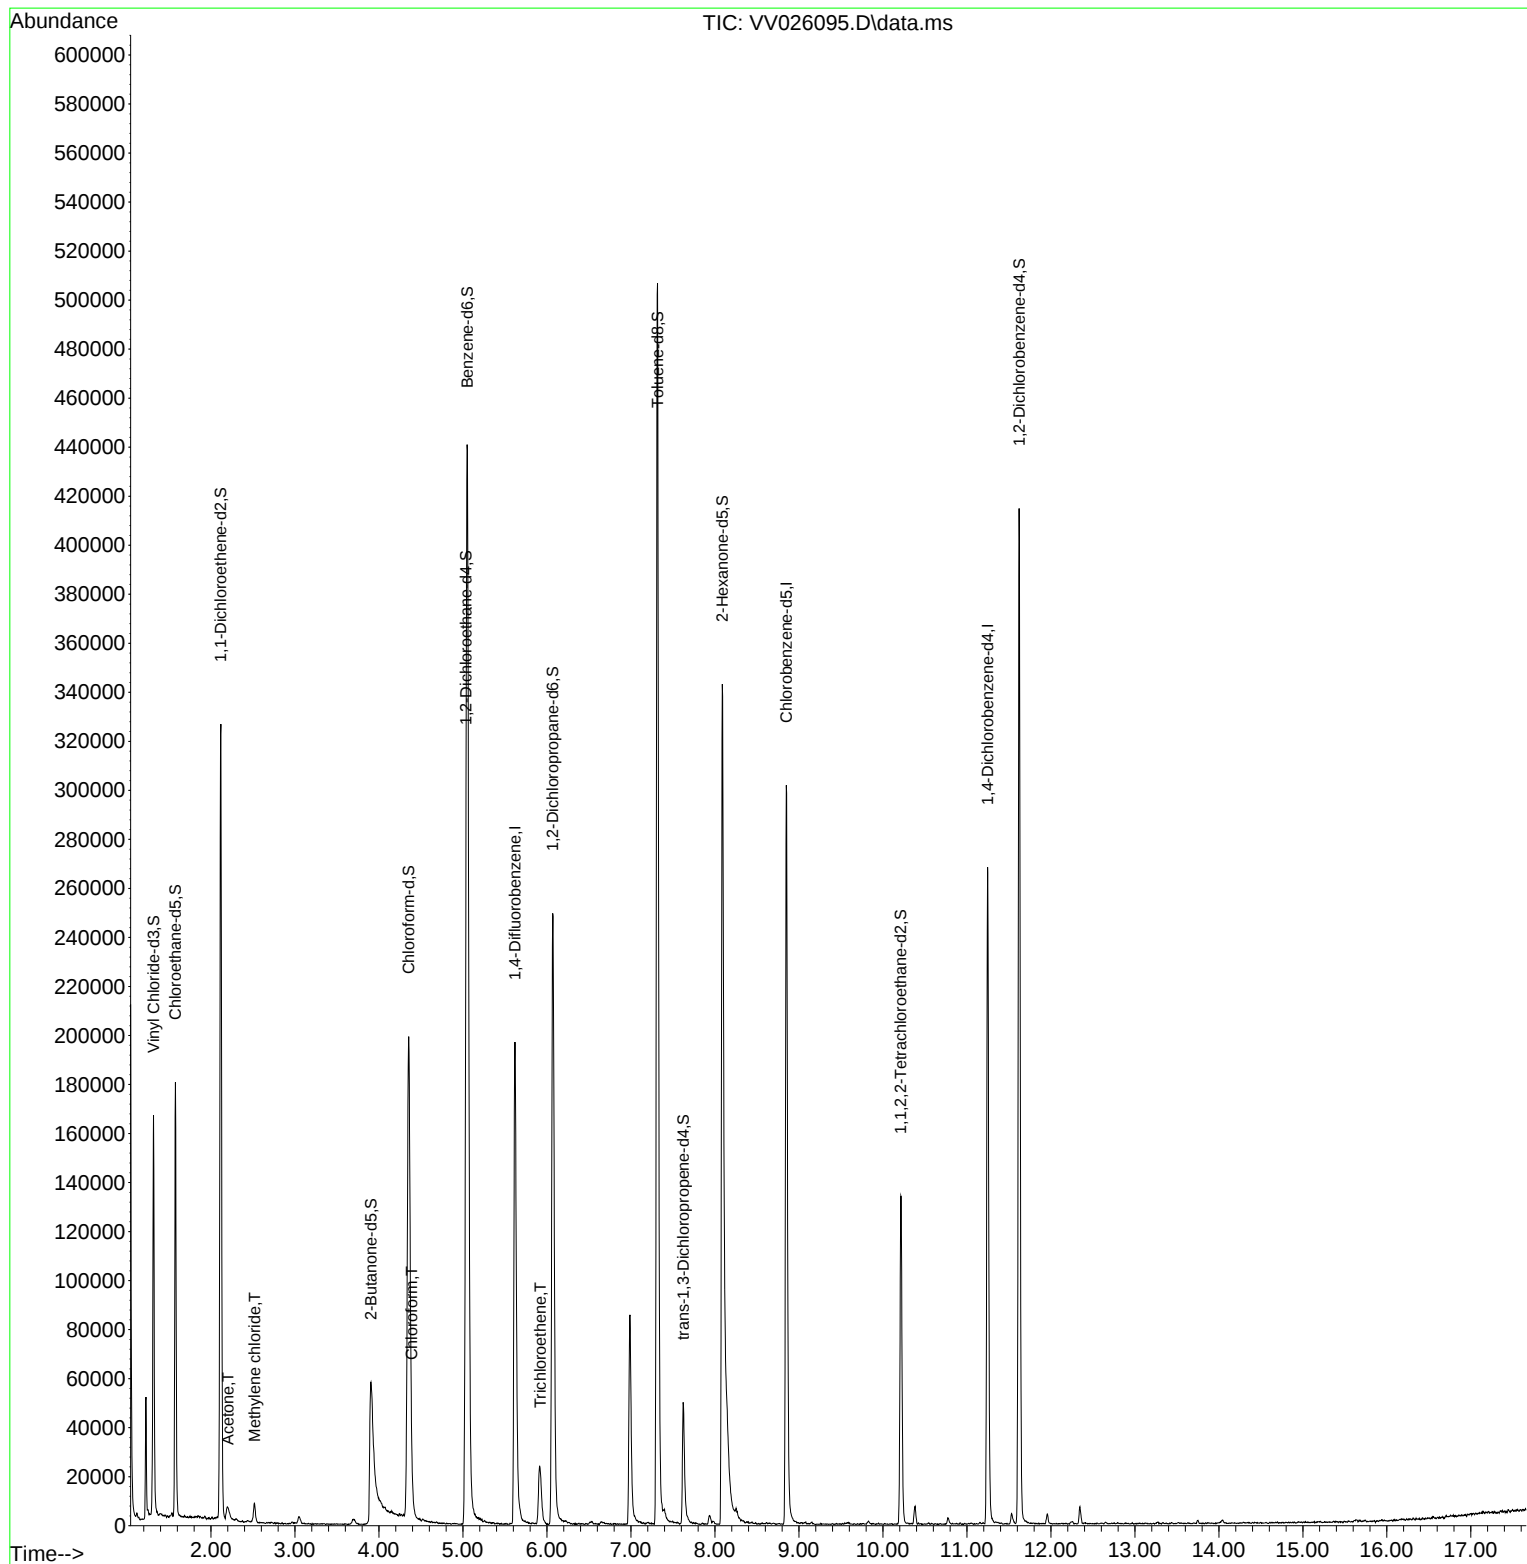


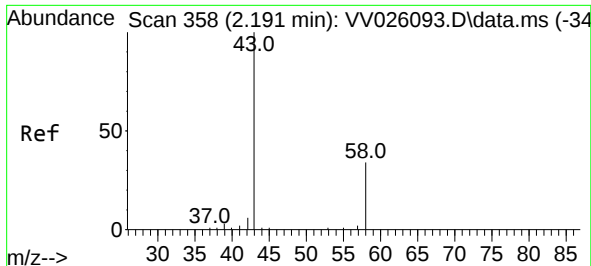

#13
Acetone
Concen: 9.220 ug/L
RT: 2.201 min Scan# 301
Delta R.T. 0.010 min
Lab File: VV026095.D
Acq: 10 Jun 2022 16:06




Instrument :
MSVOA_V
ClientSampleId :
EXYS3RE


Tgt Ion: 43 Resp: 11202
Ion Ratio Lower Upper
43 100
58 32.1 0.0 47.6

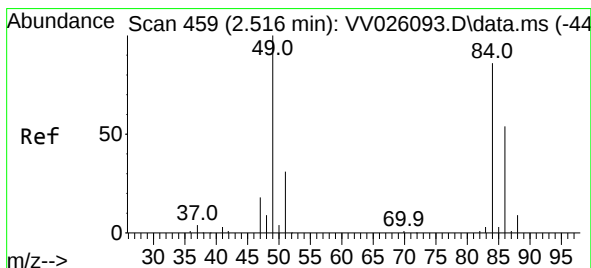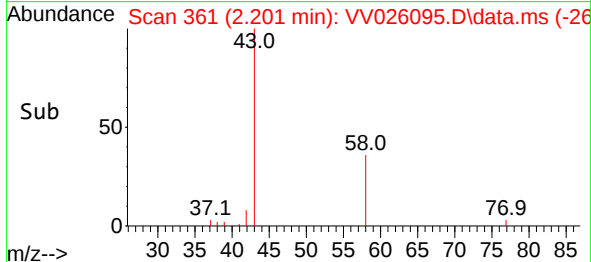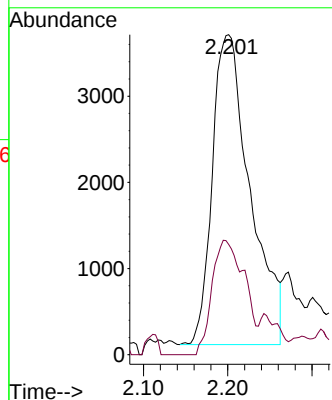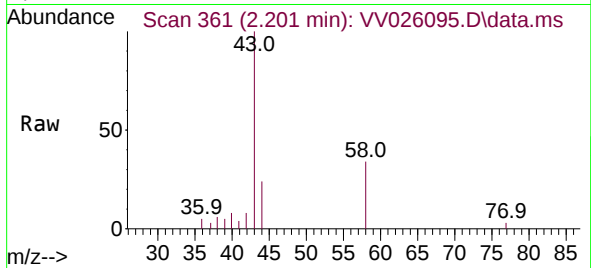

#16
Methylene chloride
Concen: 0.223 ug/L
RT: 2.519 min Scan# 460
Delta R.T. 0.003 min
Lab File: VV026095.D
Acq: 10 Jun 2022 16:06

Tgt Ion: 84 Resp: 3139
Ion Ratio Lower Upper
84 100
86 59.4 45.6 84.6
49 120.4 82.9 153.9


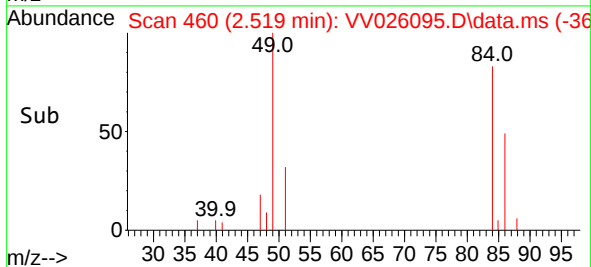
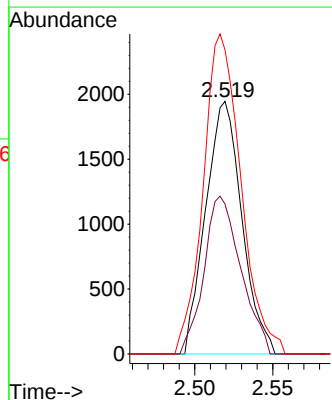
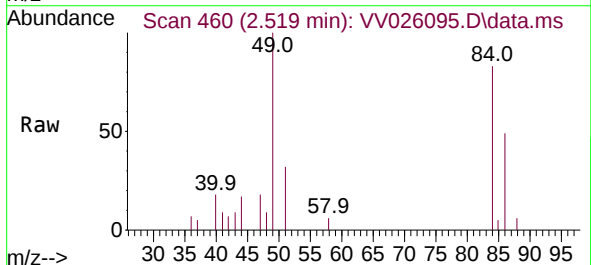


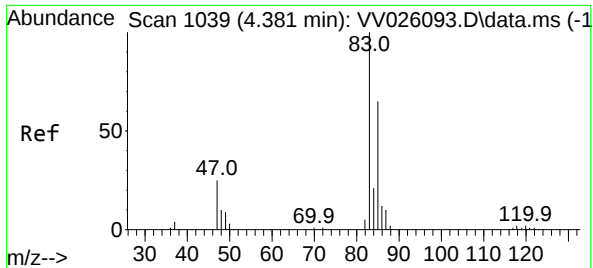

#25
Chloroform
Concen: 0.347 ug/L
RT: 4.387 min Scan# 1039
Delta R.T. 0.006 min
Lab File: VV026095.D
Acq: 10 Jun 2022 16:06

Instrument :
MSVOA_V
ClientSampleId :
EXYS3RE

Tgt Ion: 83 Resp: 8628
Ion Ratio Lower Upper
83 100
85 62.4 45.2 84.0

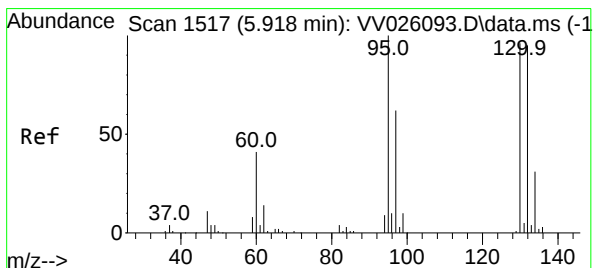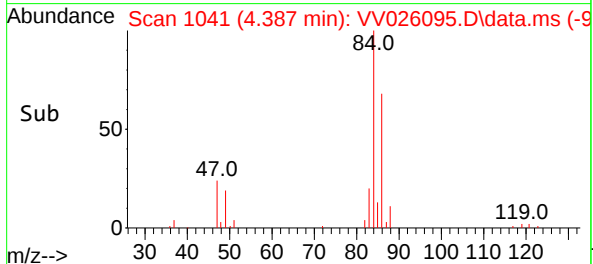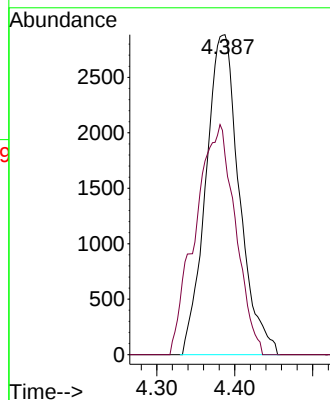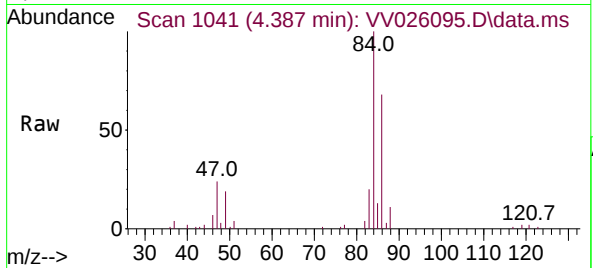

#34
Trichloroethene
Concen: 0.366 ug/L
RT: 5.921 min Scan# 1518
Delta R.T. 0.003 min
Lab File: VV026095.D
Acq: 10 Jun 2022 16:06

Tgt Ion: 95 Resp: 5117
Ion Ratio Lower Upper
95 100
97 65.8 44.0 81.6
132 96.6 67.5 125.4
130 89.2 69.7 129.5

