

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW061022\
 Data File : VW026097.D
 Acq On : 10 Jun 2022 16:54
 Operator : SY/MD
 Sample : N3247-01
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXYS3

Quant Time: Jun 11 01:26:33 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Jun 11 01:25:15 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.622	114	182385	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	178314	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	72568	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.317	65	53149	4.964	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	99.200%	
7) Chloroethane-d5	1.581	69	61854	5.526	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	110.600%	
11) 1,1-Dichloroethene-d2	2.118	63	89237	3.608	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	72.200%	
20) 2-Butanone-d5	3.908	46	80312	50.718	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	101.440%	
24) Chloroform-d	4.359	84	117004	5.156	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	103.200%	
26) 1,2-Dichloroethane-d4	5.040	65	50099	5.413	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	108.200%	
32) Benzene-d6	5.056	84	222878	5.173	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	103.400%	
36) 1,2-Dichloropropane-d6	6.076	67	71303	5.349	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	107.000%	
41) Toluene-d8	7.320	98	175078	4.598	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	92.000%	
43) trans-1,3-Dichloroprop...	7.629	79	16548	4.216	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	84.400%	
46) 2-Hexanone-d5	8.092	63	74132	42.923	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	85.840%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	39847	4.433	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	88.600%	
66) 1,2-Dichlorobenzene-d4	11.625	152	60917	5.487	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	109.800%	
Target Compounds						Qvalue
13) Acetone	2.191	43	11935	9.451	ug/L	73
25) Chloroform	4.391	83	6175	0.239	ug/L	94
34) Trichloroethene	5.928	95	4633	0.316	ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061022\
Data File : VV026097.D
Acq On : 10 Jun 2022 16:54
Operator : SY/MD
Sample : N3247-01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXYS3

Quant Time: Jun 11 01:26:33 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Jun 11 01:25:15 2022
Response via : Initial Calibration

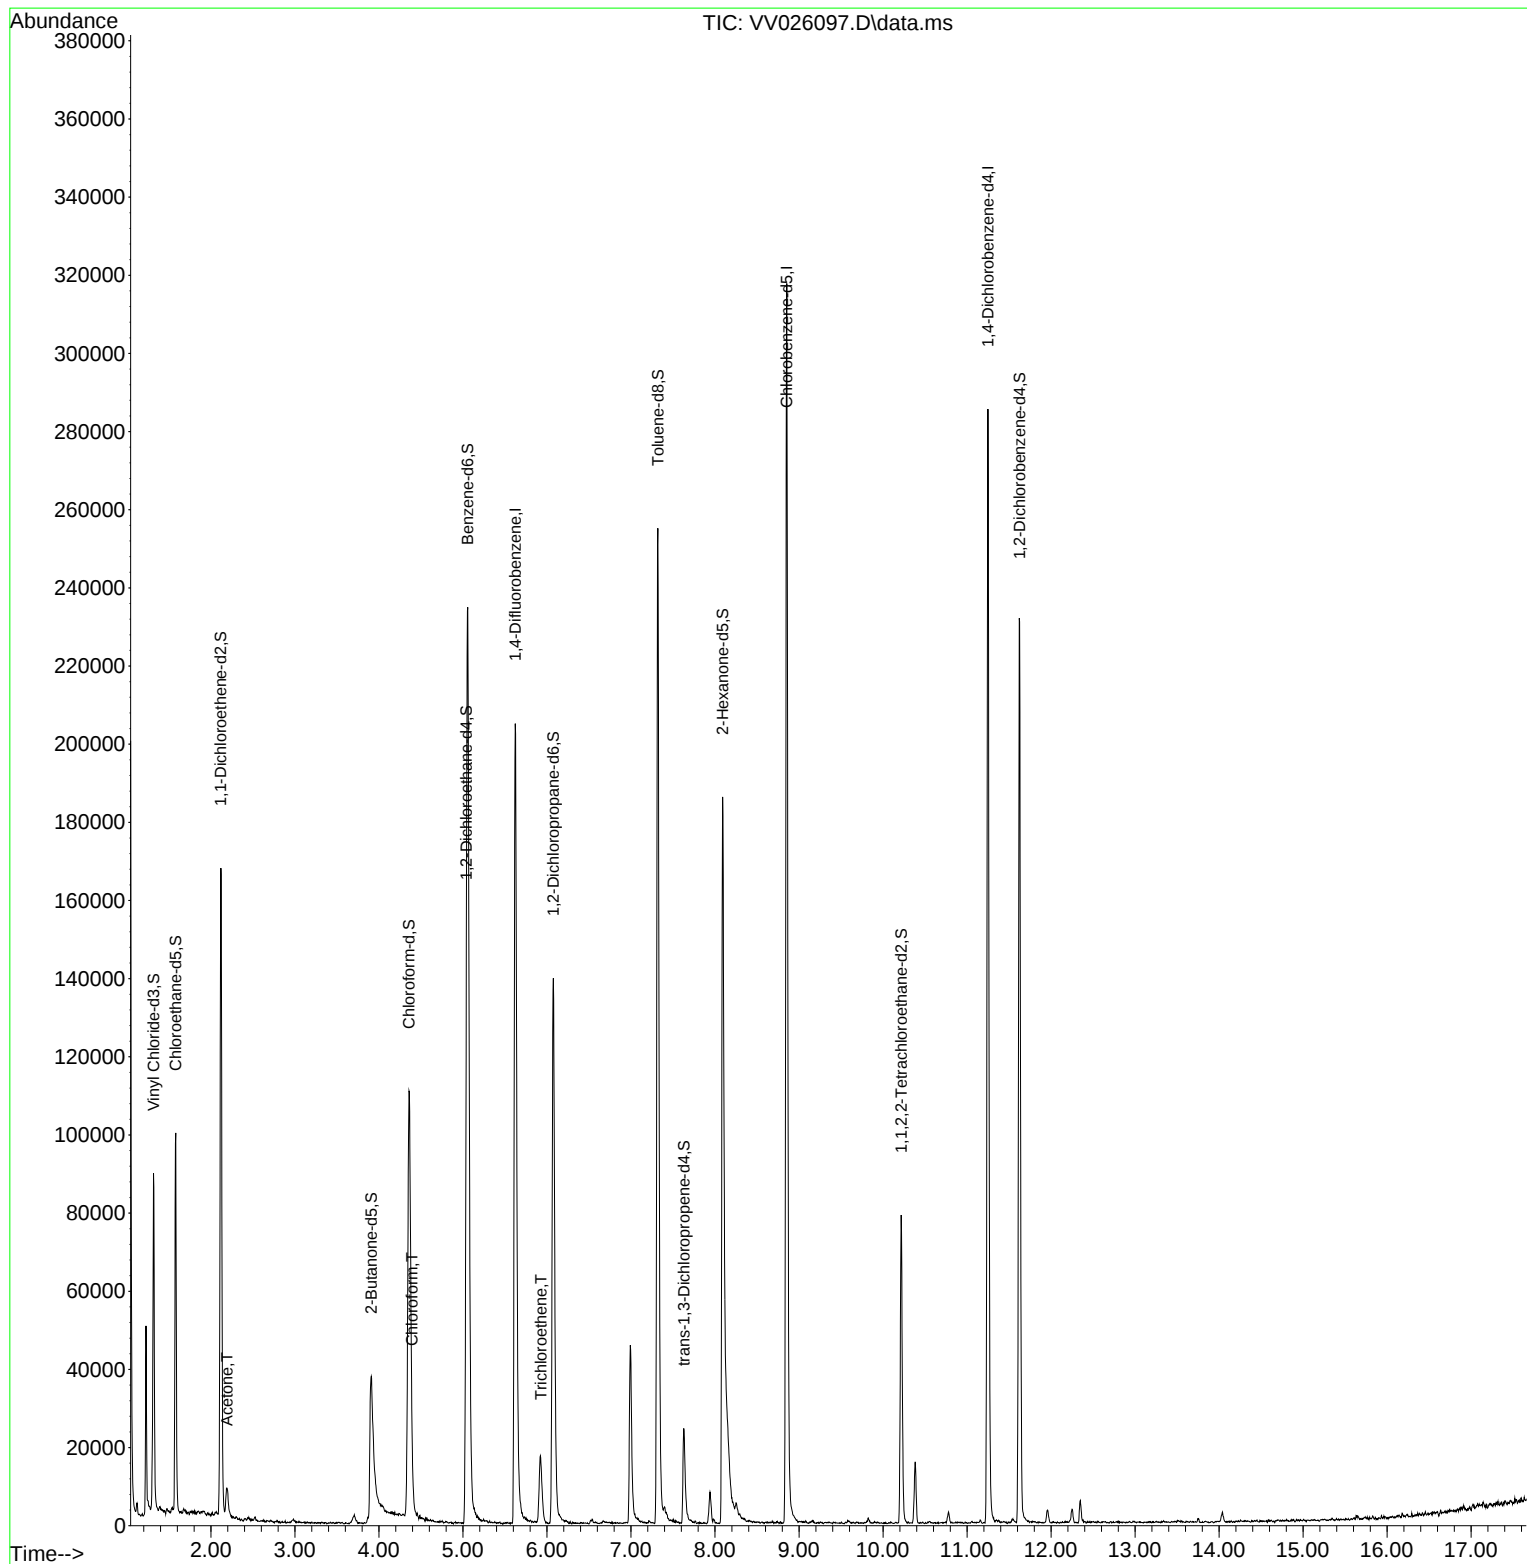

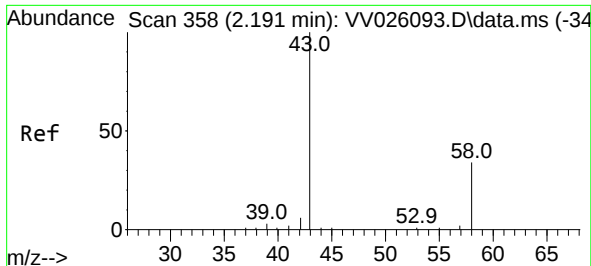

#13

Acetone

Concen: 9.451 ug/L

RT: 2.191 min Scan# 31

Delta R.T. 0.000 min

Lab File: VV026097.D

Acq: 10 Jun 2022 16:54

Instrument :

MSVOA_V

ClientSampleId :





EXYS3

Tgt Ion: 43 Resp: 11935

Ion Ratio Lower Upper

43 100

58 36.9 0.0 47.6

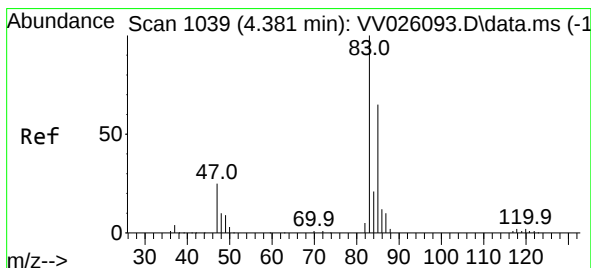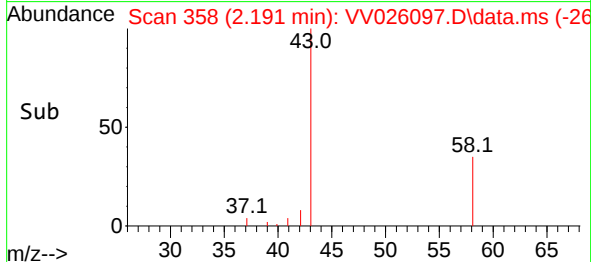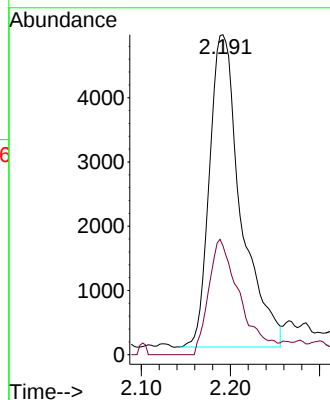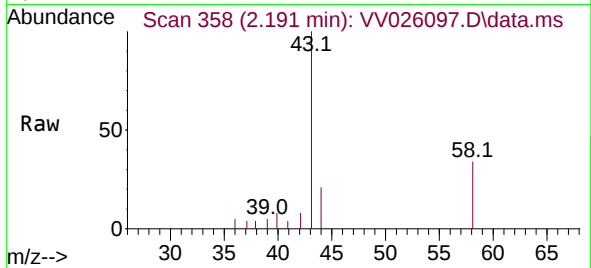

#25

Chloroform

Concen: 0.239 ug/L

RT: 4.391 min Scan# 1042

Delta R.T. 0.010 min

Lab File: VV026097.D




Acq: 10 Jun 2022 16:54


Tgt Ion: 83 Resp: 6175

Ion Ratio Lower Upper

83 100

85 69.5 45.2 84.0

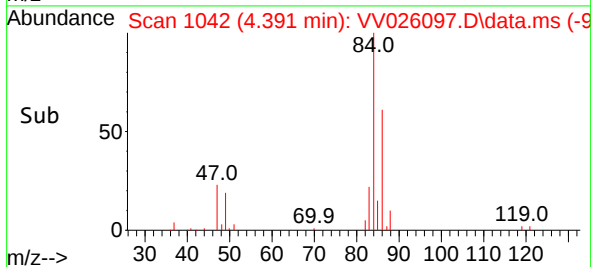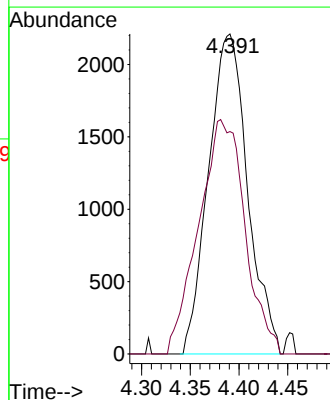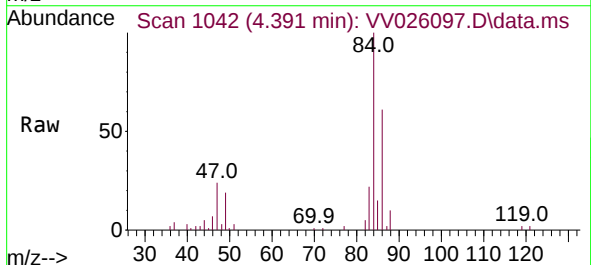

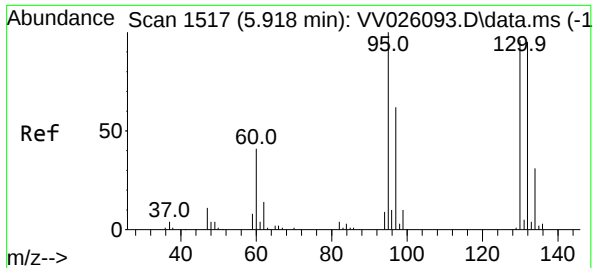

#34
 Trichloroethene
 Concen: 0.316 ug/L
 RT: 5.928 min Scan# 11
 Delta R.T. 0.010 min
 Lab File: VV026097.D
 Acq: 10 Jun 2022 16:54

Instrument :
 MSVOA_V
 ClientSampleId :
 EXYS3

Tgt Ion: 95 Resp: 4633

Ion	Ratio	Lower	Upper
95	100		
97	63.2	44.0	81.6
132	87.0	67.5	125.4
130	102.4	69.7	129.5

