

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW061022\
 Data File : VW026105.D
 Acq On : 10 Jun 2022 20:05
 Operator : SY/MD
 Sample : N3272-07
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B51

Quant Time: Jun 11 01:28:35 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Jun 11 01:25:15 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.622	114	167517	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	158800	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	63817	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.317	65	52315	5.320	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	106.400%
7) Chloroethane-d5	1.577	69	59558	5.793	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	115.800%
11) 1,1-Dichloroethene-d2	2.117	63	85947	3.784	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	75.600%
20) 2-Butanone-d5	3.912	46	88569	60.897	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	121.800%
24) Chloroform-d	4.359	84	115388	5.537	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	110.800%
26) 1,2-Dichloroethane-d4	5.040	65	50108	5.894	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	117.800%
32) Benzene-d6	5.056	84	214837	5.599	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	112.000%
36) 1,2-Dichloropropane-d6	6.075	67	71094	5.989	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	119.800%
41) Toluene-d8	7.320	98	165937	4.893	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	97.800%
43) trans-1,3-Dichloroprop...	7.628	79	15526	4.442	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	88.800%
46) 2-Hexanone-d5	8.091	63	77260	50.231	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	100.460%
56) 1,1,2,2-Tetrachloroeth...	10.217	84	44485	5.558	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	111.200%
66) 1,2-Dichlorobenzene-d4	11.625	152	56765	5.814	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	116.200%
Target Compounds						
					Qvalue	
34) Trichloroethene	5.928	95	4297	0.330	ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061022\
Data File : VV026105.D
Acq On : 10 Jun 2022 20:05
Operator : SY/MD
Sample : N3272-07
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B51


Quant Time: Jun 11 01:28:35 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Jun 11 01:25:15 2022
Response via : Initial Calibration

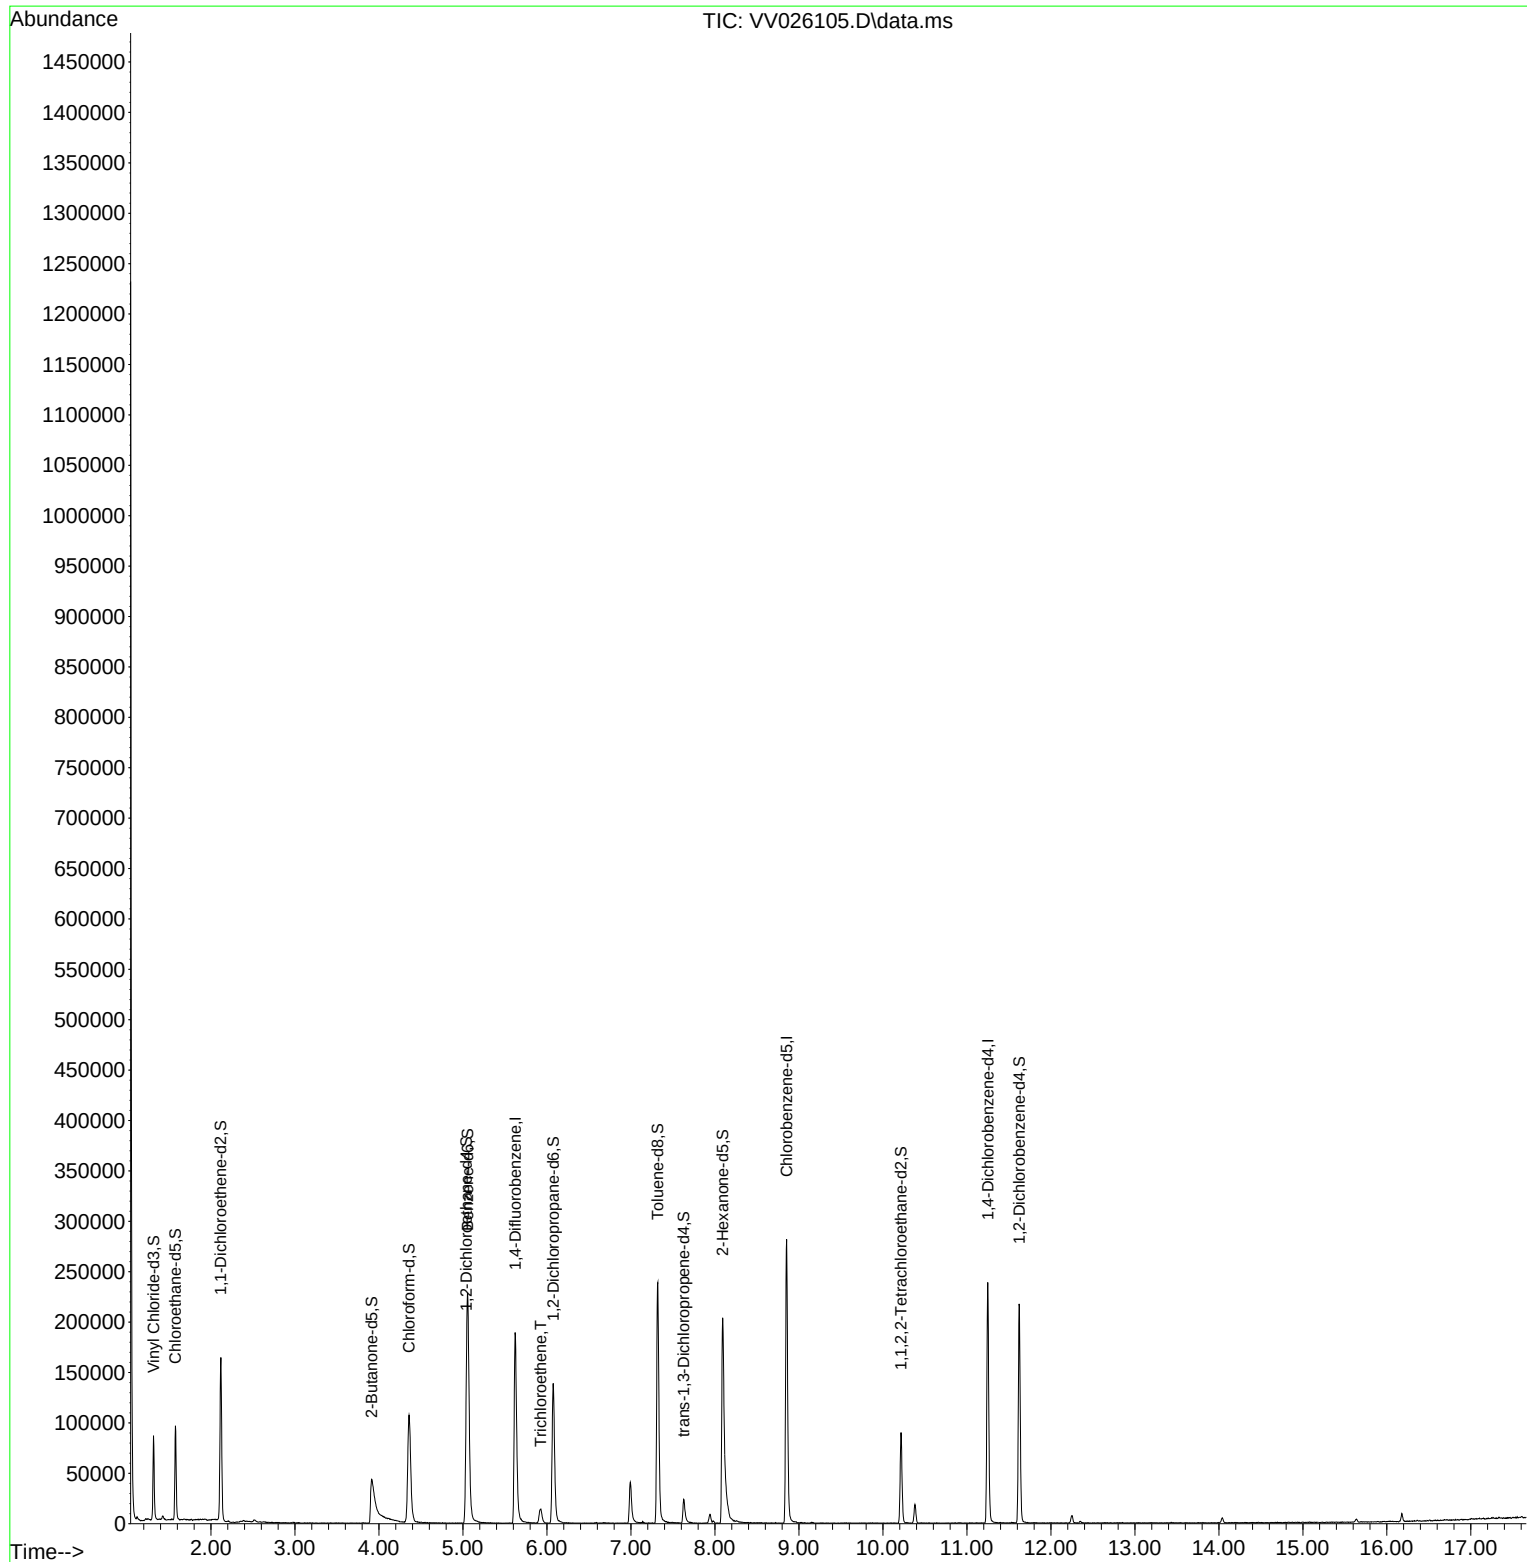

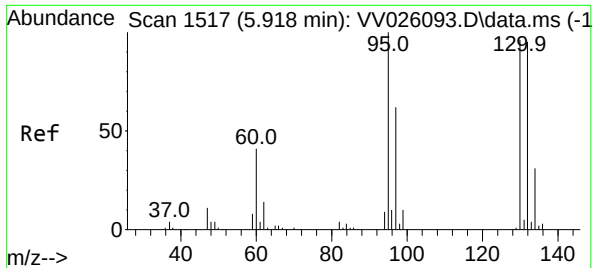

#34
 Trichloroethene
 Concen: 0.330 ug/L
 RT: 5.928 min Scan# 11
 Delta R.T. 0.010 min
 Lab File: VV026105.D
 Acq: 10 Jun 2022 20:05

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B51

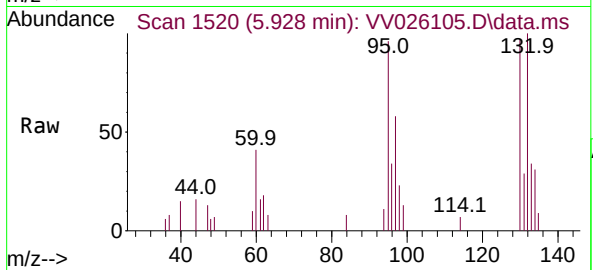

Tgt Ion: 95 Resp: 4297

Ion	Ratio	Lower	Upper
95	100		
97	60.2	44.0	81.6
132	103.8	67.5	125.4
130	100.5	69.7	129.5

