

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW061022\
 Data File : VW026106.D
 Acq On : 10 Jun 2022 20:29
 Operator : SY/MD
 Sample : N3272-08
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B52

Quant Time: Jun 11 01:28:50 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Jun 11 01:25:15 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.622	114	176649	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	174039	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	67571	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.317	65	52106	5.025	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	100.400%
7) Chloroethane-d5	1.577	69	59498	5.488	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	109.800%
11) 1,1-Dichloroethene-d2	2.117	63	85462	3.568	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	71.400%
20) 2-Butanone-d5	3.915	46	70583	46.022	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	92.040%
24) Chloroform-d	4.359	84	112719	5.129	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	102.600%
26) 1,2-Dichloroethane-d4	5.040	65	47978	5.352	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	107.000%
32) Benzene-d6	5.056	84	213645	5.080	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	101.600%
36) 1,2-Dichloropropane-d6	6.075	67	65943	5.068	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	101.400%
41) Toluene-d8	7.320	98	161936	4.357	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	87.200%
43) trans-1,3-Dichloroprop...	7.628	79	14956	3.904	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	78.000%
46) 2-Hexanone-d5	8.091	63	72300	42.890	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	85.780%
56) 1,1,2,2-Tetrachloroeth...	10.217	84	41600	4.742	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	94.800%
66) 1,2-Dichlorobenzene-d4	11.622	152	56245	5.441	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	108.800%
Target Compounds						
					Qvalue	
34) Trichloroethene	5.928	95	3974	0.278	ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061022\
Data File : VV026106.D
Acq On : 10 Jun 2022 20:29
Operator : SY/MD
Sample : N3272-08
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B52


Quant Time: Jun 11 01:28:50 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Jun 11 01:25:15 2022
Response via : Initial Calibration

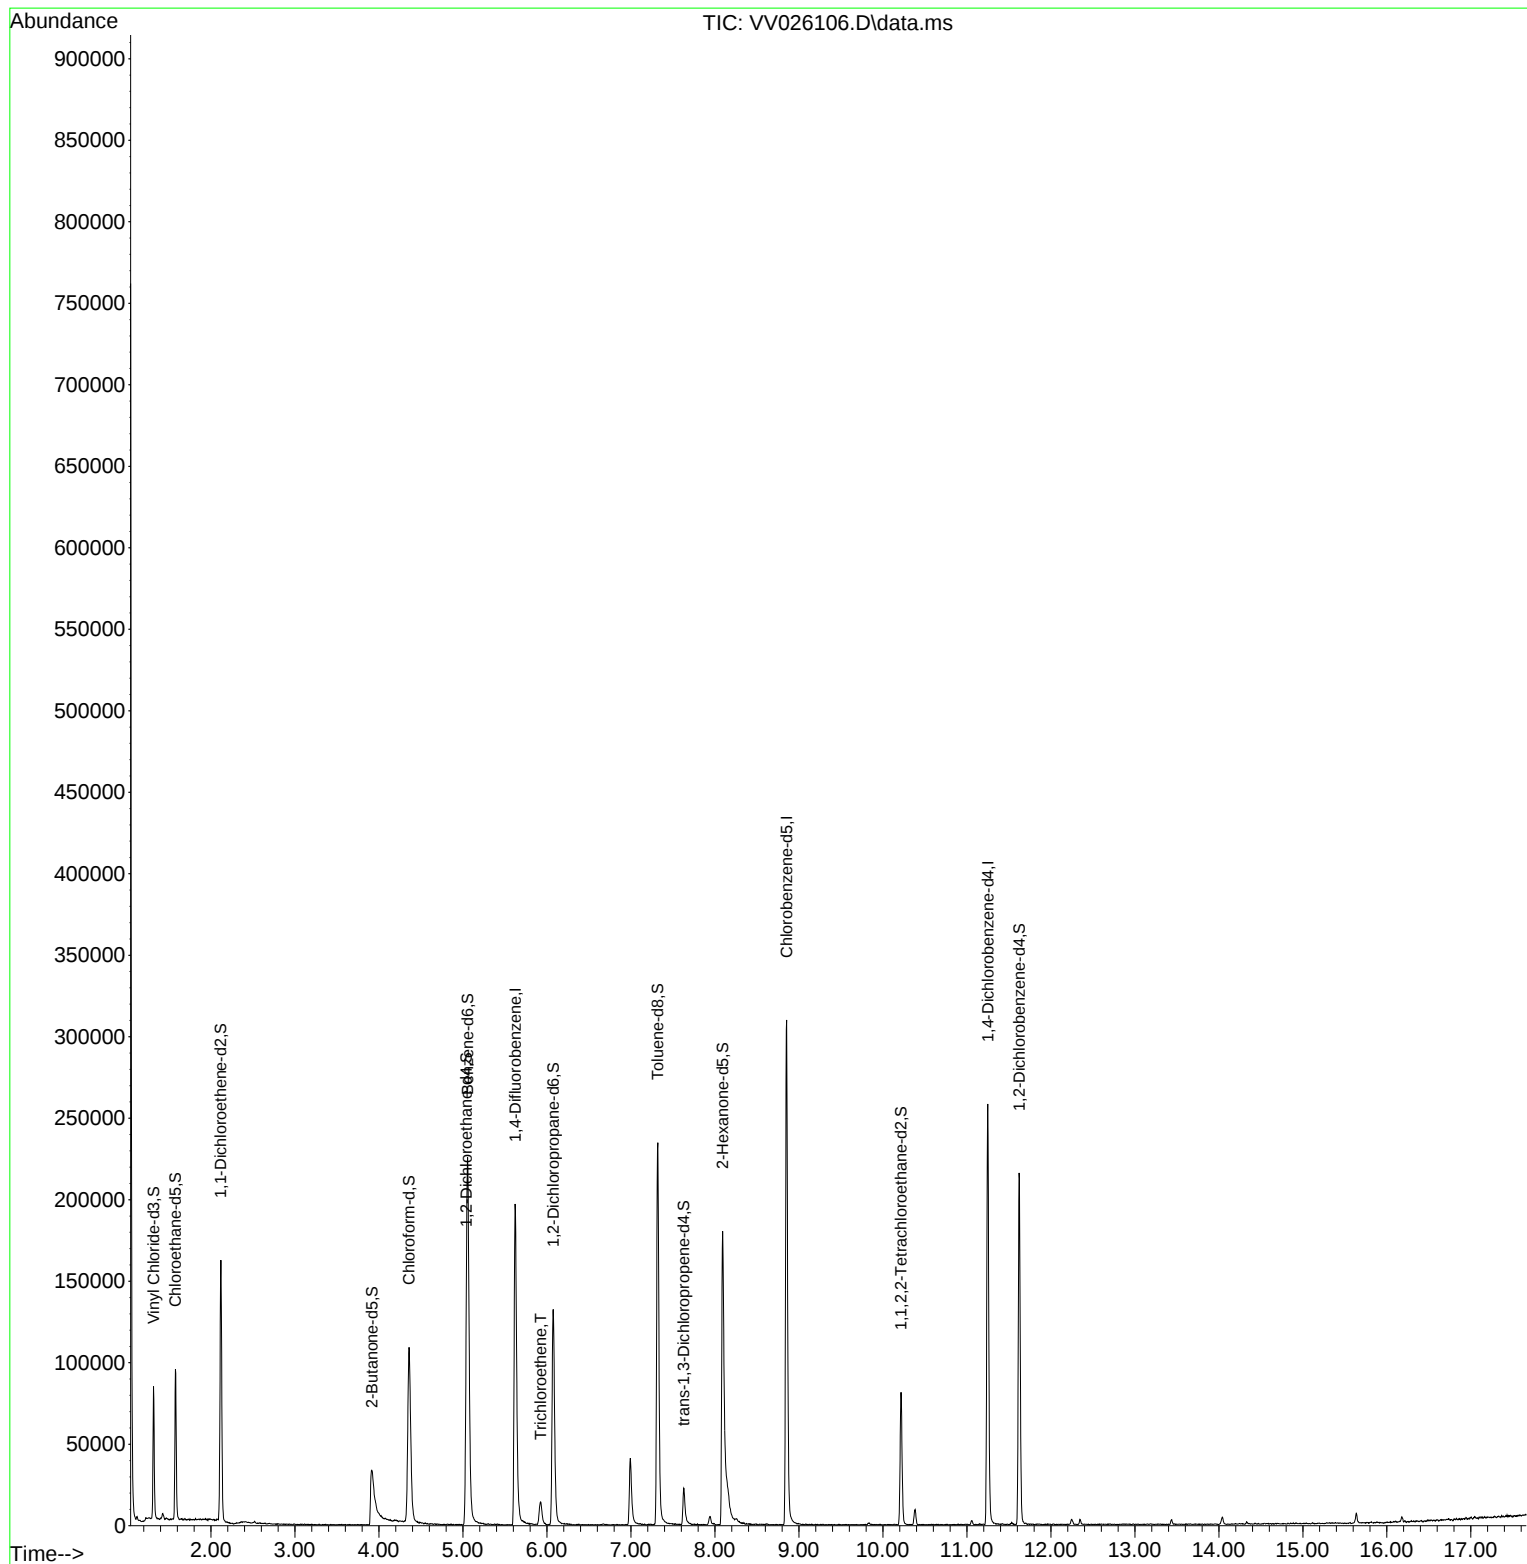

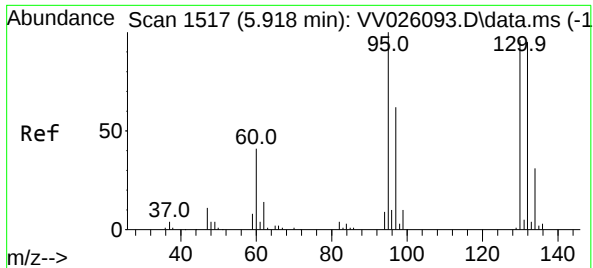

#34
 Trichloroethene
 Concen: 0.278 ug/L
 RT: 5.928 min Scan# 11
 Delta R.T. 0.010 min
 Lab File: VV026106.D
 Acq: 10 Jun 2022 20:29

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B52

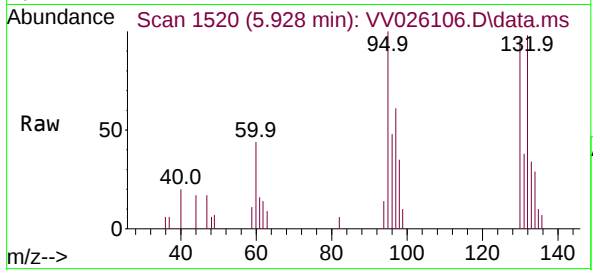

Tgt Ion: 95 Resp: 3974

Ion	Ratio	Lower	Upper
95	100		
97	60.9	44.0	81.6
132	98.0	67.5	125.4
130	96.0	69.7	129.5

