

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW061022\
 Data File : VW026108.D
 Acq On : 10 Jun 2022 21:17
 Operator : SY/MD
 Sample : N3272-16
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B61

Quant Time: Jun 11 01:29:16 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Jun 11 01:25:15 2022
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	5.622	114	155536	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.853	117	153084	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	63616	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.317	65	52109	5.707	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	114.200%	
7) Chloroethane-d5	1.577	69	58611	6.140	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	122.800%	
11) 1,1-Dichloroethene-d2	2.117	63	84753	4.019	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	80.400%	
20) 2-Butanone-d5	3.915	46	79868	59.145	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	118.280%	
24) Chloroform-d	4.359	84	112287	5.803	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	116.000%	
26) 1,2-Dichloroethane-d4	5.040	65	48315	6.121	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	122.400%	
32) Benzene-d6	5.056	84	210672	5.695	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	114.000%	
36) 1,2-Dichloropropane-d6	6.075	67	67567	5.904	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	118.000%	
41) Toluene-d8	7.320	98	163926	5.015	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	100.200%	
43) trans-1,3-Dichloroprop...	7.628	79	14075	4.177	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	83.600%	
46) 2-Hexanone-d5	8.091	63	72533	48.919	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	97.840%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	41451	5.372	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	107.400%	
66) 1,2-Dichlorobenzene-d4	11.622	152	55249	5.677	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	113.600%	
Target Compounds						
					Qvalue	
34) Trichloroethene	5.931	95	3990	0.317	ug/L	90
53) m,p-Xylene	9.146	106	2080	0.102	ug/L	84


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061022\
Data File : VV026108.D
Acq On : 10 Jun 2022 21:17
Operator : SY/MD
Sample : N3272-16
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B61

Quant Time: Jun 11 01:29:16 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Jun 11 01:25:15 2022
Response via : Initial Calibration

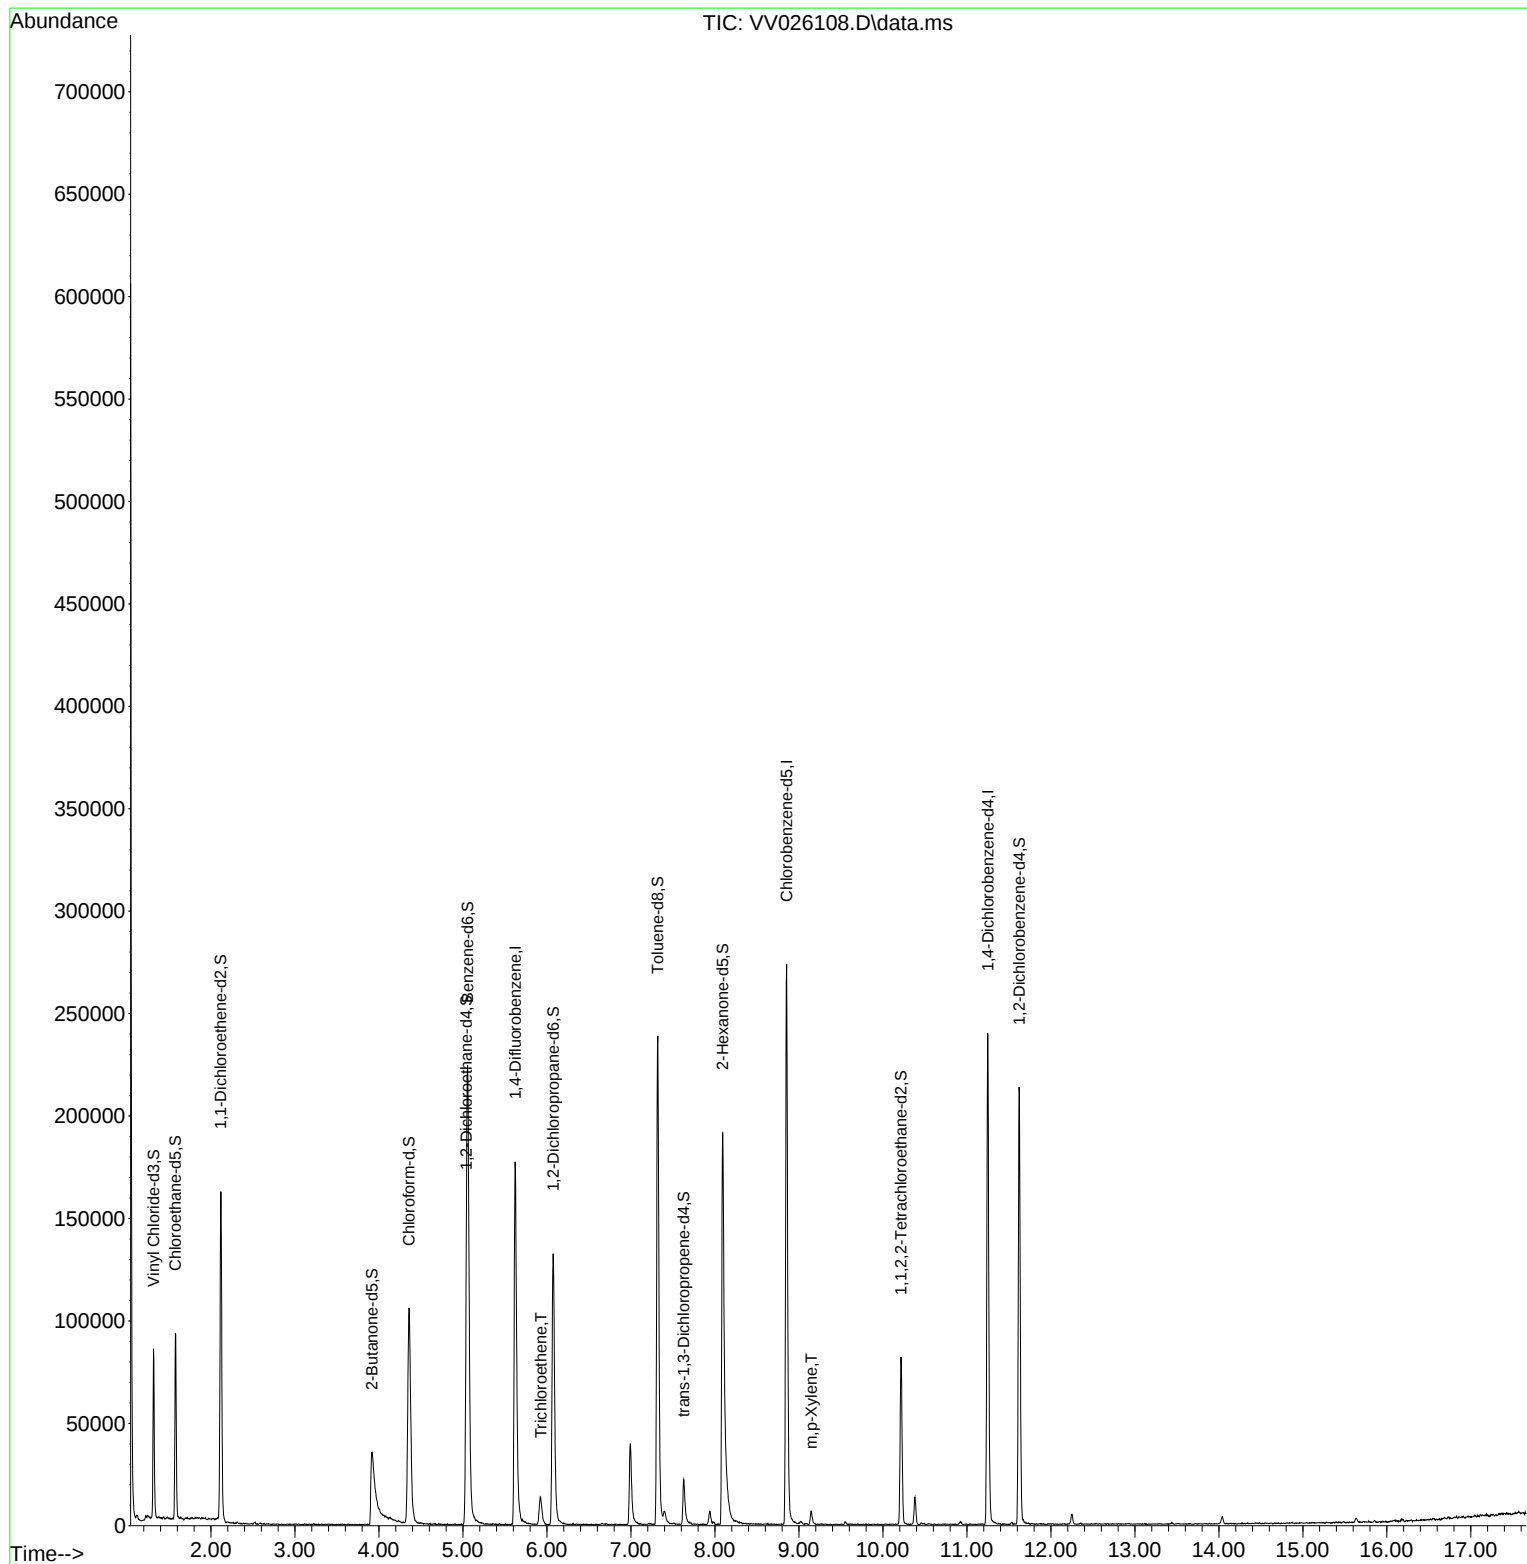




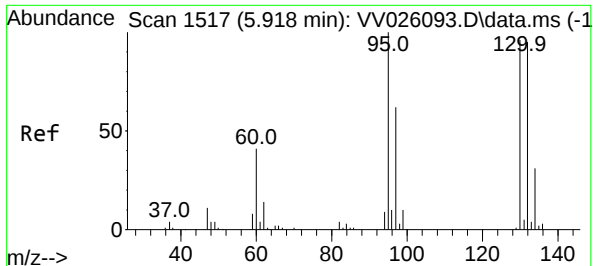


#34
Trichloroethene
Concen: 0.317 ug/L
RT: 5.931 min Scan# 11
Delta R.T. 0.013 min
Lab File: VV026108.D
Acq: 10 Jun 2022 21:17

Instrument :
MSVOA_V
ClientSampleId :
C0B61

Tgt Ion: 95 Resp: 3990

Ion	Ratio	Lower	Upper
95	100		
97	51.6	44.0	81.6
132	85.5	67.5	125.4
130	93.6	69.7	129.5

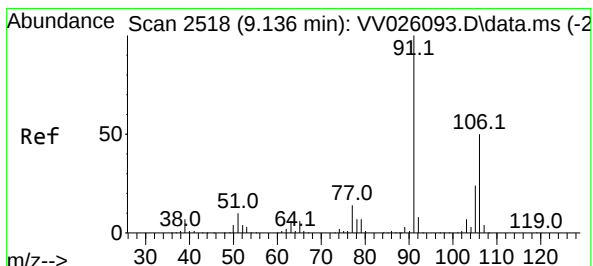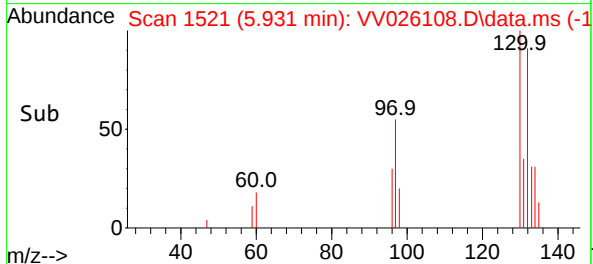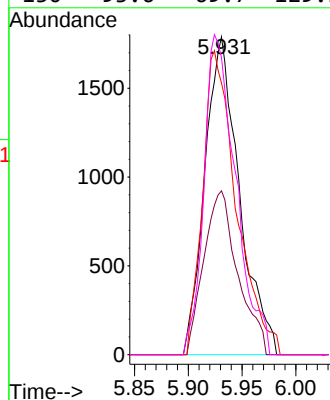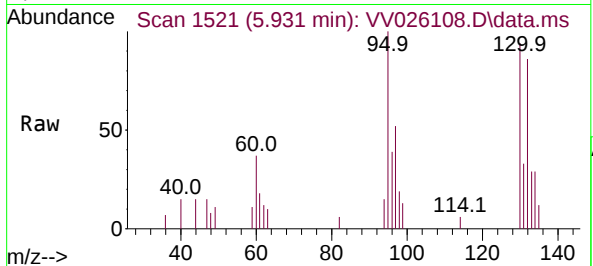

#53
m,p-Xylene
Concen: 0.102 ug/L
RT: 9.146 min Scan# 2521
Delta R.T. 0.010 min
Lab File: VV026108.D
Acq: 10 Jun 2022 21:17

Tgt Ion: 106 Resp: 2080

Ion	Ratio	Lower	Upper
106	100		
91	175.8	140.4	260.8

