

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW061022\
 Data File : VW026109.D
 Acq On : 10 Jun 2022 21:41
 Operator : SY/MD
 Sample : N3272-17
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B62

Quant Time: Jun 11 01:29:29 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Jun 11 01:25:15 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.622	114	160477	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	159212	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	63436	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.317	65	51542	5.471	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	109.400%
7) Chloroethane-d5	1.577	69	58668	5.957	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	119.200%
11) 1,1-Dichloroethene-d2	2.117	63	83904	3.856	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	77.200%
20) 2-Butanone-d5	3.921	46	87698	62.944	ug/L	0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	125.880%
24) Chloroform-d	4.362	84	111858	5.603	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	112.000%
26) 1,2-Dichloroethane-d4	5.040	65	50394	6.188	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	123.800%
32) Benzene-d6	5.056	84	213160	5.541	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	110.800%
36) 1,2-Dichloropropane-d6	6.076	67	68355	5.743	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	114.800%
41) Toluene-d8	7.320	98	162780	4.788	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	95.800%
43) trans-1,3-Dichloroprop...	7.632	79	14645	4.179	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	83.600%
46) 2-Hexanone-d5	8.092	63	72529	47.033	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	94.060%
56) 1,1,2,2-Tetrachloroeth...	10.217	84	42447	5.289	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	105.800%
66) 1,2-Dichlorobenzene-d4	11.625	152	54930	5.660	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	113.200%
Target Compounds						Qvalue
34) Trichloroethene	5.924	95	3679	0.281	ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061022\
Data File : VV026109.D
Acq On : 10 Jun 2022 21:41
Operator : SY/MD
Sample : N3272-17
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B62


Quant Time: Jun 11 01:29:29 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Jun 11 01:25:15 2022
Response via : Initial Calibration

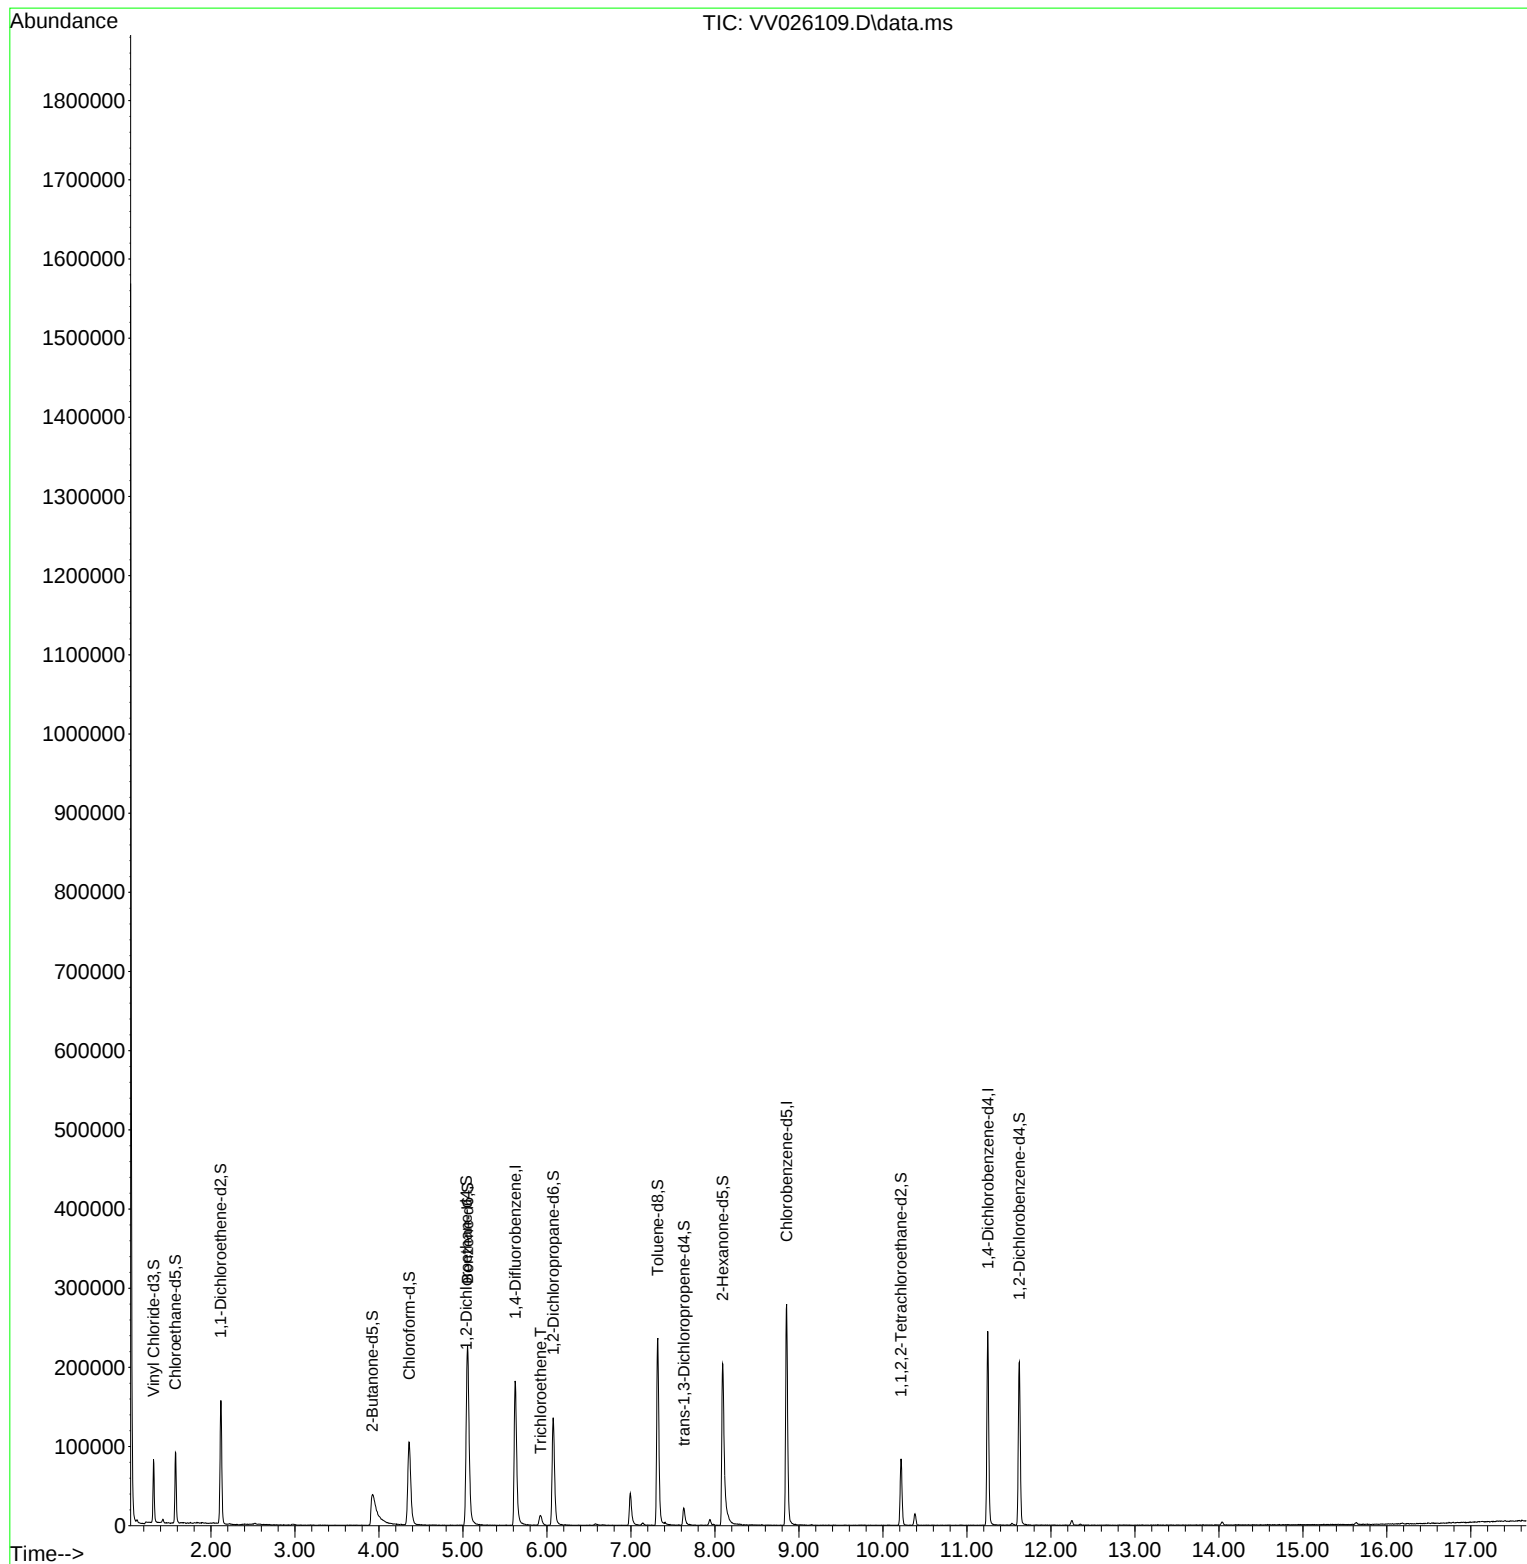

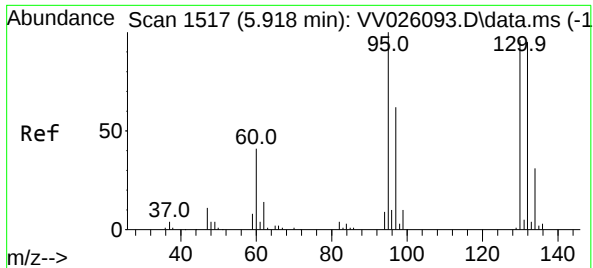

#34
 Trichloroethene
 Concen: 0.281 ug/L
 RT: 5.924 min Scan# 11
 Delta R.T. 0.006 min
 Lab File: VV026109.D
 Acq: 10 Jun 2022 21:41

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B62

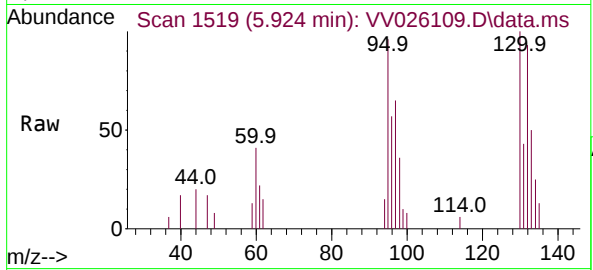

Tgt Ion: 95 Resp: 3679

Ion	Ratio	Lower	Upper
95	100		
97	68.1	44.0	81.6
132	96.3	67.5	125.4
130	104.0	69.7	129.5

