

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061022\
 Data File : VV026110.D
 Acq On : 10 Jun 2022 22:05
 Operator : SY/MD
 Sample : N3272-18
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B63

Quant Time: Jun 11 01:29:43 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Jun 11 01:25:15 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.625	114	158292	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	154931	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	62671	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.320	65	49835	5.363	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	107.200%
7) Chloroethane-d5	1.581	69	56886	5.856	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	117.200%
11) 1,1-Dichloroethene-d2	2.121	63	83947	3.911	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	78.200%
20) 2-Butanone-d5	3.931	46	78781	57.324	ug/L	0.03
Spiked Amount	50.000	Range	40 - 130	Recovery	=	114.640%
24) Chloroform-d	4.362	84	111005	5.637	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	112.800%
26) 1,2-Dichloroethane-d4	5.043	65	48342	6.018	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	120.400%
32) Benzene-d6	5.060	84	205968	5.502	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	110.000%
36) 1,2-Dichloropropane-d6	6.076	67	66462	5.738	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	114.800%
41) Toluene-d8	7.320	98	156402	4.727	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	94.600%
43) trans-1,3-Dichloroprop...	7.632	79	14421	4.229	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	84.600%
46) 2-Hexanone-d5	8.092	63	70996	47.311	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	94.620%
56) 1,1,2,2-Tetrachloroeth...	10.217	84	41246	5.282	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	105.600%
66) 1,2-Dichlorobenzene-d4	11.622	152	53624	5.593	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	111.800%
Target Compounds						
					Qvalue	
34) Trichloroethene	5.928	95	3779	0.297	ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061022\
Data File : VV026110.D
Acq On : 10 Jun 2022 22:05
Operator : SY/MD
Sample : N3272-18
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B63


Quant Time: Jun 11 01:29:43 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Jun 11 01:25:15 2022
Response via : Initial Calibration

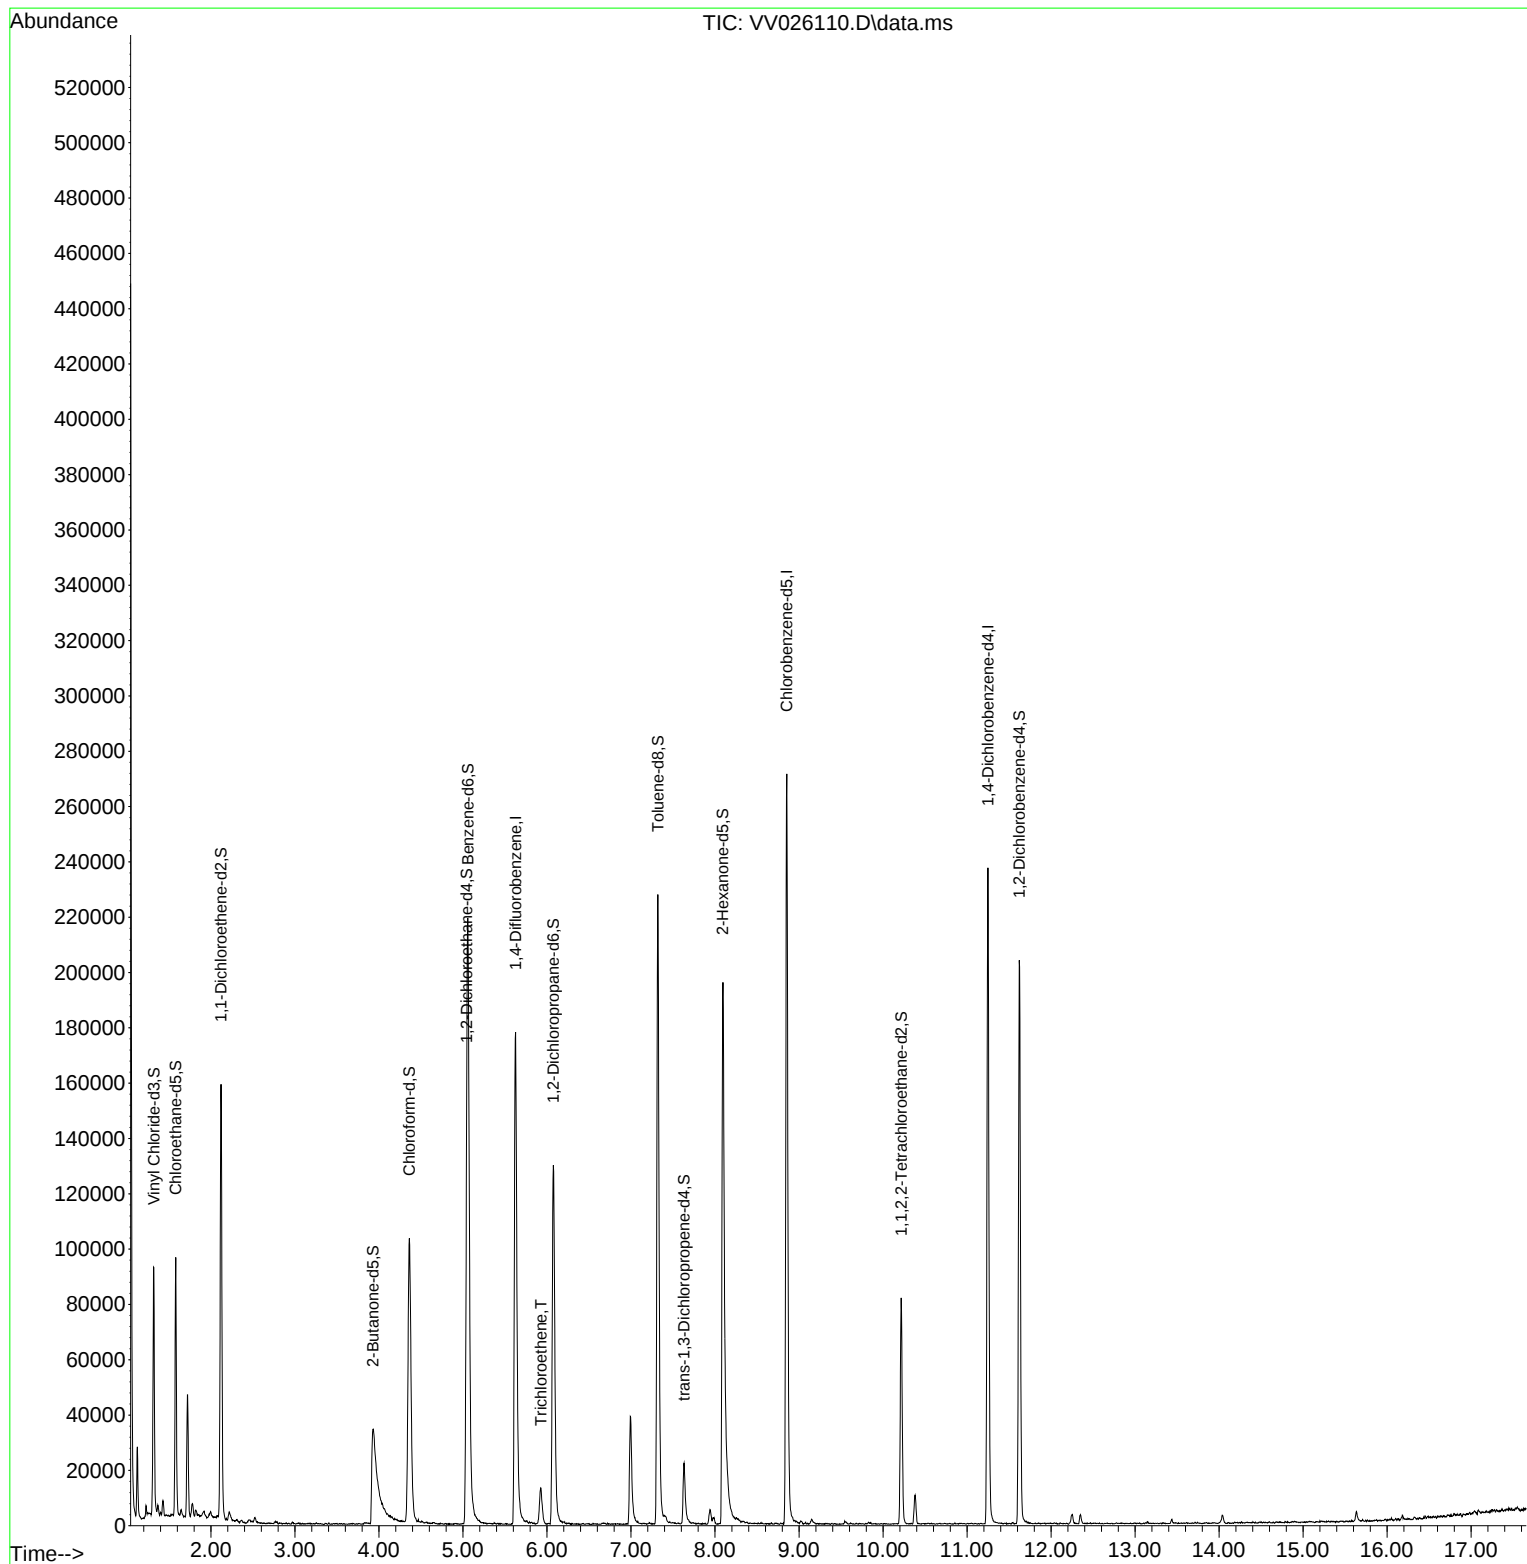

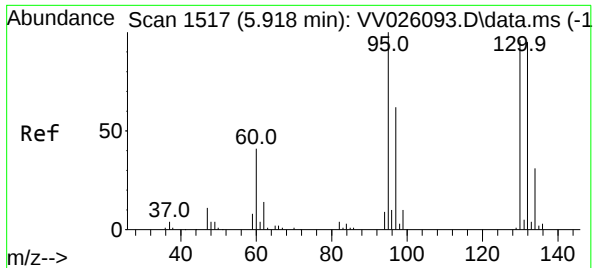

#34
 Trichloroethene
 Concen: 0.297 ug/L
 RT: 5.928 min Scan# 11
 Delta R.T. 0.010 min
 Lab File: VV026110.D
 Acq: 10 Jun 2022 22:05

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B63

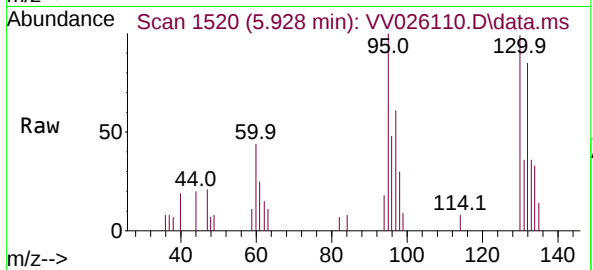

Tgt Ion: 95 Resp: 3779

Ion	Ratio	Lower	Upper
95	100		
97	61.2	44.0	81.6
132	84.7	67.5	125.4
130	98.6	69.7	129.5

