

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\Data\VW061022\  
 Data File : VW026112.D  
 Acq On : 10 Jun 2022 22:53  
 Operator : SY/MD  
 Sample : N3273-01  
 Misc : 25mL/MSVOA\_V/WATER  
 ALS Vial : 21 Sample Multiplier: 1

Instrument :  
 MSVOA\_V  
 ClientSampleId :  
 C0B70

Quant Time: Jun 11 01:30:11 2022  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVTR060822WMA.M  
 Quant Title : TRACE VOA SFAM1.0  
 QLast Update : Sat Jun 11 01:25:15 2022  
 Response via : Initial Calibration


| Compound                      | R.T. QIon |                | Response | Conc        | Units | Dev(Min) |
|-------------------------------|-----------|----------------|----------|-------------|-------|----------|
| Internal Standards            |           |                |          |             |       |          |
| 1) 1,4-Difluorobenzene        | 5.625     | 114            | 161461   | 5.000       | ug/L  | 0.00     |
| 28) Chlorobenzene-d5          | 8.854     | 117            | 158145   | 5.000       | ug/L  | 0.00     |
| 58) 1,4-Dichlorobenzene-d4    | 11.249    | 152            | 64474    | 5.000       | ug/L  | 0.00     |
| System Monitoring Compounds   |           |                |          |             |       |          |
| 4) Vinyl Chloride-d3          | 1.320     | 65             | 50786    | 5.358       | ug/L  | 0.00     |
| Spiked Amount                 | 5.000     | Range 40 - 130 | Recovery | = 107.200%  |       |          |
| 7) Chloroethane-d5            | 1.581     | 69             | 57611    | 5.814       | ug/L  | 0.00     |
| Spiked Amount                 | 5.000     | Range 65 - 130 | Recovery | = 116.200%  |       |          |
| 11) 1,1-Dichloroethene-d2     | 2.121     | 63             | 82545    | 3.770       | ug/L  | 0.00     |
| Spiked Amount                 | 5.000     | Range 60 - 125 | Recovery | = 75.400%   |       |          |
| 20) 2-Butanone-d5             | 3.925     | 46             | 91595    | 65.340      | ug/L  | 0.02     |
| Spiked Amount                 | 50.000    | Range 40 - 130 | Recovery | = 130.680%# |       |          |
| 24) Chloroform-d              | 4.362     | 84             | 110535   | 5.503       | ug/L  | 0.00     |
| Spiked Amount                 | 5.000     | Range 70 - 125 | Recovery | = 110.000%  |       |          |
| 26) 1,2-Dichloroethane-d4     | 5.043     | 65             | 48373    | 5.904       | ug/L  | 0.00     |
| Spiked Amount                 | 5.000     | Range 70 - 130 | Recovery | = 118.000%  |       |          |
| 32) Benzene-d6                | 5.059     | 84             | 206914   | 5.415       | ug/L  | 0.00     |
| Spiked Amount                 | 5.000     | Range 70 - 125 | Recovery | = 108.200%  |       |          |
| 36) 1,2-Dichloropropane-d6    | 6.076     | 67             | 67372    | 5.699       | ug/L  | 0.00     |
| Spiked Amount                 | 5.000     | Range 60 - 140 | Recovery | = 114.000%  |       |          |
| 41) Toluene-d8                | 7.320     | 98             | 159578   | 4.725       | ug/L  | 0.00     |
| Spiked Amount                 | 5.000     | Range 70 - 130 | Recovery | = 94.600%   |       |          |
| 43) trans-1,3-Dichloroprop... | 7.629     | 79             | 13225    | 3.799       | ug/L  | 0.00     |
| Spiked Amount                 | 5.000     | Range 55 - 130 | Recovery | = 76.000%   |       |          |
| 46) 2-Hexanone-d5             | 8.092     | 63             | 68301    | 44.590      | ug/L  | 0.00     |
| Spiked Amount                 | 50.000    | Range 45 - 130 | Recovery | = 89.180%   |       |          |
| 56) 1,1,2,2-Tetrachloroeth... | 10.217    | 84             | 41383    | 5.191       | ug/L  | 0.00     |
| Spiked Amount                 | 5.000     | Range 65 - 120 | Recovery | = 103.800%  |       |          |
| 66) 1,2-Dichlorobenzene-d4    | 11.625    | 152            | 53406    | 5.414       | ug/L  | 0.00     |
| Spiked Amount                 | 5.000     | Range 80 - 120 | Recovery | = 108.200%  |       |          |
| Target Compounds              |           |                |          |             |       | Qvalue   |
| 34) Trichloroethene           | 5.931     | 95             | 2946     | 0.227       | ug/L  | 91       |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\Data\VV061022\  
Data File : VV026112.D  
Acq On : 10 Jun 2022 22:53  
Operator : SY/MD  
Sample : N3273-01  
Misc : 25mL/MSVOA\_V/WATER  
ALS Vial : 21 Sample Multiplier: 1

Instrument :  
MSVOA\_V  
ClientSampleId :  
C0B70

Quant Time: Jun 11 01:30:11 2022  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVTR060822WMA.M  
Quant Title : TRACE VOA SFAM1.0  
QLast Update : Sat Jun 11 01:25:15 2022  
Response via : Initial Calibration

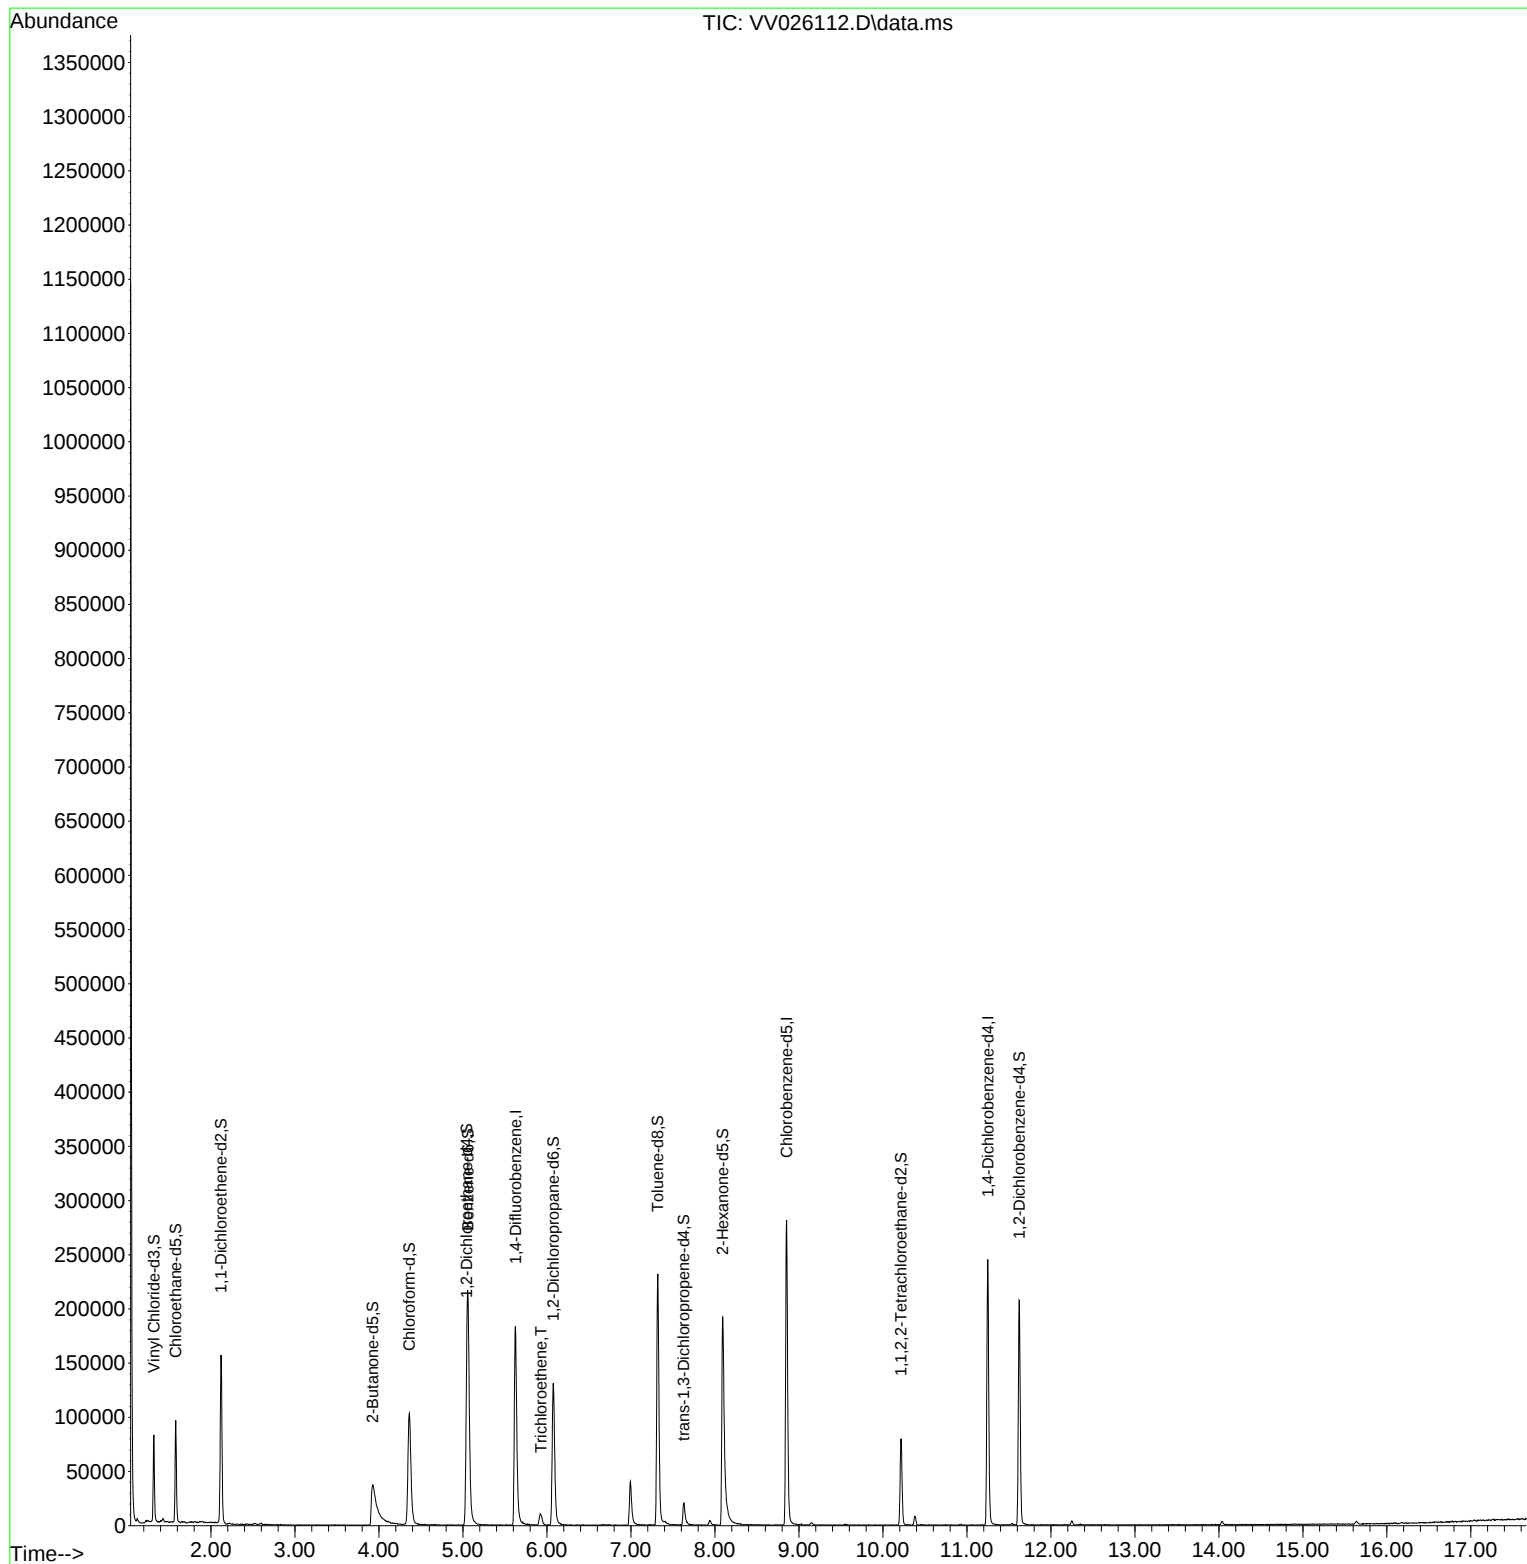

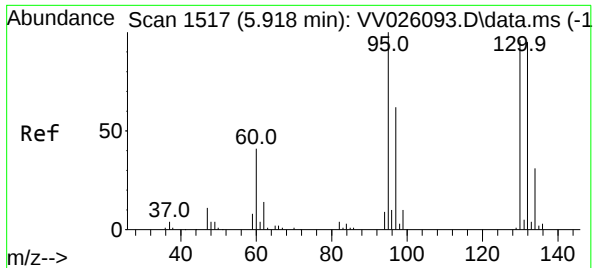

#34  
 Trichloroethene  
 Concen: 0.227 ug/L  
 RT: 5.931 min Scan# 11  
 Delta R.T. 0.013 min  
 Lab File: VV026112.D  
 Acq: 10 Jun 2022 22:53

Instrument :  
 MSVOA\_V  
 ClientSampleId :  
 C0B70

|             |       |       |       |
|-------------|-------|-------|-------|
| Tgt Ion: 95 | Resp: | 2946  |       |
| Ion         | Ratio | Lower | Upper |
| 95          | 100   |       |       |
| 97          | 69.9  | 44.0  | 81.6  |
| 132         | 92.6  | 67.5  | 125.4 |
| 130         | 85.4  | 69.7  | 129.5 |

