

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061022\
 Data File : VV026094.D
 Acq On : 10 Jun 2022 15:36
 Operator : SY/MD
 Sample : VV0610WBL01
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK366

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV026094.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.317	77	86	106	rVB	121390	132460	15.60%	1.943%
2	1.577	160	167	180	rBV	134105	152331	17.94%	2.234%
3	2.117	324	335	352	rVB	243248	351313	41.37%	5.152%
4	2.516	449	459	475	rVB	15509	25786	3.04%	0.378%
5	3.918	881	895	946	rBV3	72965	298523	35.15%	4.378%
6	4.355	1014	1031	1060	rBV	151376	382871	45.08%	5.615%
7	5.050	1229	1247	1276	rBV2	343302	849296	100.00%	12.455%
8	5.619	1411	1424	1455	rBV	289929	598303	70.45%	8.774%
9	5.915	1505	1516	1536	rBV6	21567	52389	6.17%	0.768%
10	6.069	1549	1564	1591	rBV	199838	414771	48.84%	6.083%
11	6.989	1840	1850	1873	rBV	67911	129727	15.27%	1.902%
12	7.317	1937	1952	1976	rBV	381955	668682	78.73%	9.806%
13	7.625	2039	2048	2072	rBV2	39287	74565	8.78%	1.093%
14	8.091	2182	2193	2231	rBV2	304950	638359	75.16%	9.361%
15	8.419	2285	2295	2308	rBV3	16857	29131	3.43%	0.427%
16	8.850	2416	2429	2452	rBV	443651	714440	84.12%	10.477%
17	10.214	2842	2853	2871	rBV	112496	184245	21.69%	2.702%
18	11.246	3162	3174	3196	rBV	384094	601977	70.88%	8.828%
19	11.622	3279	3291	3313	rBV	330352	519829	61.21%	7.623%




Sum of corrected areas: 6818998

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061022\
Data File : VV026094.D
Acq On : 10 Jun 2022 15:36
Operator : SY/MD
Sample : VV0610WBL01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK366

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

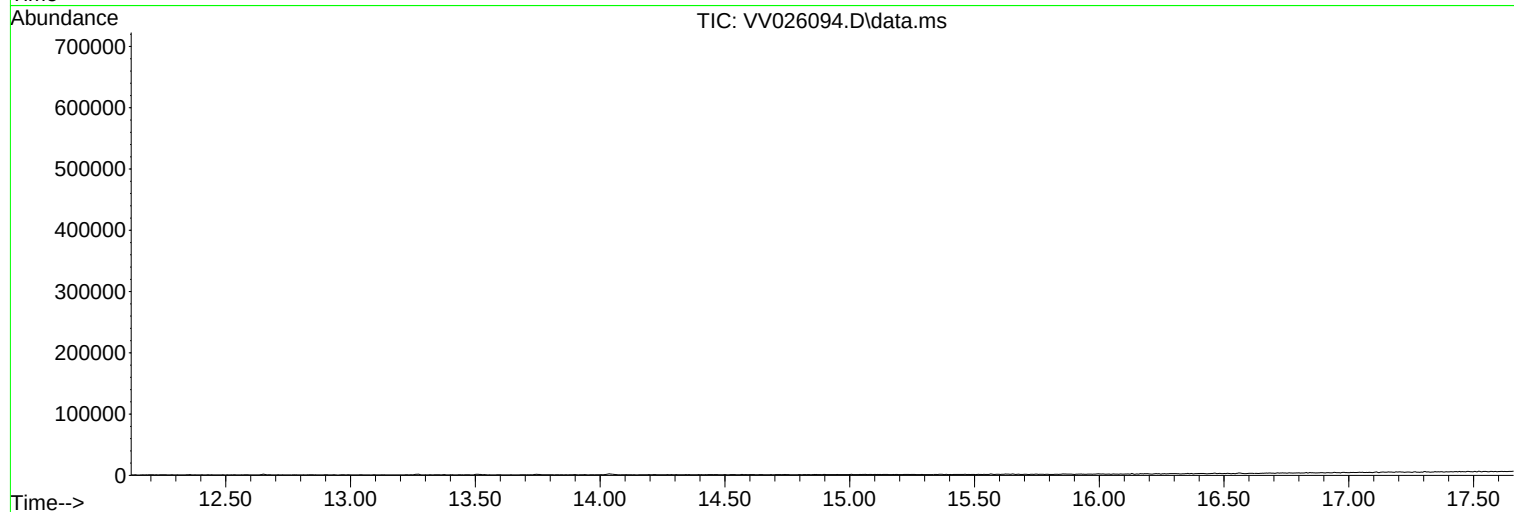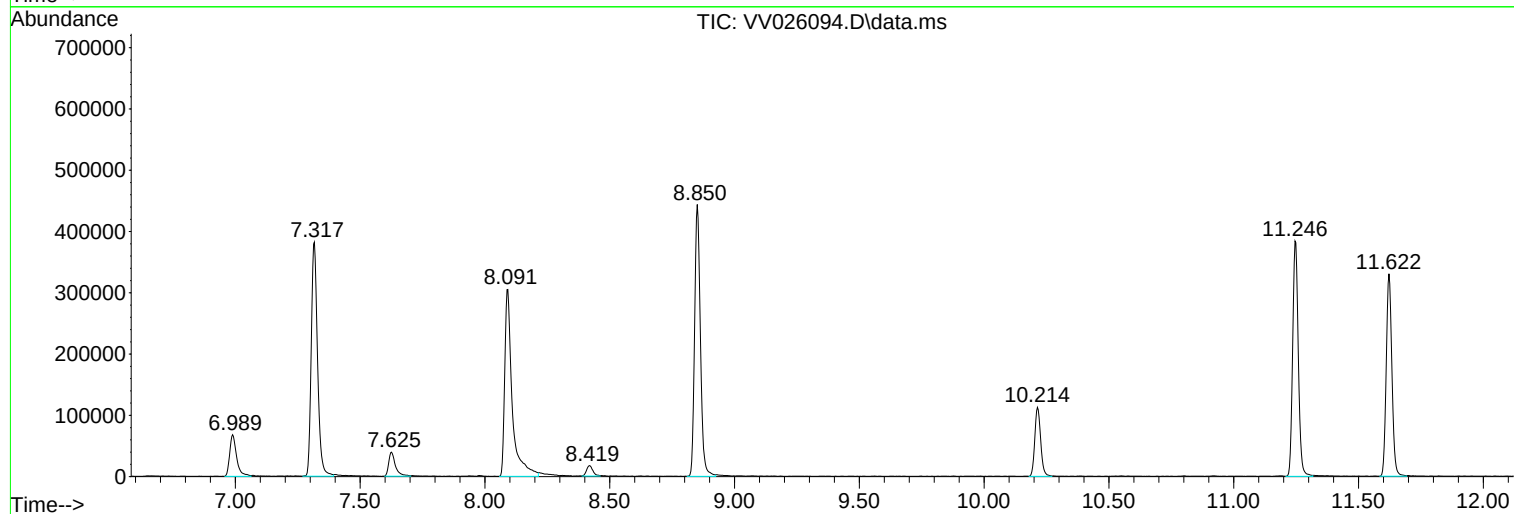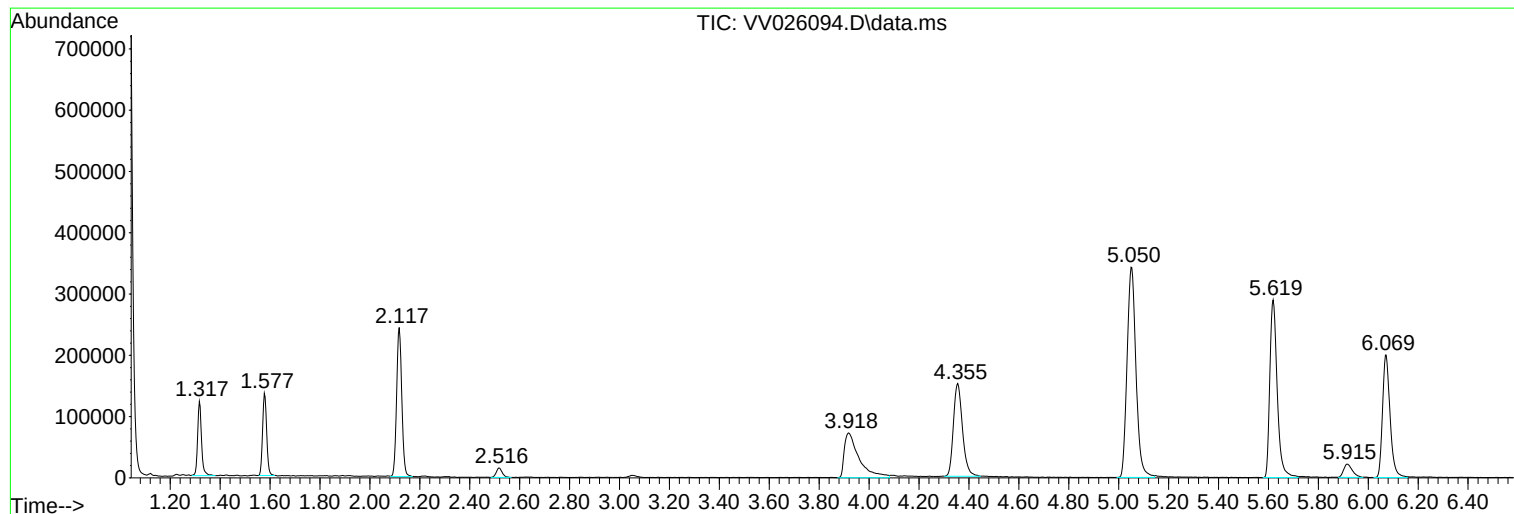

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061022\
Data File : VV026094.D
Acq On : 10 Jun 2022 15:36
Operator : SY/MD
Sample : VV0610WBL01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK366

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061022\
Data File : VV026094.D
Acq On : 10 Jun 2022 15:36
Operator : SY/MD
Sample : VV0610WBL01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK366

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc