

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061022\
 Data File : VV026095.D
 Acq On : 10 Jun 2022 16:06
 Operator : SY/MD
 Sample : N3247-01RE
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXYS3RE

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV026095.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.227	51	58	64	rBV	49756	45060	4.15%	0.605%
2	1.317	76	86	104	rVB	163143	186066	17.15%	2.497%
3	1.577	158	167	182	rBV	177088	199399	18.38%	2.676%
4	2.117	324	335	351	rVB	324097	461598	42.56%	6.194%
5	2.195	351	359	377	rVB3	5025	12725	1.17%	0.171%
6	2.516	450	459	473	rVB3	7964	13969	1.29%	0.187%
7	3.905	875	891	918	rBV	57701	204387	18.84%	2.743%
8	4.355	1015	1031	1067	rVB	196908	500033	46.10%	6.710%
9	5.050	1230	1247	1274	rBV2	440483	1084639	100.00%	14.555%
10	5.619	1412	1424	1452	rBV	196478	405291	37.37%	5.439%
11	5.915	1503	1516	1537	rBV8	23454	59325	5.47%	0.796%
12	6.069	1549	1564	1594	rBV	249274	520305	47.97%	6.982%
13	6.989	1839	1850	1875	rBV	85453	164379	15.16%	2.206%
14	7.317	1940	1952	1971	rBV	506229	889207	81.98%	11.933%
15	7.622	2036	2047	2073	rBV	49499	92361	8.52%	1.239%
16	8.088	2181	2192	2236	rBV2	342798	811538	74.82%	10.890%
17	8.850	2417	2429	2456	rBV	301527	502342	46.31%	6.741%
18	10.214	2842	2853	2874	rBV	133721	220675	20.35%	2.961%
19	10.384	2896	2906	2915	rVB3	7330	11382	1.05%	0.153%
20	11.246	3163	3174	3199	rBV	267903	420078	38.73%	5.637%
21	11.622	3277	3291	3312	rBV	414158	647104	59.66%	8.684%




Sum of corrected areas: 7451863

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061022\
Data File : VV026095.D
Acq On : 10 Jun 2022 16:06
Operator : SY/MD
Sample : N3247-01RE
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXYS3RE

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

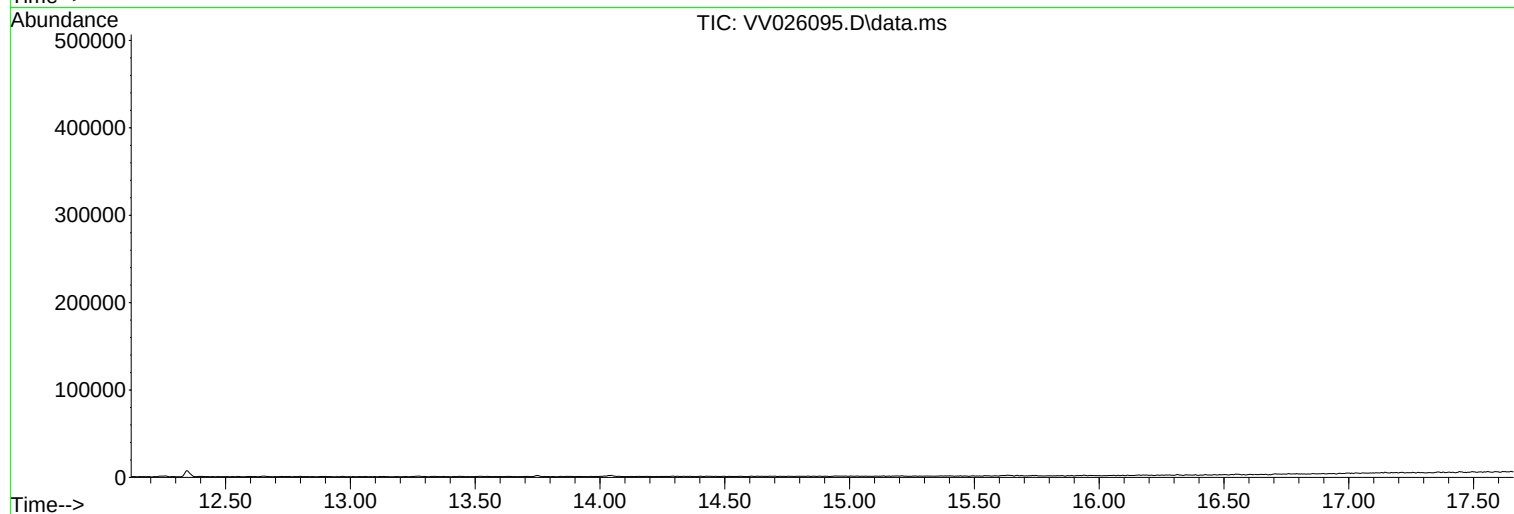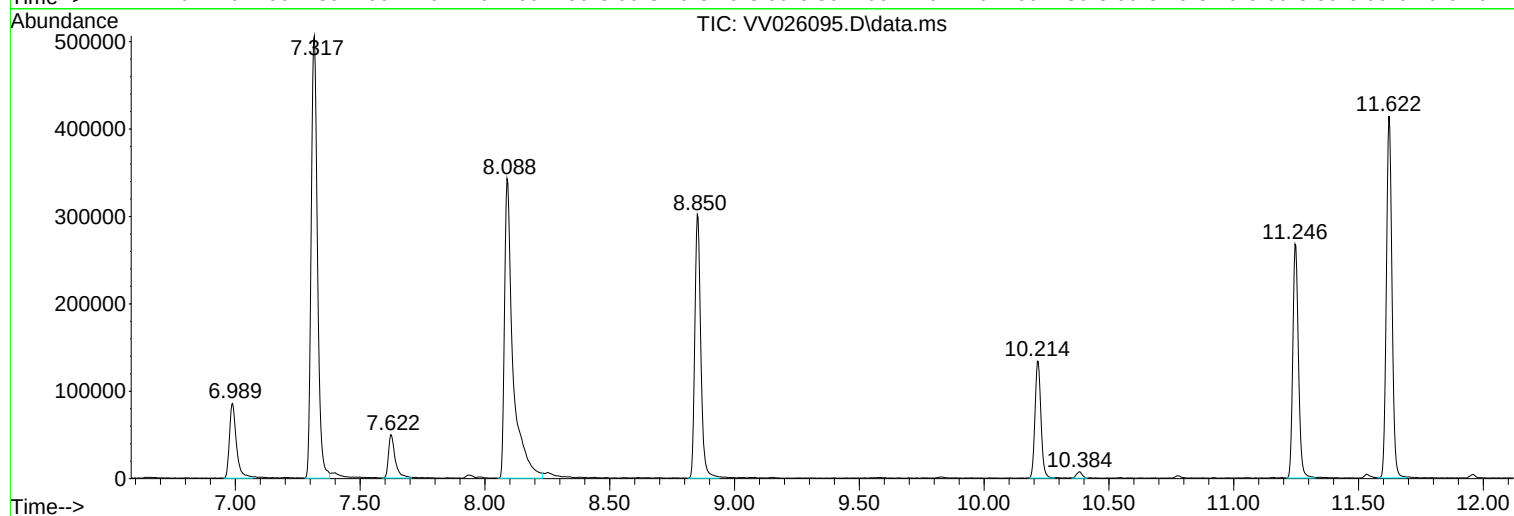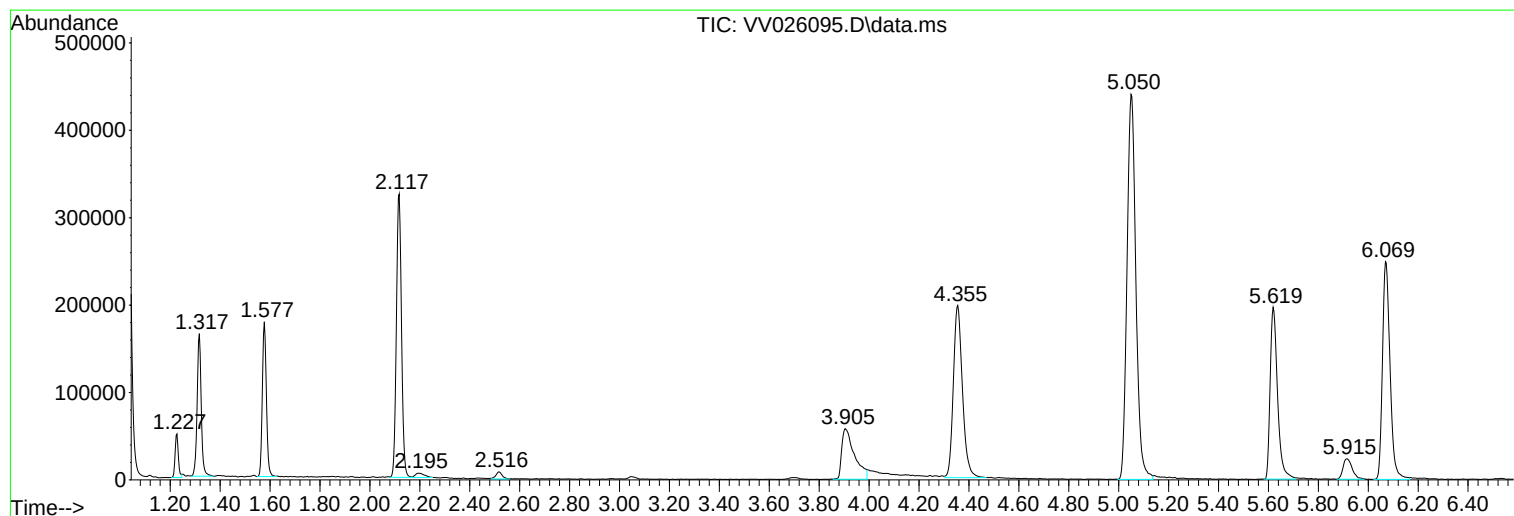

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061022\
Data File : VV026095.D
Acq On : 10 Jun 2022 16:06
Operator : SY/MD
Sample : N3247-01RE
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXYS3RE










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Straight-Chai... Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
1.227	0.56 ug/L	45060	1,4-Difluorobenzene	5.619

Hit#	of 5	Tentative ID	MW	MolForm	CAS#	Qual
1		Isobutane	58	C4H10	000075-28-5	64
2		Isobutane	58	C4H10	000075-28-5	64
3		Isobutane	58	C4H10	000075-28-5	64
4		Isobutane	58	C4H10	000075-28-5	64
5		Isobutane	58	C4H10	000075-28-5	45

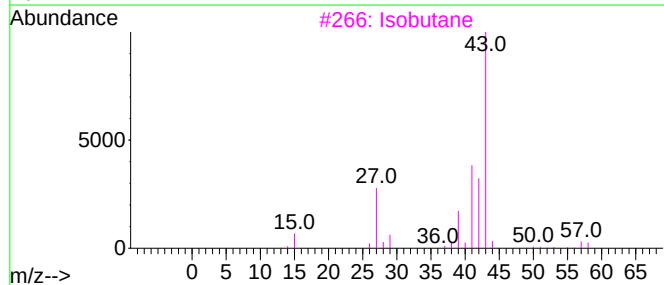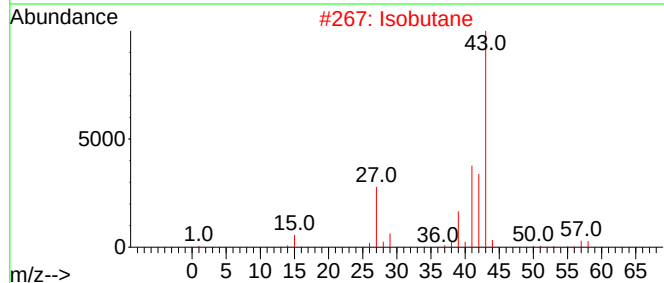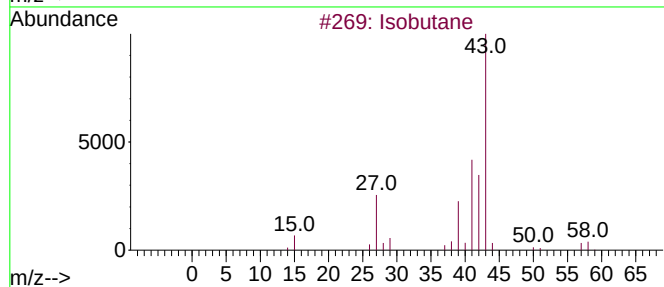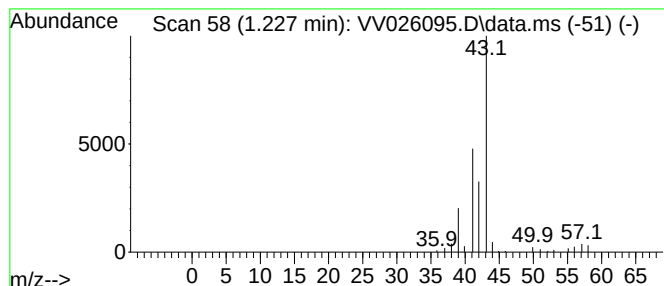

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061022\
Data File : VV026095.D
Acq On : 10 Jun 2022 16:06
Operator : SY/MD
Sample : N3247-01RE
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXYS3RE

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: S...	1.227	0.6	ug/L	45060	1	5.619	405291	5.0