

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061022\
 Data File : VV026096.D
 Acq On : 10 Jun 2022 16:30
 Operator : SY/MD
 Sample : N3247-04DL 5X
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXYW2DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV026096.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.317	77	86	100	rBV	159578	174193	16.42%	2.107%
2	1.581	159	168	169	rBV	177931	176879	16.67%	2.139%
3	2.118	324	335	350	rVB	313444	446087	42.04%	5.395%
4	3.201	656	672	694	rBV	172497	358252	33.76%	4.333%
5	3.912	881	893	918	rBV2	82712	297435	28.03%	3.597%
6	4.359	1015	1032	1055	rBV	188203	466216	43.94%	5.639%
7	4.616	1095	1112	1130	rBV3	88488	221609	20.89%	2.680%
8	5.053	1232	1248	1279	rBV2	432493	1061037	100.00%	12.833%
9	5.622	1414	1425	1450	rBV2	194034	397904	37.50%	4.813%
10	5.918	1505	1517	1537	rBV3	101152	212872	20.06%	2.575%
11	6.072	1552	1565	1599	rBV	248044	519257	48.94%	6.280%
12	6.989	1837	1850	1871	rBV	81581	156778	14.78%	1.896%
13	7.317	1940	1952	1981	rBV	487409	854247	80.51%	10.332%
14	7.625	2037	2048	2073	rBV	48110	96140	9.06%	1.163%
15	7.944	2132	2147	2152	rBV3	9598	17761	1.67%	0.215%
16	7.982	2152	2159	2174	rVB2	12437	21905	2.06%	0.265%
17	8.092	2180	2193	2233	rBV2	358101	813081	76.63%	9.834%
18	8.854	2416	2430	2449	rBV	297100	490494	46.23%	5.933%
19	9.934	2756	2766	2779	rBV	17403	27396	2.58%	0.331%
20	10.217	2841	2854	2872	rBV	141385	228187	21.51%	2.760%
21	10.362	2888	2899	2900	rBV	13981	17863	1.68%	0.216%
22	10.381	2901	2905	2916	rVB2	19189	28794	2.71%	0.348%
23	11.088	3118	3125	3137	rVB2	16191	24824	2.34%	0.300%
24	11.249	3164	3175	3195	rBV	268105	419283	39.52%	5.071%
25	11.538	3253	3265	3279	rVB5	17911	40685	3.83%	0.492%
26	11.622	3279	3291	3318	rBV	415898	684346	64.50%	8.277%
27	12.114	3436	3444	3448	rBV	9957	14329	1.35%	0.173%




Sum of corrected areas: 8267854

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061022\
Data File : VV026096.D
Acq On : 10 Jun 2022 16:30
Operator : SY/MD
Sample : N3247-04DL 5X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXYW2DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

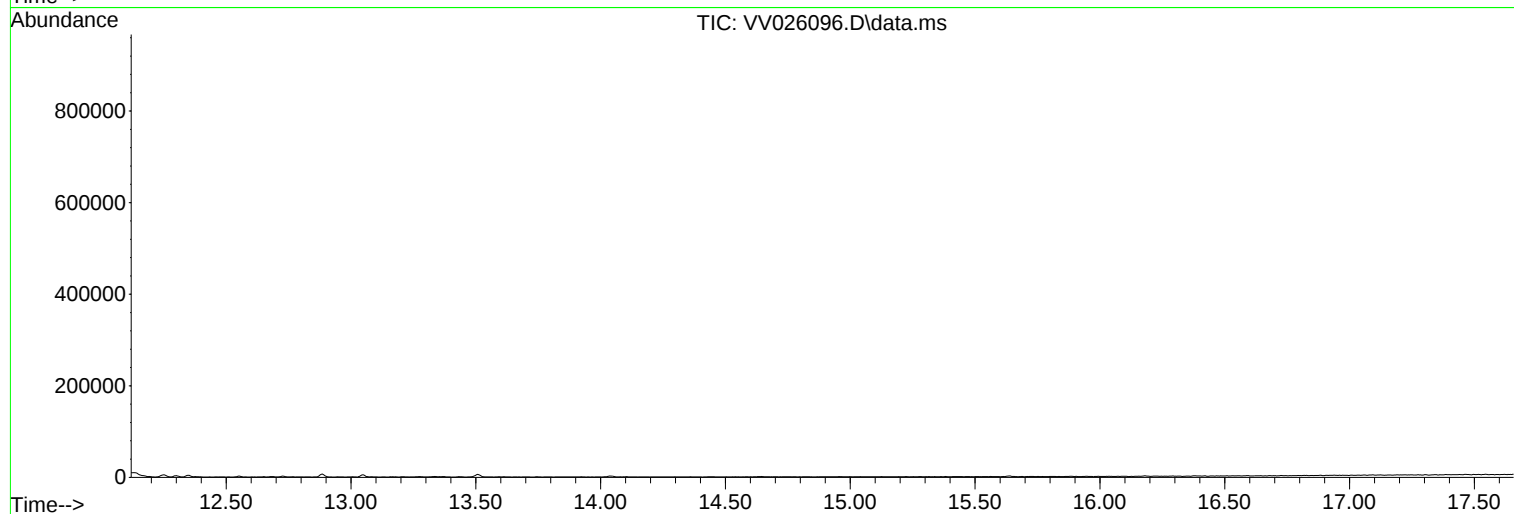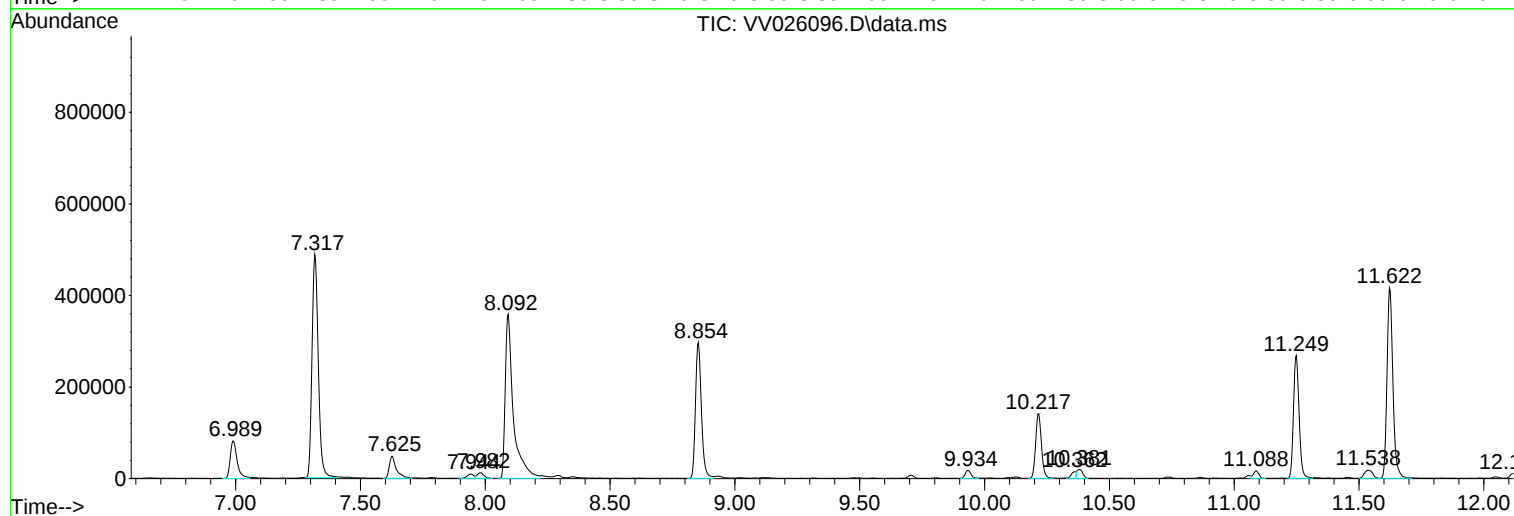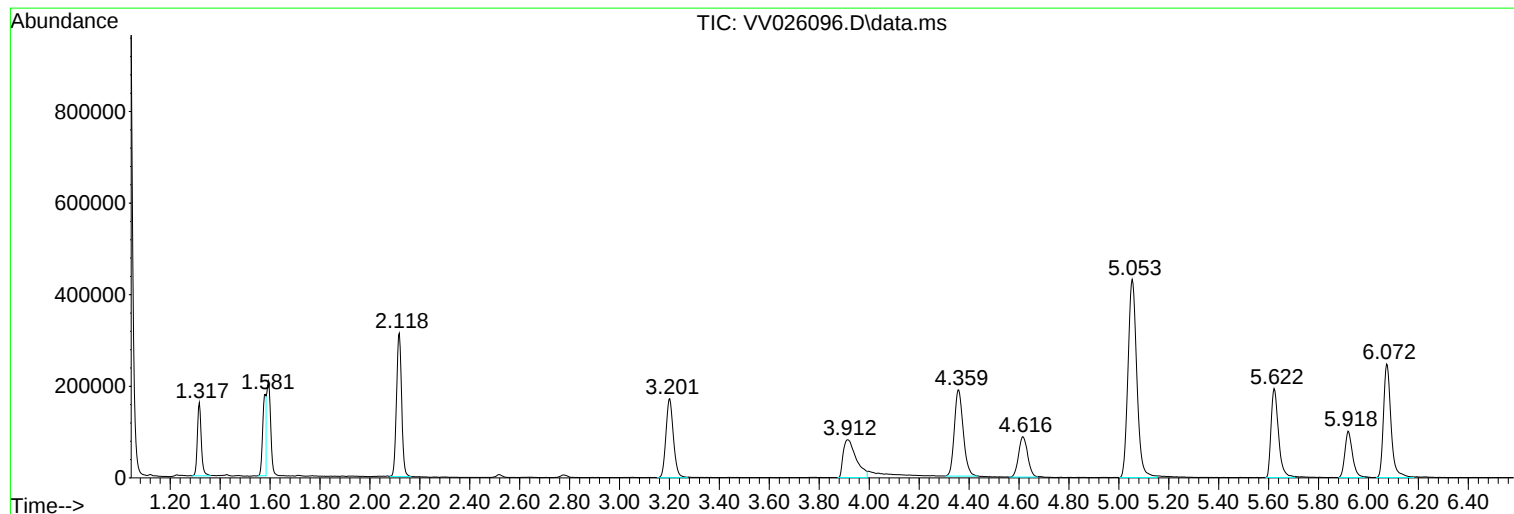

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061022\
Data File : VV026096.D
Acq On : 10 Jun 2022 16:30
Operator : SY/MD
Sample : N3247-04DL 5X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXYW2DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061022\
Data File : VV026096.D
Acq On : 10 Jun 2022 16:30
Operator : SY/MD
Sample : N3247-04DL 5X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXYW2DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc