

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061022\
 Data File : VV026098.D
 Acq On : 10 Jun 2022 17:18
 Operator : SY/MD
 Sample : N3247-12
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXYS4

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV026098.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.224	50	57	64	rBV	46727	42932	6.78%	0.799%
2	1.314	75	85	100	rBV2	96212	125633	19.83%	2.337%
3	1.577	159	167	184	rVB	102602	117988	18.62%	2.195%
4	2.118	323	335	350	rBV	185055	264327	41.71%	4.918%
5	2.195	351	359	374	rVB	6238	15323	2.42%	0.285%
6	3.696	814	826	840	rBV4	2304	6402	1.01%	0.119%
7	3.912	879	893	920	rBV	40560	147011	23.20%	2.735%
8	4.359	1015	1032	1061	rBV	118491	302760	47.78%	5.633%
9	5.053	1233	1248	1276	rBV2	257367	633651	100.00%	11.789%
10	5.622	1413	1425	1455	rBV	229281	473862	74.78%	8.816%
11	5.921	1506	1518	1535	rBV7	18624	43782	6.91%	0.815%
12	6.072	1553	1565	1593	rBV	151692	316943	50.02%	5.897%
13	6.992	1841	1851	1878	rBV2	47961	96489	15.23%	1.795%
14	7.317	1941	1952	1972	rBV	274906	492651	77.75%	9.166%
15	7.629	2040	2049	2069	rBV2	26905	52252	8.25%	0.972%
16	7.940	2132	2146	2158	rBV2	16104	28951	4.57%	0.539%
17	8.092	2182	2193	2237	rBV2	221317	498079	78.60%	9.267%
18	8.256	2239	2244	2256	rVB7	3282	6402	1.01%	0.119%
19	8.854	2418	2430	2456	rBV	351871	580031	91.54%	10.791%
20	10.217	2842	2854	2880	rVB	87570	139682	22.04%	2.599%
21	10.384	2894	2906	2919	rVB	32576	52158	8.23%	0.970%
22	11.249	3163	3175	3197	rBV	304813	479875	75.73%	8.928%
23	11.529	3253	3262	3281	rBV2	19787	35193	5.55%	0.655%
24	11.625	3281	3292	3310	rBV	255066	397173	62.68%	7.389%
25	12.252	3474	3487	3496	rBV2	9463	15940	2.52%	0.297%
26	12.349	3508	3517	3528	rVB6	6317	9491	1.50%	0.177%




Sum of corrected areas: 5374981

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061022\
Data File : VV026098.D
Acq On : 10 Jun 2022 17:18
Operator : SY/MD
Sample : N3247-12
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXYS4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

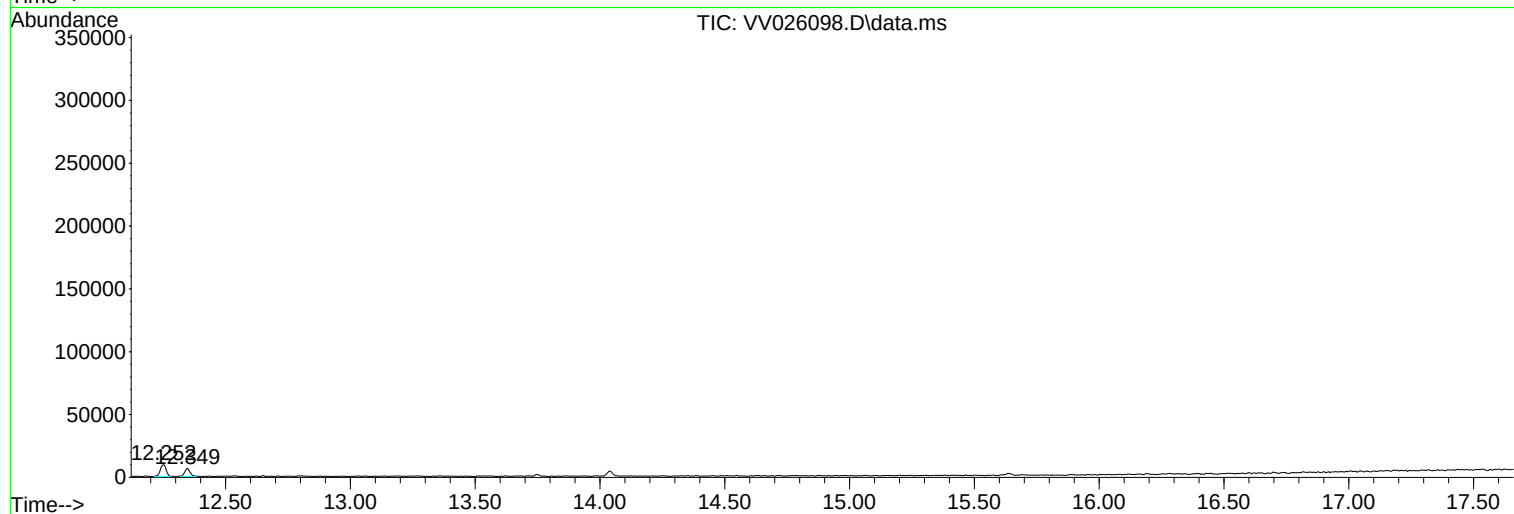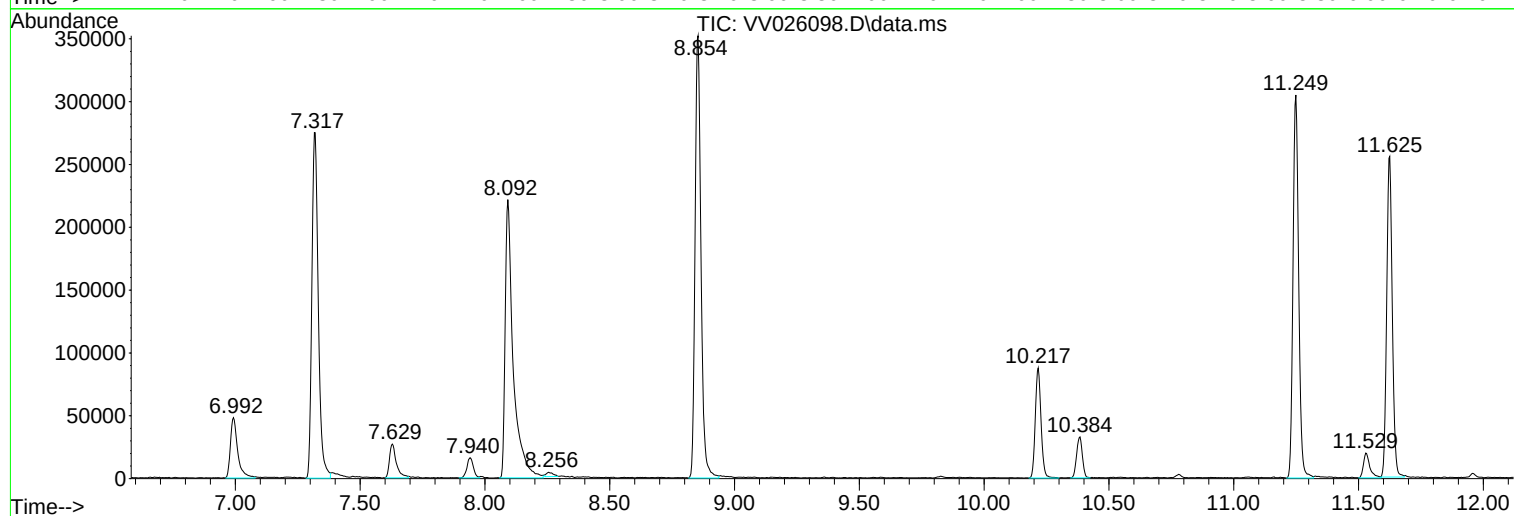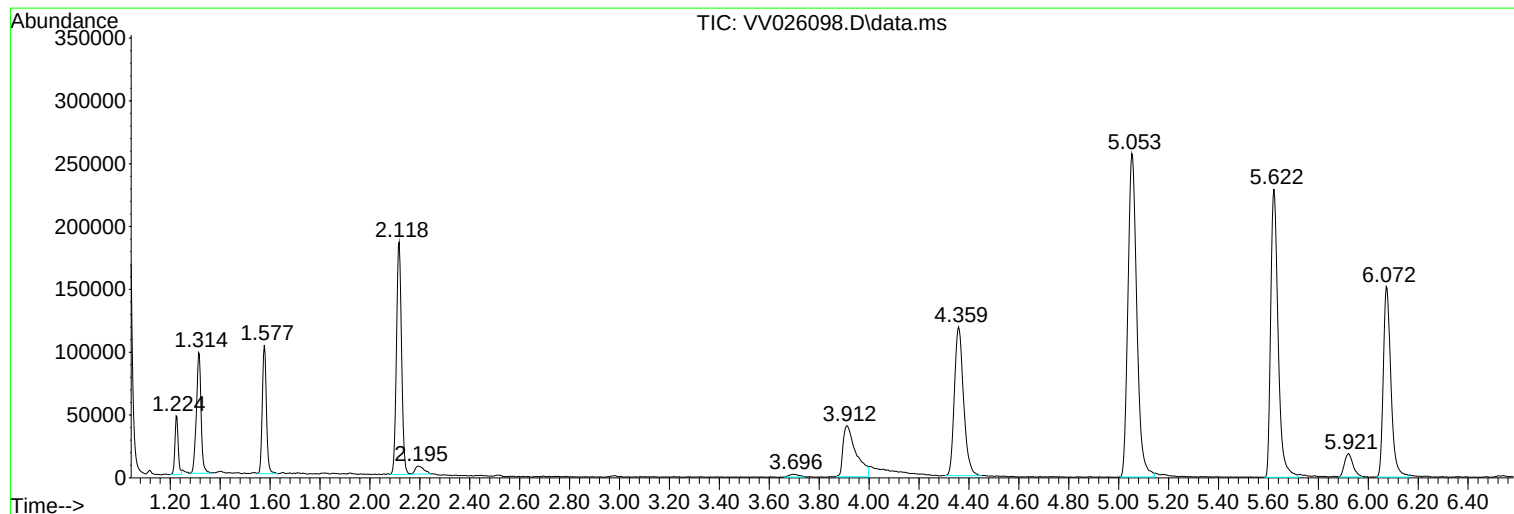

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061022\
Data File : VV026098.D
Acq On : 10 Jun 2022 17:18
Operator : SY/MD
Sample : N3247-12
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXYS4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061022\
Data File : VV026098.D
Acq On : 10 Jun 2022 17:18
Operator : SY/MD
Sample : N3247-12
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXYS4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc