

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061022\
 Data File : VV026099.D
 Acq On : 10 Jun 2022 17:42
 Operator : SY/MD
 Sample : N3247-13
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXYS7

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV026099.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.224	51	57	61	rBV	8373	7618	1.41%	0.169%
2	1.314	77	85	99	rVB	58410	61970	11.44%	1.375%
3	1.574	159	166	178	rBV	69894	79255	14.63%	1.759%
4	2.114	324	334	349	rVB	112207	161334	29.79%	3.580%
5	3.912	880	893	932	rBV2	48637	192921	35.62%	4.281%
6	4.355	1015	1031	1054	rBV2	102018	256410	47.34%	5.690%
7	4.619	1103	1113	1125	rVB7	3972	8504	1.57%	0.189%
8	5.053	1231	1248	1275	rBV2	197015	494581	91.31%	10.974%
9	5.622	1414	1425	1456	rBV	193499	399854	73.82%	8.872%
10	5.921	1506	1518	1537	rVB7	17168	40240	7.43%	0.893%
11	6.076	1548	1566	1593	rBV	126976	270751	49.99%	6.008%
12	6.992	1841	1851	1870	rBV2	43413	82373	15.21%	1.828%
13	7.320	1941	1953	1971	rBV	186508	334679	61.79%	7.426%
14	7.629	2039	2049	2069	rBV2	23712	46960	8.67%	1.042%
15	7.940	2136	2146	2155	rBV2	14326	26969	4.98%	0.598%
16	8.092	2183	2193	2235	rBV2	236582	541630	100.00%	12.018%
17	8.256	2239	2244	2256	rVB6	3671	5702	1.05%	0.127%
18	8.854	2418	2430	2451	rBV	289327	481566	88.91%	10.686%
19	10.217	2842	2854	2873	rBV	92162	148688	27.45%	3.299%
20	10.381	2894	2905	2918	rVB2	40582	65323	12.06%	1.449%
21	11.249	3164	3175	3196	rBV	268426	406059	74.97%	9.010%
22	11.622	3280	3291	3316	rBV	216827	346336	63.94%	7.685%
23	12.249	3474	3486	3497	rBV	16340	25346	4.68%	0.562%
24	12.345	3509	3516	3528	rVB6	9208	13512	2.49%	0.300%
25	14.040	4031	4043	4053	rBV	4609	8091	1.49%	0.180%




Sum of corrected areas: 4506672

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061022\
Data File : VV026099.D
Acq On : 10 Jun 2022 17:42
Operator : SY/MD
Sample : N3247-13
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXYS7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

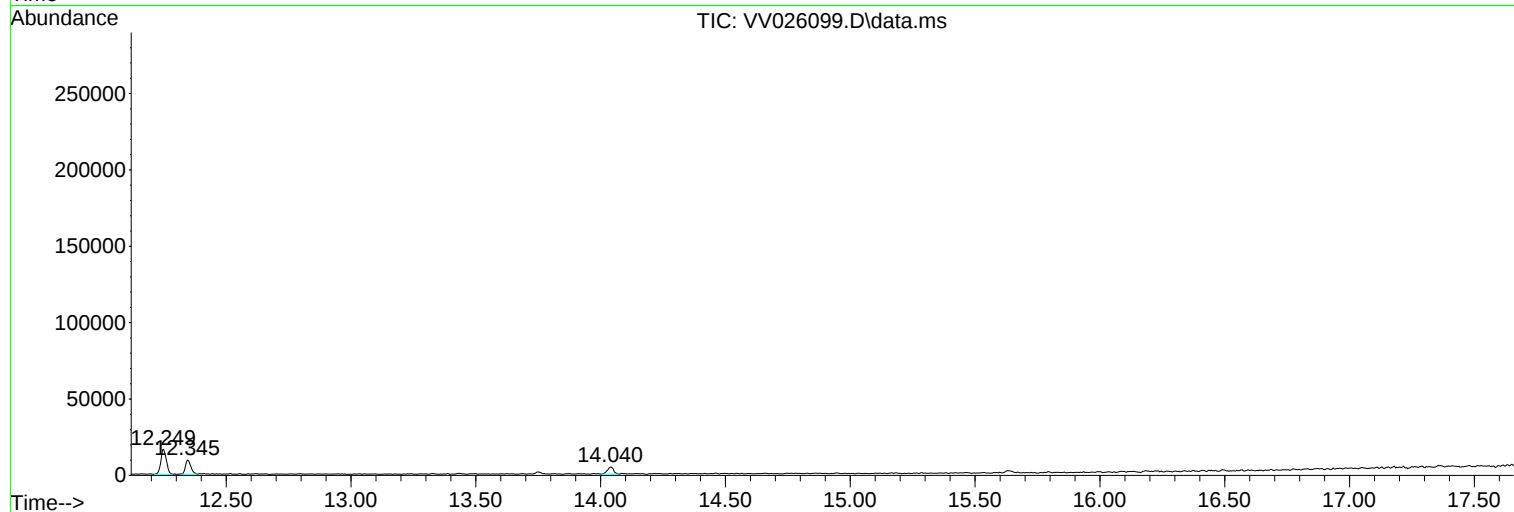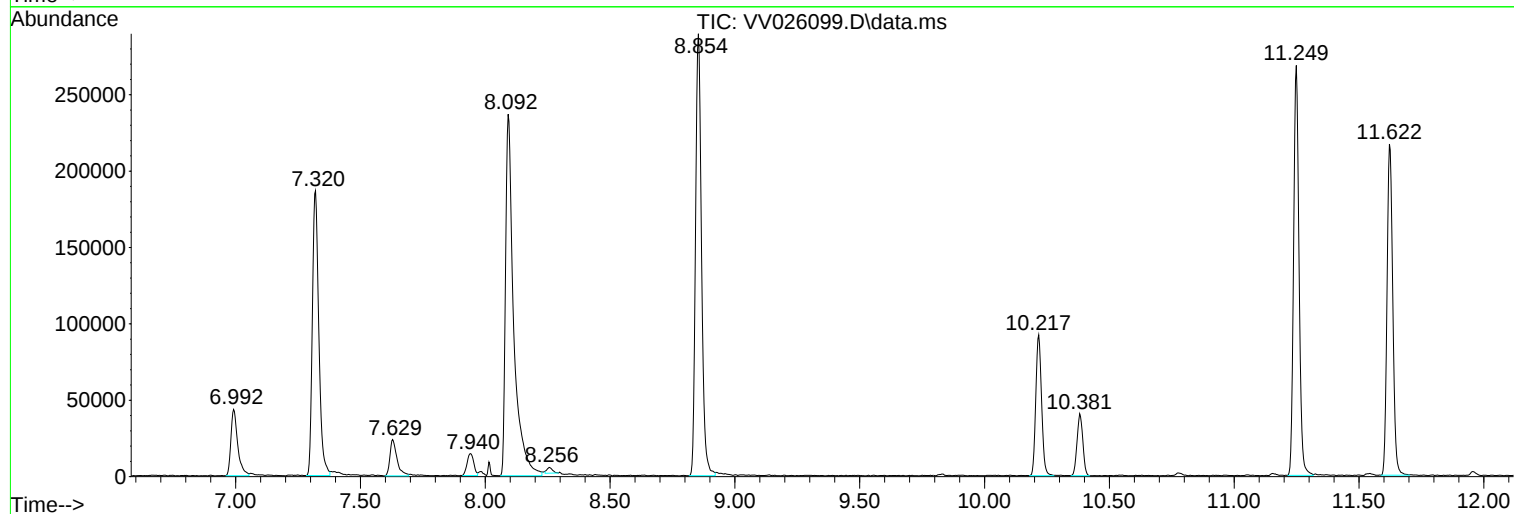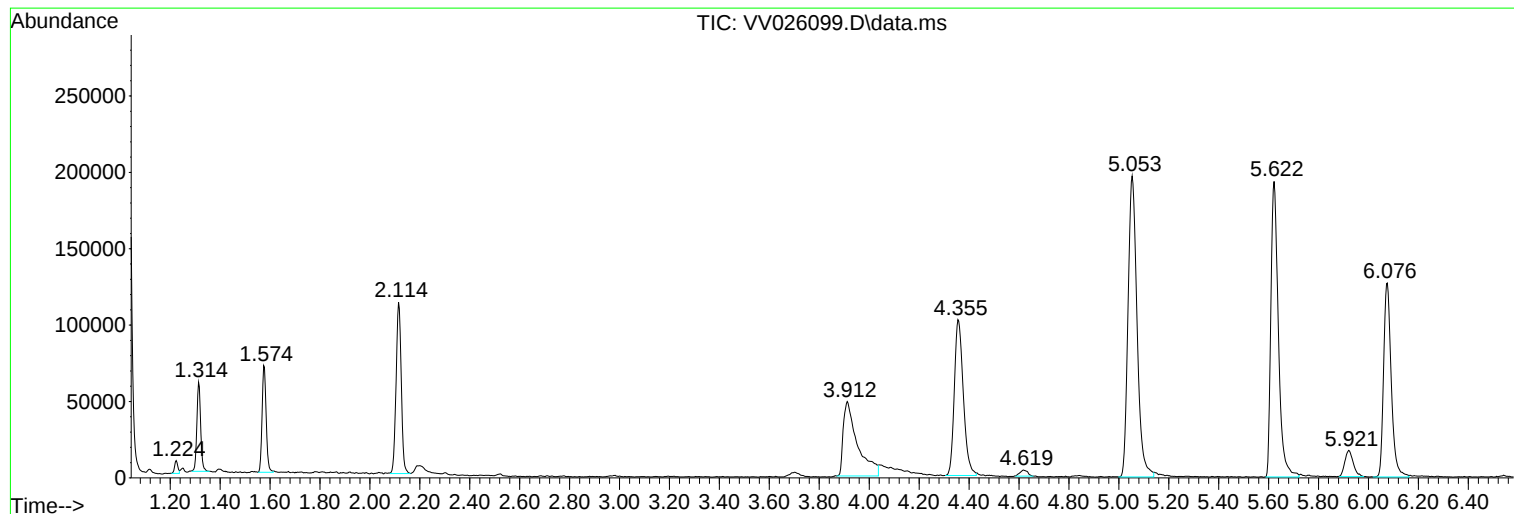

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061022\
Data File : VV026099.D
Acq On : 10 Jun 2022 17:42
Operator : SY/MD
Sample : N3247-13
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXYS7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061022\
Data File : VV026099.D
Acq On : 10 Jun 2022 17:42
Operator : SY/MD
Sample : N3247-13
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXYS7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc