

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061022\
 Data File : VV026100.D
 Acq On : 10 Jun 2022 18:06
 Operator : SY/MD
 Sample : N3247-14
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXYS8

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV026100.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.317	77	86	98	rVB	63300	71053	11.58%	1.437%
2	1.577	159	167	176	rBV	77587	87626	14.28%	1.773%
3	2.118	324	335	352	rVB	127327	184162	30.01%	3.725%
4	3.204	659	673	688	rBV2	11449	23707	3.86%	0.480%
5	3.915	883	894	926	rBV2	64423	236046	38.47%	4.775%
6	4.359	1016	1032	1061	rVB	112137	288833	47.07%	5.843%
7	5.053	1233	1248	1274	rBV2	218247	544709	88.77%	11.019%
8	5.622	1413	1425	1454	rBV	206507	422711	68.89%	8.551%
9	5.921	1506	1518	1538	rBV8	28740	66208	10.79%	1.339%
10	6.076	1552	1566	1588	rBV	142482	298616	48.66%	6.041%
11	6.992	1840	1851	1874	rBV2	47795	93998	15.32%	1.902%
12	7.320	1942	1953	1973	rBV	209188	371859	60.60%	7.522%
13	7.629	2039	2049	2072	rBV2	27467	52103	8.49%	1.054%
14	7.944	2131	2147	2152	rBV3	12584	21865	3.56%	0.442%
15	7.979	2152	2158	2172	rVB2	13715	23977	3.91%	0.485%
16	8.092	2178	2193	2236	rBV2	263991	613630	100.00%	12.413%
17	8.854	2419	2430	2455	rBV	313370	521542	84.99%	10.550%
18	10.217	2842	2854	2871	rBV	102798	165366	26.95%	3.345%
19	10.381	2894	2905	2921	rBV2	30148	46888	7.64%	0.949%
20	11.249	3163	3175	3192	rBV	274281	424635	69.20%	8.590%
21	11.622	3279	3291	3313	rBV	240921	383803	62.55%	7.764%




Sum of corrected areas: 4943337

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061022\
Data File : VV026100.D
Acq On : 10 Jun 2022 18:06
Operator : SY/MD
Sample : N3247-14
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXYS8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

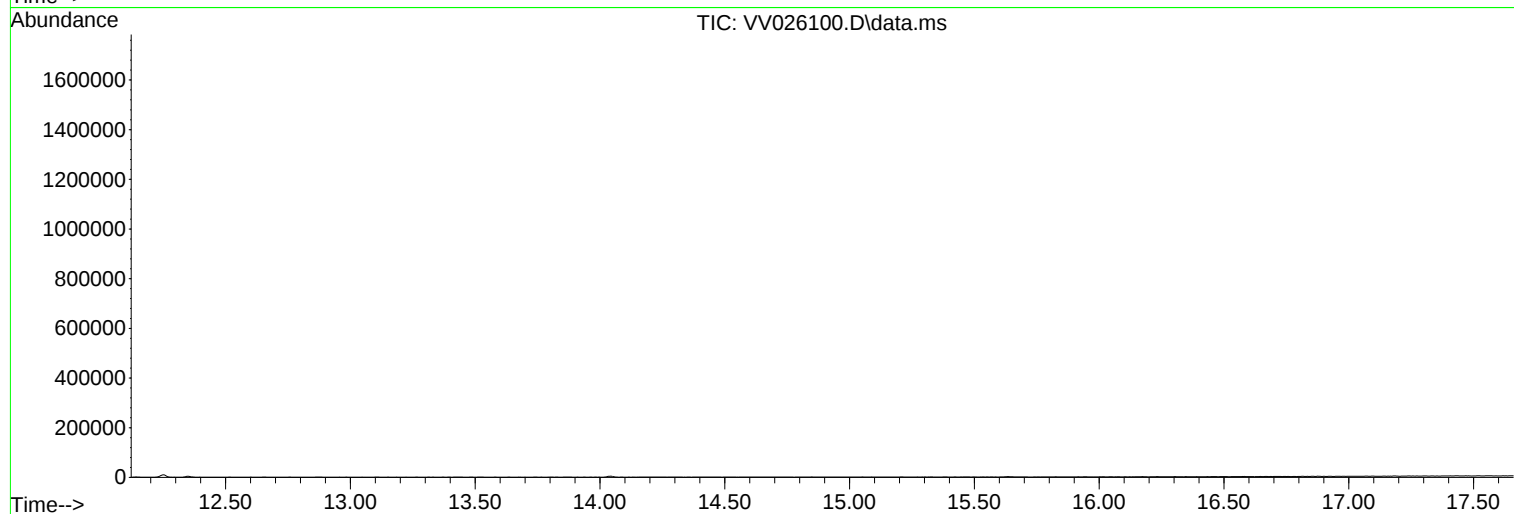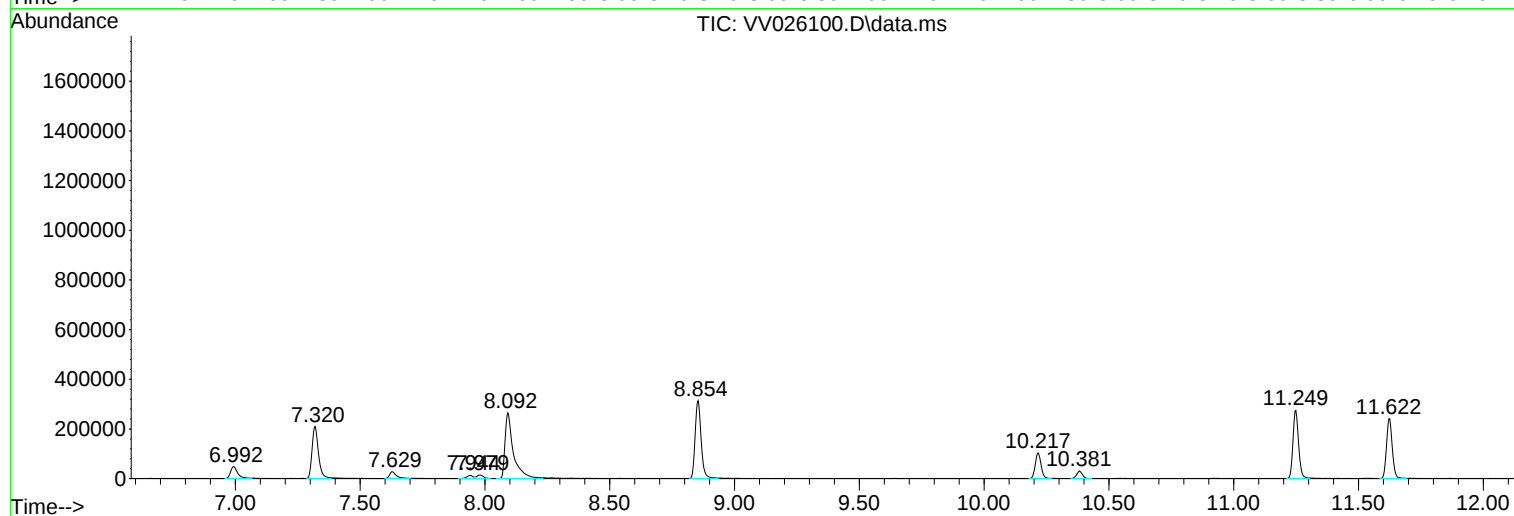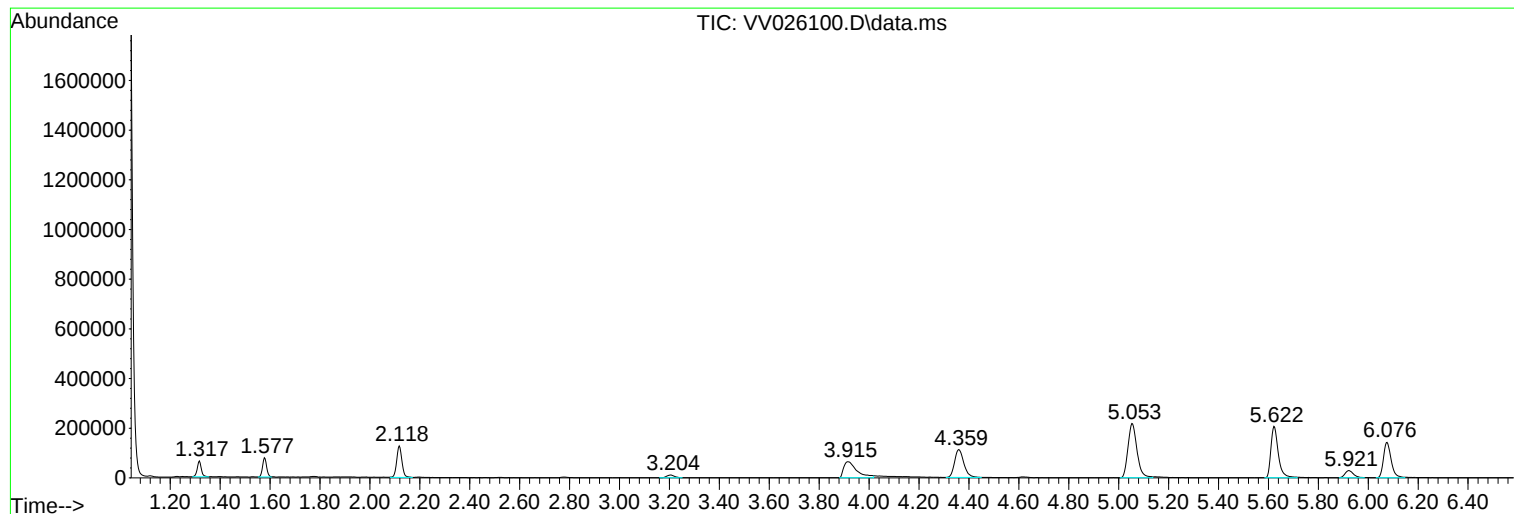

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061022\
Data File : VV026100.D
Acq On : 10 Jun 2022 18:06
Operator : SY/MD
Sample : N3247-14
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXYS8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061022\
Data File : VV026100.D
Acq On : 10 Jun 2022 18:06
Operator : SY/MD
Sample : N3247-14
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXYS8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
